
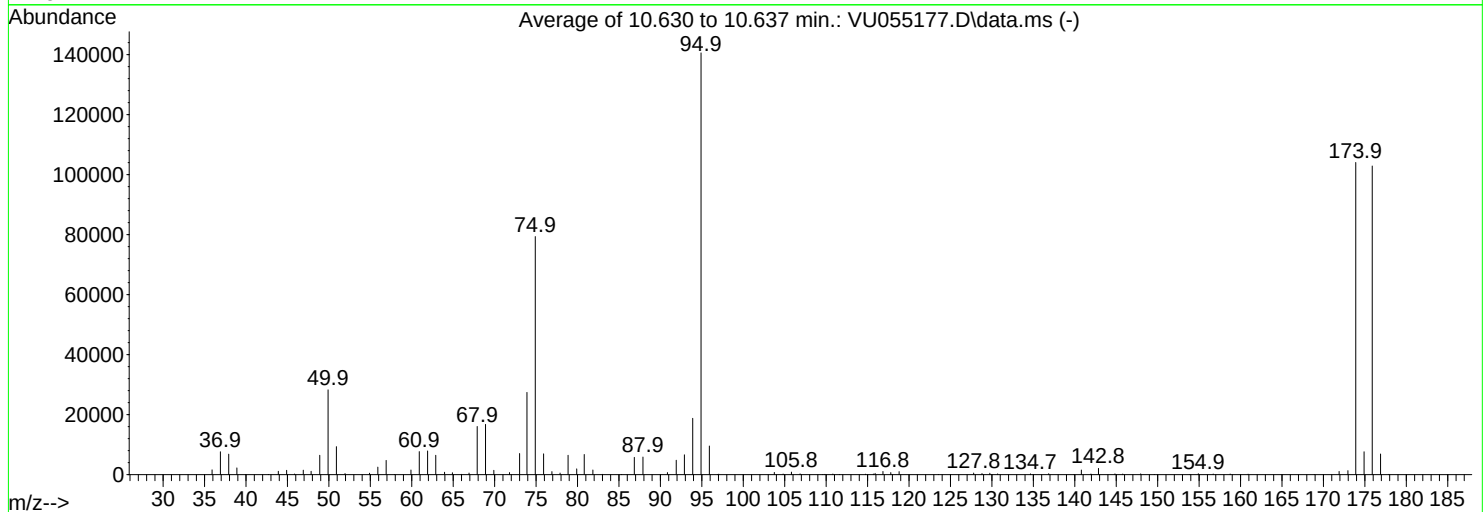


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090723\
Data File : VU055177.D
Acq On : 07 Sep 2023 09:17
Operator : MD/SY
Sample : BFB041
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB041

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Sep 14 05:00:29 2023

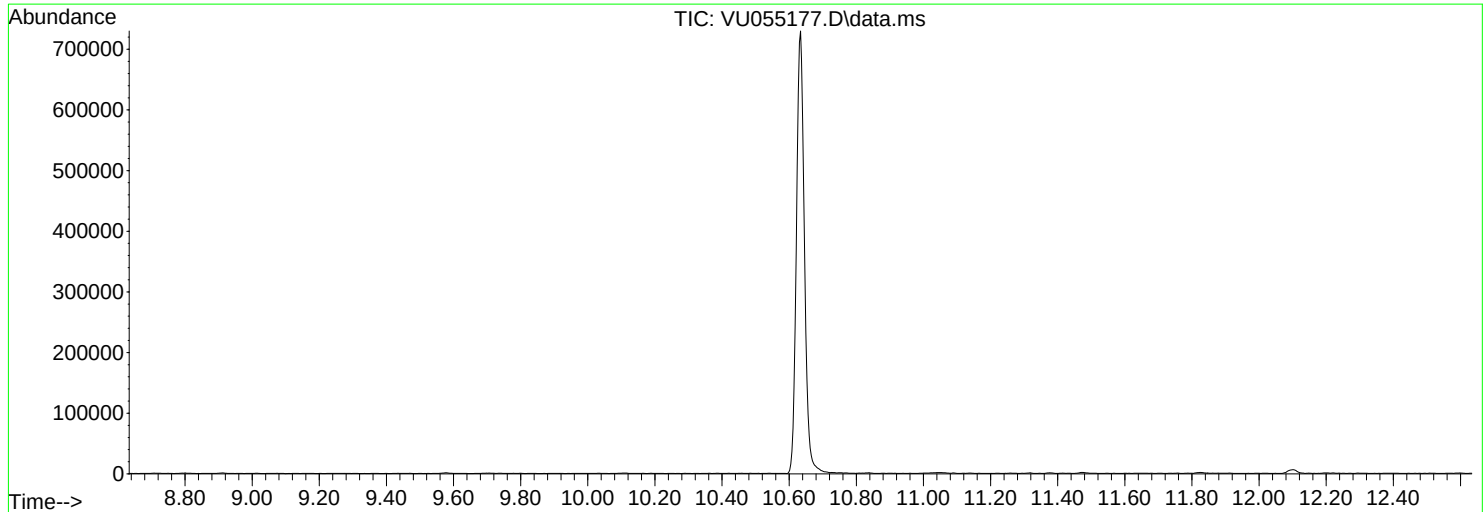

AutoFind: Scans 2905, 2906, 2907; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	28245	PASS
75	95	30	80	56.4	79355	PASS
95	95	100	100	100.0	140587	PASS
96	95	5	9	6.8	9572	PASS
173	174	0.00	2	1.3	1322	PASS
174	95	50	120	74.0	104035	PASS
175	174	5	9	7.4	7652	PASS
176	174	95	101	98.9	102875	PASS
177	176	5	9	6.7	6885	PASS

m/z	Abundance
39.90	238.0
43.90	619.0

Instrument :
MSVOA_U
ClientSampleId :
BFB041

m/z	Abundance
35.90	1655.0
36.90	8103.0
37.90	6989.0
38.90	2245.0
40.00	291.0
43.90	1757.0
44.90	1484.0
45.90	218.0
46.90	1429.0
47.90	1041.0
48.90	6758.0
49.90	29320.0
50.90	9695.0
52.00	369.0
54.90	493.0
55.90	2368.0
56.90	4822.0
59.90	1489.0
60.90	7650.0
61.90	7923.0
62.90	6548.0
64.00	787.0
64.90	603.0
66.00	131.0
66.90	473.0
67.90	16440.0
68.90	16624.0
69.90	1474.0
71.80	734.0
73.00	7325.0
73.90	27728.0
74.90	79432.0
75.90	7036.0
76.90	1033.0
78.00	613.0
78.80	6508.0
79.90	1924.0
80.80	6908.0
81.80	1699.0
83.00	108.0
85.30	114.0
86.80	5650.0
87.90	6106.0
90.90	795.0
91.90	4751.0
92.90	6282.0
93.90	18832.0
94.90	142720.0
95.90	9841.0
96.90	178.0
103.70	762.0
104.80	216.0
105.80	819.0
106.90	248.0
109.90	151.0
110.80	190.0
114.70	154.0
115.70	589.0
116.80	1118.0
117.80	676.0
118.80	987.0
123.60	113.0
127.80	601.0
128.80	338.0
129.90	480.0
130.70	246.0
134.60	288.0
136.80	267.0
140.80	1611.0
141.90	228.0
142.90	2064.0
144.80	243.0
145.80	232.0
147.90	333.0
154.90	277.0
156.70	178.0
158.70	210.0
160.90	153.0
171.90	986.0
172.90	1256.0
173.90	102640.0
174.90	7823.0
175.90	102232.0
176.90	6882.0

Instrument :
MSVOA_U
ClientSampleId :
BFB041

m/z	Abundance
35.90	1700.0
36.90	7767.0
37.90	7125.0
38.90	2249.0
40.00	345.0
42.70	100.0
43.90	1788.0
44.90	1515.0
45.80	205.0
46.90	1557.0
47.90	1172.0
48.90	6659.0
49.90	29144.0
50.90	9606.0
51.90	356.0
54.90	476.0
55.90	2583.0
56.90	4991.0
59.90	1625.0
60.90	7948.0
61.90	8261.0
62.90	6679.0
64.00	835.0
64.90	655.0
66.00	160.0
66.90	586.0
67.90	16504.0
68.90	17368.0
69.90	1508.0
71.80	752.0
73.00	7068.0
73.90	28224.0
74.90	81808.0
75.90	7257.0
76.90	1081.0
77.90	523.0
78.80	6644.0
79.90	1982.0
80.80	6944.0
81.90	1595.0
83.00	125.0
86.90	6001.0
87.90	6049.0
90.80	675.0
91.90	4970.0
92.90	6903.0
93.90	19392.0
94.90	145024.0
95.90	9803.0
97.10	210.0
103.70	774.0
104.80	228.0
105.80	891.0
106.90	316.0
109.80	160.0
110.80	207.0
114.80	177.0
115.90	628.0
116.80	1049.0
117.80	726.0
118.80	1097.0
123.50	100.0
127.80	517.0
128.80	386.0
129.70	474.0
130.70	296.0
134.70	317.0
136.80	311.0
139.90	102.0
140.80	1569.0
142.00	240.0
142.90	2210.0
144.80	264.0
145.80	229.0
148.00	293.0
153.90	110.0
154.90	320.0
156.70	194.0
158.80	218.0
160.90	170.0
168.90	101.0
171.90	1153.0
173.00	1417.0
173.90	107160.0
174.90	7930.0
175.90	105952.0
176.90	7125.0
177.90	163.0

Instrument :
MSVOA_U
ClientSampleId :
BFB041

m/z	Abundance
35.90	1452.0
36.90	7049.0
37.90	6328.0
38.90	2218.0
40.00	318.0
42.70	109.0
43.90	1667.0
44.90	1382.0
45.80	153.0
46.90	1474.0
47.80	1098.0
48.90	5900.0
49.90	26272.0
50.90	8691.0
51.90	384.0
54.90	415.0
55.90	2556.0
56.90	4424.0
57.90	124.0
59.90	1558.0
60.90	7451.0
61.90	7567.0
62.90	6073.0
63.90	826.0
64.90	695.0
66.00	112.0
66.90	558.0
67.90	15298.0
68.90	16253.0
69.90	1390.0
71.80	694.0
73.00	6687.0
73.90	26240.0
74.90	76824.0
75.90	6443.0
76.90	970.0
77.80	531.0
78.90	6250.0
79.90	1875.0
80.80	6323.0
81.80	1432.0
83.00	164.0
86.90	5652.0
87.90	5445.0
90.80	558.0
91.90	4654.0
92.90	6739.0
93.90	18160.0
94.90	134016.0
95.90	9072.0
97.00	239.0
103.80	707.0
104.80	222.0
105.80	934.0
106.80	266.0
109.60	197.0
110.80	212.0
111.60	116.0
114.80	174.0
115.90	645.0
116.90	1001.0
117.80	743.0
118.80	989.0
127.80	491.0
128.80	359.0
129.70	468.0
130.70	321.0
134.70	277.0
136.90	324.0
140.80	1491.0
141.90	217.0
142.80	2030.0
144.90	277.0
145.80	167.0
148.00	252.0
149.60	107.0
153.90	126.0
154.90	311.0
156.70	213.0
158.80	202.0
160.90	162.0
171.90	1109.0
173.00	1292.0
173.90	102304.0
174.90	7202.0
175.90	100440.0
176.90	6649.0
177.90	227.0

Instrument :
MSVOA_U
ClientSampleId :
BFB041