

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090818\
 Data File : VU026630.D
 Acq On : 07 Sep 2018 19:56
 Operator : MD/SY
 Sample : J5071-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BF4

Quant Time: Sep 08 02:14:05 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Sep 08 01:21:38 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	155602	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	146190	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	61567	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	56975	59.10	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	118.20%
7) Chloroethane-d5	1.68	69	50221	57.68	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	115.36%
11) 1,1-Dichloroethene-d2	2.27	63	80848	37.24	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.48%
21) 2-Butanone-d5	4.18	46	88923	118.84	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	118.84%
24) Chloroform-d	4.65	84	99334	54.55	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	109.10%
26) 1,2-Dichloroethane-d4	5.31	65	67492	55.67	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	111.34%
32) Benzene-d6	5.34	84	198538	58.92	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	117.84%
36) 1,2-Dichloropropane-d6	6.33	67	67963	58.72	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	117.44%
41) Toluene-d8	7.57	98	175913	54.08	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	108.16%
43) trans-1,3-Dichloropropene-	7.85	79	27479	51.99	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	103.98%
47) 2-Hexanone-d5	8.31	63	61683	116.19	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	116.19%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	92510	54.25	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	108.50%
64) 1,2-Dichlorobenzene-d4	11.86	152	67792	60.69	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	121.38%#


Target Compounds					Ovalue
13) Acetone	2.32	43	3280	5.062 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU090818\
Data File : VU026630.D
Acq On : 07 Sep 2018 19:56
Operator : MD/SY
Sample : J5071-01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BF4

Quant Time: Sep 08 02:14:05 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 08 01:21:38 2018
Response via : Initial Calibration

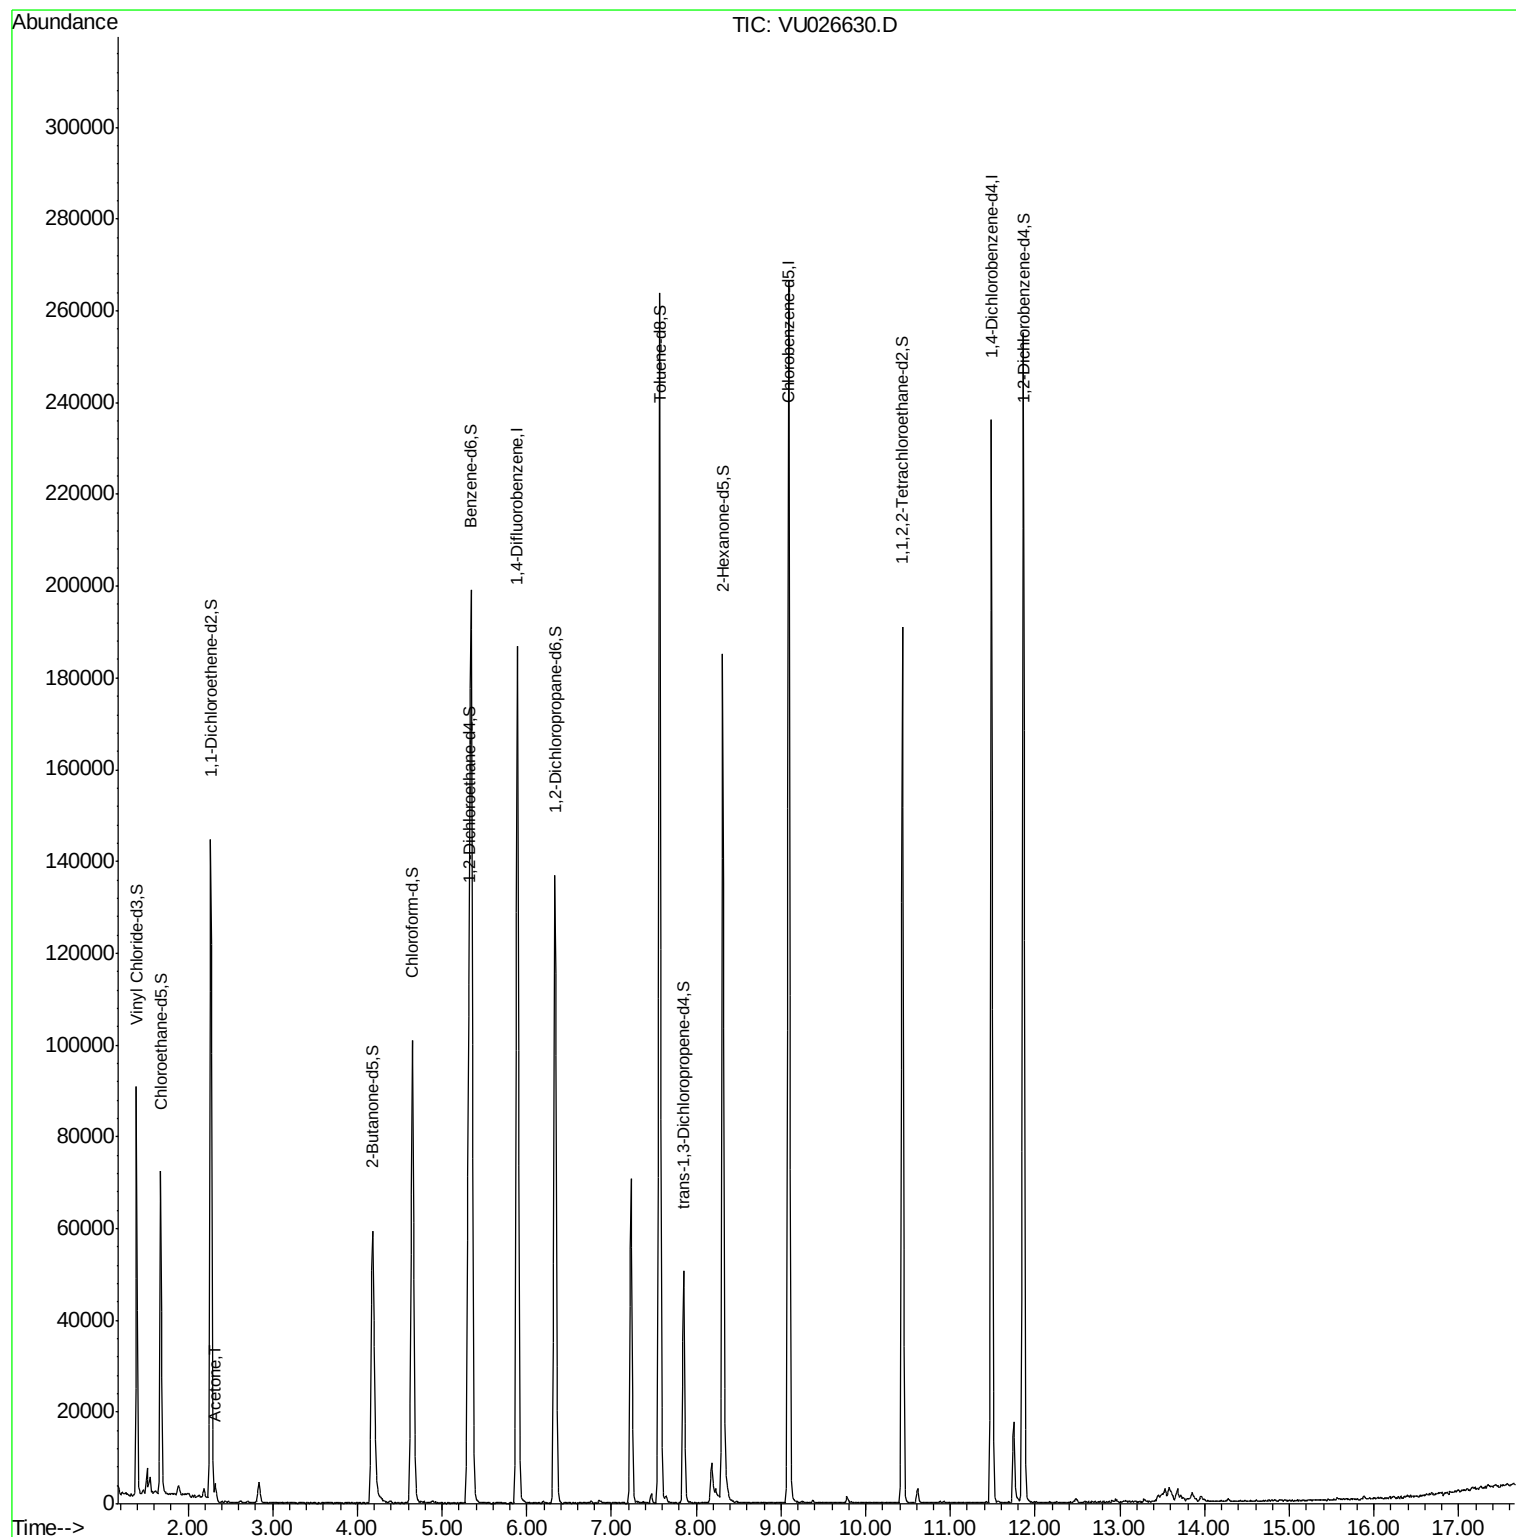

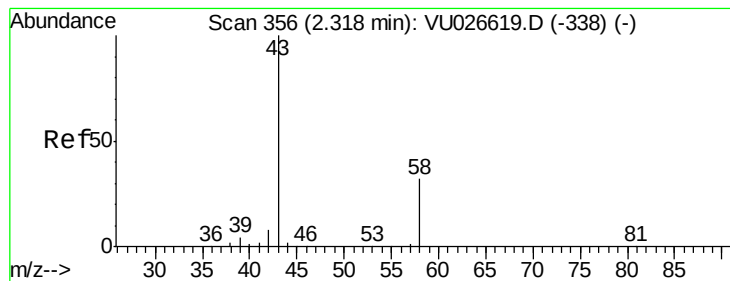

#13
 Acetone
 Concen: 5.062 ug/L
 RT: 2.32 min Scan# 357
 Delta R.T. 0.00 min
 Lab File: VU026630.D
 Acq: 07 Sep 2018 19:56

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BF4

Tot Ion: 43 Resp: 3280
 Ion Ratio Lower Upper
 43 100
 58 27.2 0.0 61.2

