

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090818\
 Data File : VU026621.D
 Acq On : 07 Sep 2018 15:41
 Operator : MD/SY
 Sample : J4718-21
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	63	69	80	rBV	66307	67388	13.85%	1.738%
2	1.678	150	157	172	rVB	54194	70981	14.59%	1.830%
3	2.270	331	341	356	rVB	112013	165374	33.99%	4.265%
4	2.698	469	474	482	rVB	739	1056	0.22%	0.027%
5	2.778	496	499	502	rBV2	130	84	0.02%	0.002%
6	2.794	502	504	505	rVV2	113	47	0.01%	0.001%
7	2.836	506	517	530	rVB2	2902	6379	1.31%	0.165%
8	2.945	548	551	554	rVB2	190	114	0.02%	0.003%
9	3.000	565	568	571	rBV2	191	149	0.03%	0.004%
10	3.173	620	622	626	rBV	110	64	0.01%	0.002%
11	3.209	630	633	636	rBV	114	77	0.02%	0.002%
12	3.286	654	657	663	rVB2	168	142	0.03%	0.004%
13	3.370	679	683	691	rBV	71	100	0.02%	0.003%
14	3.427	697	701	705	rBV	122	101	0.02%	0.003%
15	3.608	750	757	758	rBV	87	74	0.02%	0.002%
16	3.723	791	793	796	rVB	186	97	0.02%	0.003%
17	3.823	816	824	826	rBV2	201	191	0.04%	0.005%
18	3.865	832	837	839	rBV	49	45	0.01%	0.001%
19	3.900	845	848	854	rVV	78	65	0.01%	0.002%
20	3.952	861	864	867	rVB	149	74	0.02%	0.002%
21	4.016	882	884	886	rBV	152	72	0.01%	0.002%
22	4.051	892	895	897	rBV	85	51	0.01%	0.001%
23	4.112	912	914	918	rVB	101	55	0.01%	0.001%
24	4.177	918	934	969	rBV	51247	135307	27.81%	3.489%
25	4.398	1000	1003	1005	rBV	164	118	0.02%	0.003%
26	4.450	1015	1019	1020	rBV	71	48	0.01%	0.001%
27	4.543	1043	1048	1053	rBV	58	74	0.02%	0.002%
28	4.649	1064	1081	1102	rBV	81146	194056	39.89%	5.004%
29	4.935	1168	1170	1172	rVB2	155	81	0.02%	0.002%
30	4.958	1172	1177	1180	rVB	159	102	0.02%	0.003%
31	4.990	1185	1187	1190	rBV	117	96	0.02%	0.002%
32	5.132	1228	1231	1233	rBV	72	52	0.01%	0.001%
33	5.222	1256	1259	1263	rVB	88	57	0.01%	0.001%
34	5.344	1272	1297	1323	rVV2	163866	486478	100.00%	12.545%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090818\
 Data File : VU026621.D
 Acq On : 07 Sep 2018 15:41
 Operator : MD/SY
 Sample : J4718-21
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

35	5.437	1323	1326	1332	rVB2	248	285	0.06%	0.007%
36	5.463	1332	1334	1338	rBV	179	81	0.02%	0.002%
37	5.479	1338	1339	1341	rBV	134	53	0.01%	0.001%
38	5.591	1370	1374	1377	rBV	85	63	0.01%	0.002%
39	5.611	1377	1380	1382	rBV	84	55	0.01%	0.001%
40	5.710	1401	1411	1413	rBV	185	144	0.03%	0.004%
41	5.736	1416	1419	1423	rVV	72	53	0.01%	0.001%
42	5.887	1451	1466	1488	rBV	180894	347640	71.46%	8.965%
43	6.013	1503	1505	1507	rBV	145	52	0.01%	0.001%
44	6.022	1507	1508	1511	rVB	179	63	0.01%	0.002%
45	6.115	1534	1537	1540	rVB	94	64	0.01%	0.002%
46	6.154	1546	1549	1552	rVV	69	44	0.01%	0.001%
47	6.180	1552	1557	1563	rVV2	274	320	0.07%	0.008%
48	6.334	1590	1605	1628	rVB	115494	228950	47.06%	5.904%
49	6.427	1630	1634	1636	rBV	90	70	0.01%	0.002%
50	6.456	1642	1643	1648	rVB	159	55	0.01%	0.001%
51	6.537	1665	1668	1671	rBV	67	58	0.01%	0.001%
52	6.726	1724	1727	1729	rBV	82	53	0.01%	0.001%
53	6.784	1740	1745	1751	rVB	120	123	0.03%	0.003%
54	6.829	1751	1759	1762	rBV	226	160	0.03%	0.004%
55	6.852	1762	1766	1770	rBV2	339	349	0.07%	0.009%
56	6.932	1787	1791	1794	rBV	84	63	0.01%	0.002%
57	7.013	1811	1816	1820	rBV	96	107	0.02%	0.003%
58	7.070	1830	1834	1835	rBV	94	60	0.01%	0.002%
59	7.122	1847	1850	1854	rBV	85	69	0.01%	0.002%
60	7.173	1860	1866	1869	rBV	73	73	0.02%	0.002%
61	7.228	1869	1883	1900	rBV2	60328	105815	21.75%	2.729%
62	7.321	1908	1912	1913	rBV	117	73	0.02%	0.002%
63	7.459	1953	1955	1963	rVB2	291	230	0.05%	0.006%
64	7.569	1975	1989	2008	rBV	209483	362470	74.51%	9.347%
65	7.720	2034	2036	2039	rBV	143	62	0.01%	0.002%
66	7.852	2066	2077	2093	rBV	43536	71991	14.80%	1.857%
67	7.951	2101	2108	2111	rBV	130	133	0.03%	0.003%
68	7.993	2117	2121	2123	rBV	90	66	0.01%	0.002%
69	8.003	2123	2124	2128	rVB	124	90	0.02%	0.002%
70	8.122	2159	2161	2165	rVB	175	105	0.02%	0.003%
71	8.183	2166	2180	2191	rBV2	7227	16025	3.29%	0.413%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090818\
 Data File : VU026621.D
 Acq On : 07 Sep 2018 15:41
 Operator : MD/SY
 Sample : J4718-21
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

72	8.312	2210	2220	2248	rVB	161476	267470	54.98%	6.898%
73	8.620	2308	2316	2326	rVB2	1242	1856	0.38%	0.048%
74	8.868	2390	2393	2400	rVB	107	103	0.02%	0.003%
75	8.938	2411	2415	2418	rBV	79	60	0.01%	0.002%
76	9.090	2450	2462	2486	rBV	251093	415511	85.41%	10.715%
77	9.221	2500	2503	2504	rBV	131	57	0.01%	0.001%
78	9.598	2619	2620	2624	rVB	184	71	0.01%	0.002%
79	9.623	2624	2628	2630	rBV	101	83	0.02%	0.002%
80	9.749	2665	2667	2670	rVB	153	53	0.01%	0.001%
81	9.781	2675	2677	2680	rVV	193	144	0.03%	0.004%
82	9.797	2680	2682	2685	rVB	212	97	0.02%	0.003%
83	9.852	2696	2699	2701	rBV	73	44	0.01%	0.001%
84	10.022	2748	2752	2753	rBV	154	104	0.02%	0.003%
85	10.080	2766	2770	2773	rBV2	304	288	0.06%	0.007%
86	10.192	2803	2805	2808	rVB	206	98	0.02%	0.003%
87	10.218	2810	2813	2816	rVV2	201	119	0.02%	0.003%
88	10.363	2855	2858	2859	rBV	155	88	0.02%	0.002%
89	10.434	2868	2880	2898	rVB	163968	258324	53.10%	6.662%
90	10.562	2918	2920	2922	rBV	152	53	0.01%	0.001%
91	10.614	2926	2936	2942	rBV3	2022	2893	0.59%	0.075%
92	10.874	3014	3017	3019	rBV	233	149	0.03%	0.004%
93	10.935	3034	3036	3038	rBV	138	58	0.01%	0.001%
94	11.096	3083	3086	3087	rBV	171	78	0.02%	0.002%
95	11.421	3184	3187	3192	rVB	710	552	0.11%	0.014%
96	11.485	3195	3207	3222	rBV	220779	340404	69.97%	8.778%
97	11.601	3241	3243	3245	rBV	170	47	0.01%	0.001%
98	11.861	3312	3324	3343	rBV	204390	322035	66.20%	8.305%
99	12.006	3365	3369	3371	rBV	276	255	0.05%	0.007%
100	12.482	3509	3517	3527	rVB2	707	1245	0.26%	0.032%


Sum of corrected areas: 3877755

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU090818\
Data File : VU026621.D
Acq On : 07 Sep 2018 15:41
Operator : MD/SY
Sample : J4718-21
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

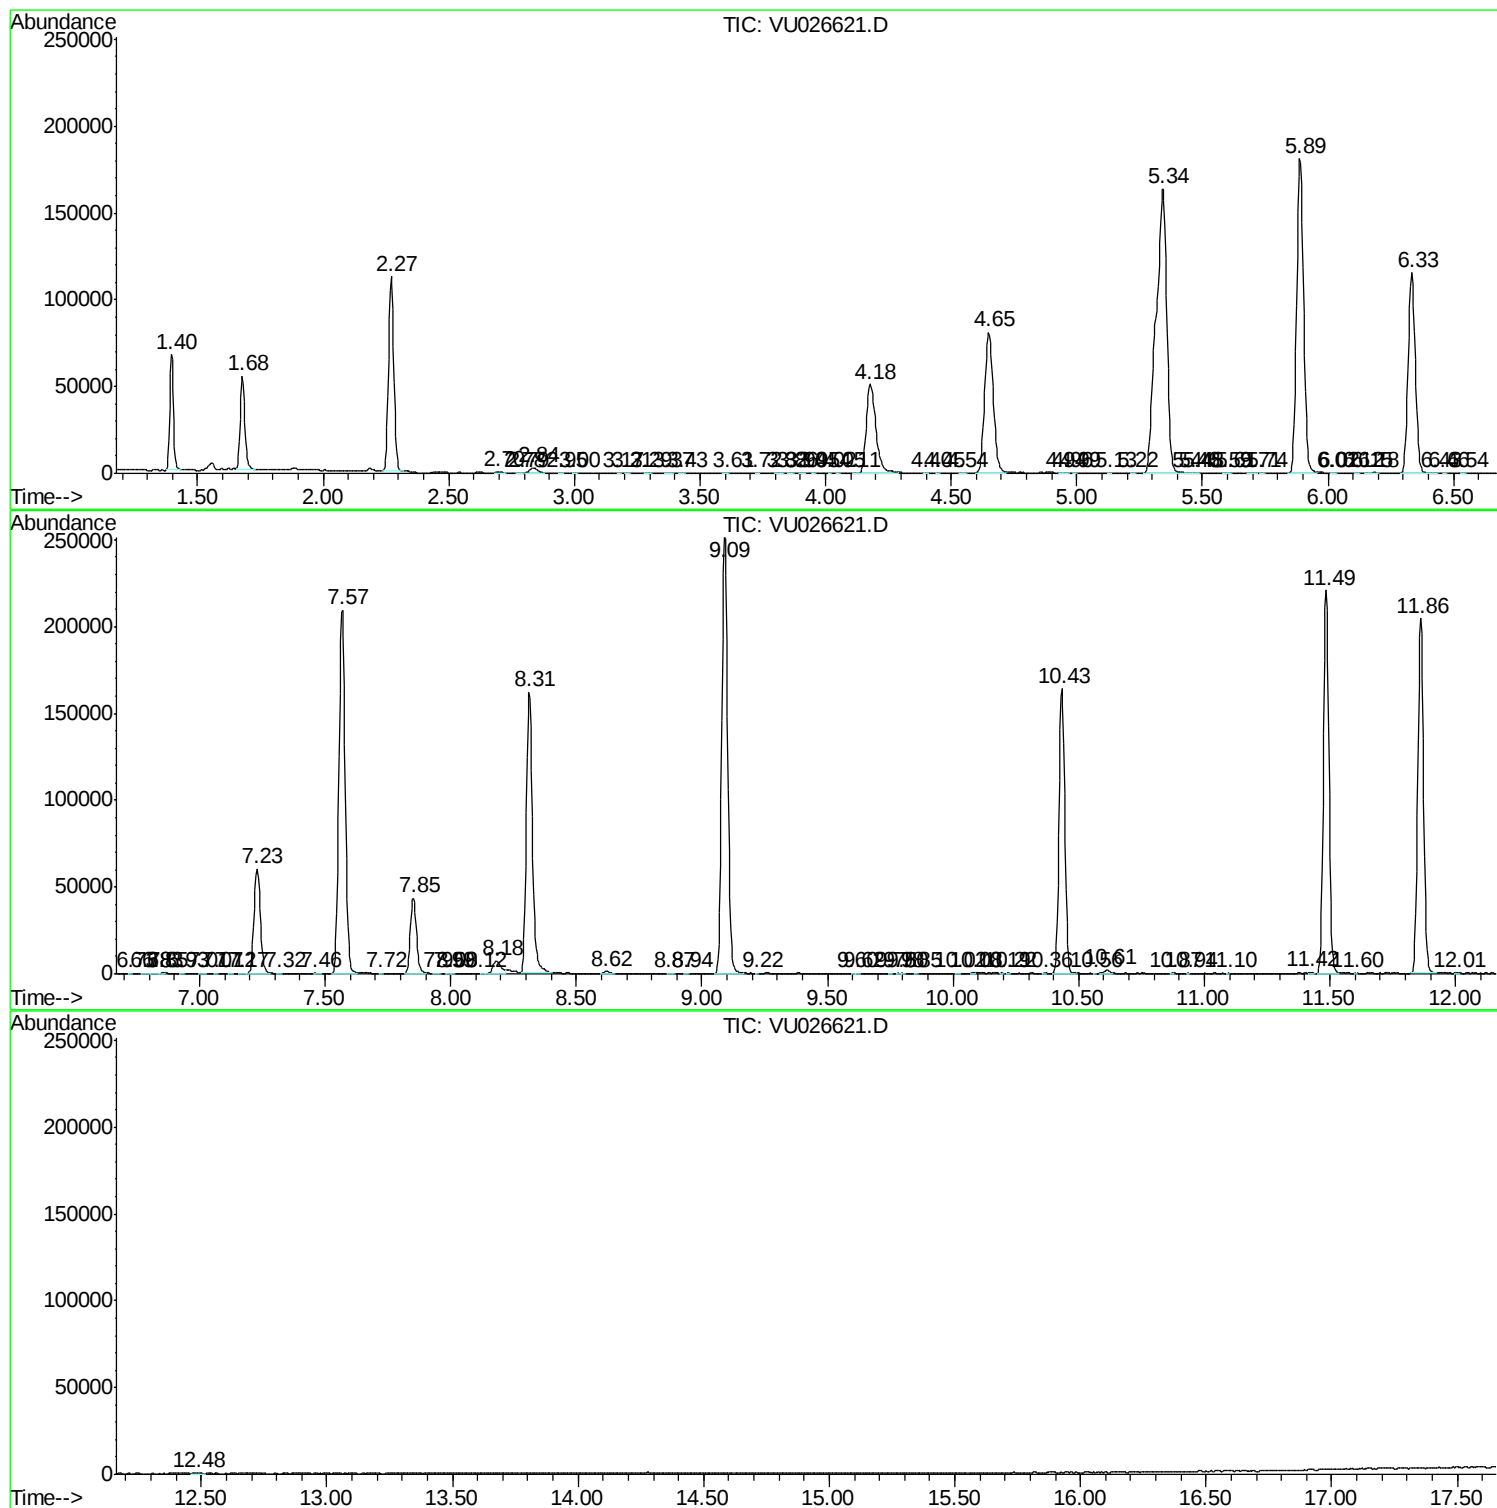

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU090818\
Data File : VU026621.D
Acq On : 07 Sep 2018 15:41
Operator : MD/SY
Sample : J4718-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU090818\
Data File : VU026621.D
Acq On : 07 Sep 2018 15:41
Operator : MD/SY
Sample : J4718-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc