


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090818\
Data File : VU026618.D
Acq On : 07 Sep 2018 13:45
Operator : MD/SY
Sample : BFB51
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB51

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Title : VOC Analysis
Last Update : Sat Sep 08 01:21:38 2018

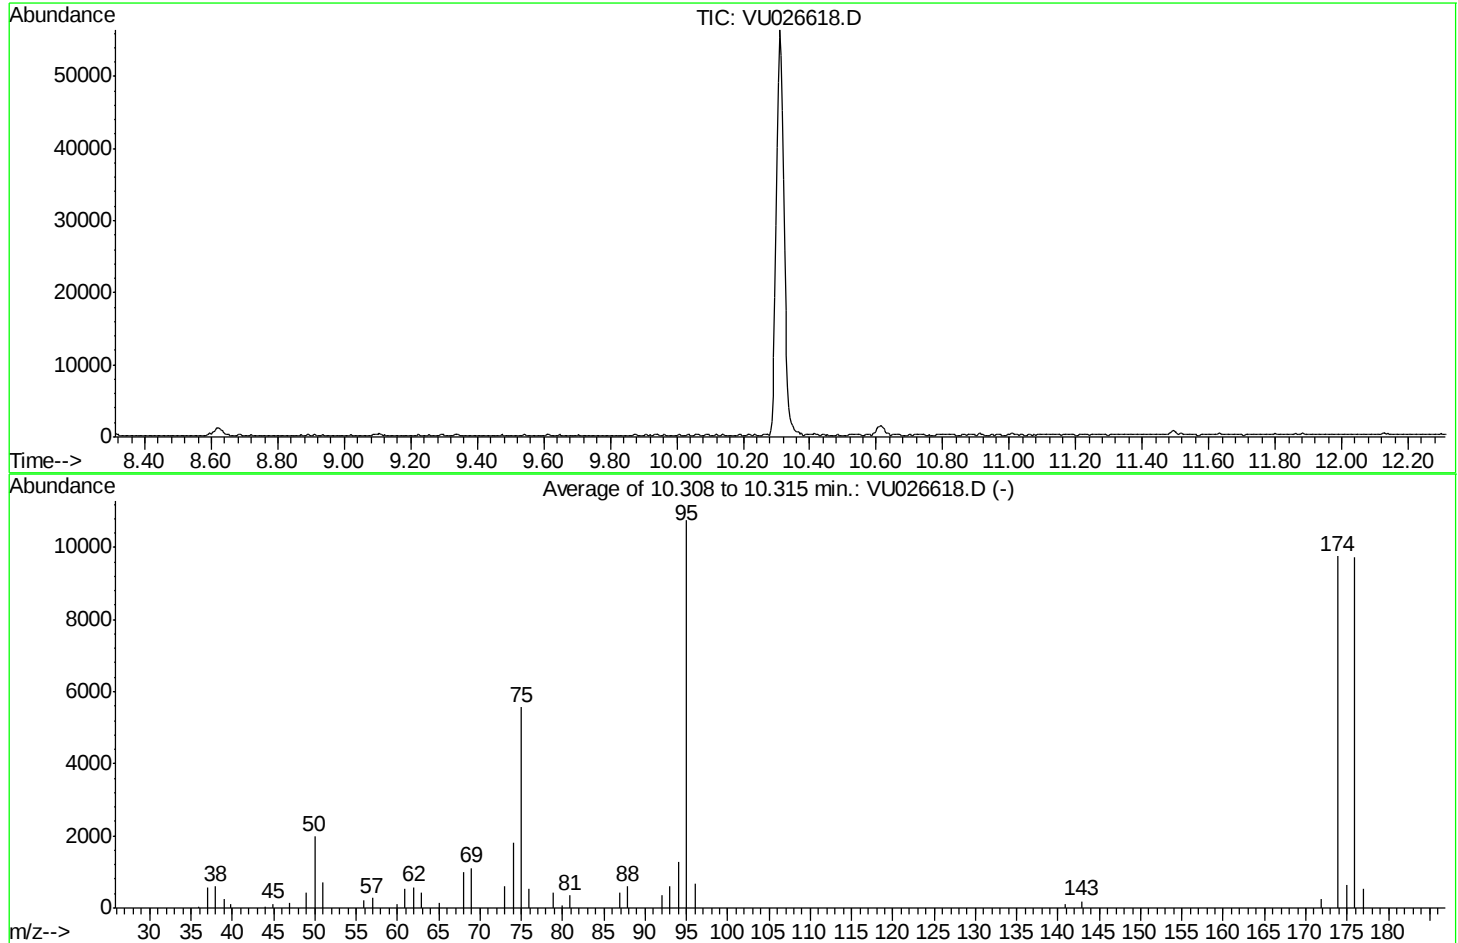

AutoFind: Scans 2841, 2842, 2843; Background Corrected with Scan 2831

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	1983	PASS
75	95	30	80	51.8	5567	PASS
95	95	100	100	100.0	10750	PASS
96	95	5	9	6.4	693	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	90.8	9758	PASS
175	174	5	9	6.6	645	PASS
176	174	95	101	99.6	9716	PASS
177	176	5	9	5.6	546	PASS

Scan 2831 (10.276 min): VU026618.D
BFB51

m/z	Abundance
44.00	279.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

m/z	Abundance
35.90	104.0
37.00	563.0
38.00	619.0
39.00	272.0
39.90	101.0
44.00	370.0
45.00	129.0
47.00	150.0
48.90	446.0
50.00	2136.0
50.90	733.0
55.90	233.0
57.00	272.0
60.00	101.0
60.90	499.0
62.00	574.0
63.00	422.0
65.10	145.0
68.00	1055.0
69.00	1171.0
73.00	596.0
74.00	1868.0
75.00	5645.0
76.00	571.0
78.90	428.0
79.90	108.0
80.90	369.0
86.90	448.0
87.90	602.0
92.00	326.0
93.00	643.0
94.00	1316.0
95.00	10652.0
96.00	658.0
140.80	124.0
142.90	188.0
171.90	208.0
173.90	9704.0
175.00	598.0
175.90	9584.0
176.90	598.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

m/z	Abundance
37.00	588.0
38.00	623.0
39.00	271.0
39.80	105.0
43.90	305.0
45.00	112.0
47.00	136.0
48.90	434.0
50.00	2026.0
50.90	739.0
55.90	225.0
57.00	267.0
60.00	118.0
60.90	555.0
62.00	594.0
62.90	416.0
65.00	157.0
68.00	1005.0
69.00	1149.0
73.00	625.0
74.00	1840.0
75.00	5700.0
75.90	532.0
78.90	418.0
79.90	105.0
80.90	352.0
87.00	439.0
87.90	649.0
92.00	359.0
93.00	640.0
94.00	1316.0
95.00	11083.0
96.00	723.0
140.80	135.0
142.90	193.0
171.90	262.0
173.90	10006.0
174.90	654.0
175.90	10027.0
176.90	550.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

m/z	Abundance
37.00	510.0
38.00	540.0
39.00	236.0
39.90	103.0
44.00	246.0
44.90	100.0
46.90	118.0
48.90	413.0
50.00	1789.0
51.00	662.0
56.00	171.0
57.00	270.0
59.90	123.0
61.00	543.0
62.00	559.0
62.90	406.0
64.90	154.0
68.00	914.0
69.00	1018.0
73.00	595.0
74.00	1737.0
75.00	5357.0
75.90	473.0
78.90	389.0
80.90	316.0
87.00	391.0
87.90	549.0
92.00	335.0
92.90	546.0
94.00	1210.0
95.00	10516.0
96.00	700.0
140.80	118.0
142.90	173.0
171.90	278.0
173.90	9566.0
174.90	684.0
175.90	9538.0
176.90	490.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51