

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090819\
 Data File : VU034372.D
 Acq On : 07 Sep 2019 11:48
 Operator : JC/SP
 Sample : K4682-07
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0BN1

Quant Time: Sep 09 05:11:55 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR090119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Sep 03 14:18:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.86	114	363687	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	350876	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.46	152	176840	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	75703	3.09	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	61.80%
7) Chloroethane-d5	1.68	69	67094	3.42	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	68.40%
11) 1,1-Dichloroethene-d2	2.26	63	112611	2.45	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	49.00%#
20) 2-Butanone-d5	4.17	46	207114	36.60	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	73.20%
24) Chloroform-d	4.63	84	155573	3.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	72.00%
26) 1,2-Dichloroethane-d4	5.29	65	76544	3.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.80%
32) Benzene-d6	5.32	84	335839	3.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	73.40%
36) 1,2-Dichloropropane-d6	6.31	67	107266	3.77	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	75.40%
41) Toluene-d8	7.55	98	300809	3.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	70.20%
43) trans-1,3-Dichloropropene-	7.84	79	37001	3.66	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.20%
46) 2-Hexanone-d5	8.30	63	162013	37.00	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	74.00%
57) 1,1,2,2-Tetrachloroethane-	10.41	84	82346	3.90	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	78.00%
64) 1,2-Dichlorobenzene-d4	11.84	152	126226	4.15	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	83.00%


Target Compounds					Ovalue
13) Acetone	2.32	43	5138	1.356 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090819\
Data File : VU034372.D
Acq On : 07 Sep 2019 11:48
Operator : JC/SP
Sample : K4682-07
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0BN1

Quant Time: Sep 09 05:11:55 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR090119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Sep 03 14:18:00 2019
Response via : Initial Calibration

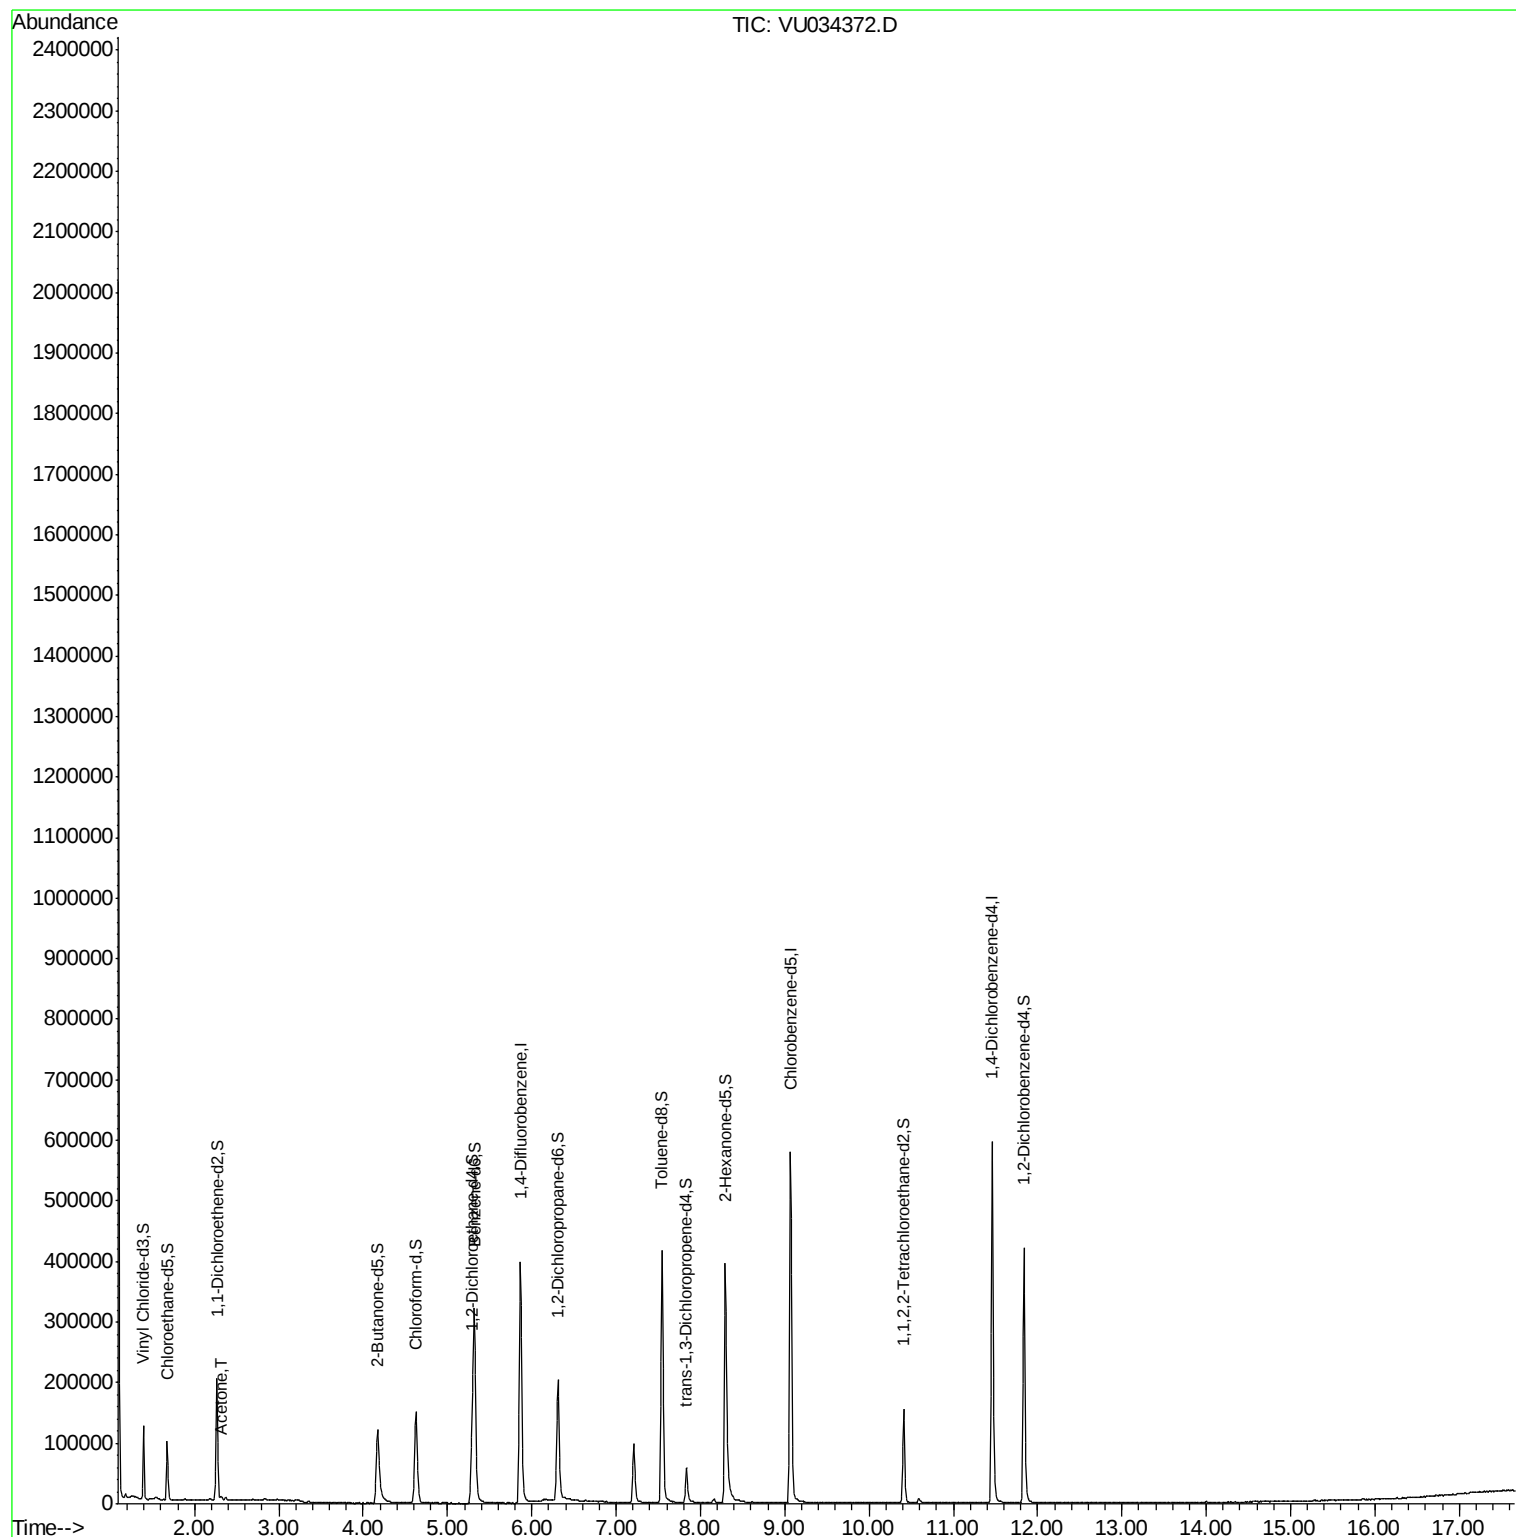

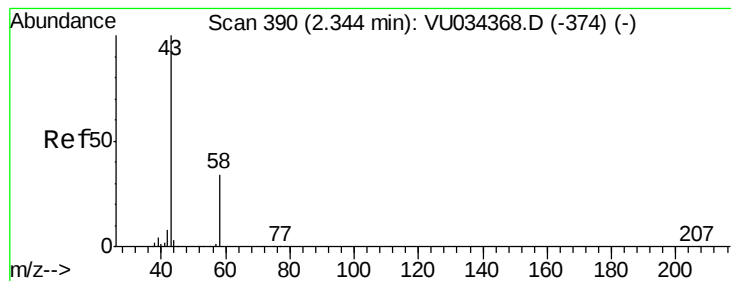

#13

Acetone

Concen: 1.356 ug/L

RT: 2.32 min Scan# 381

Delta R.T. -0.01 min

Lab File: VU034372.D

Acq: 07 Sep 2019 11:48

Instrument :

MSVOA_U

ClientSampleId :

H0BN1

Tot Ion: 43 Resp: 5138

Ion Ratio Lower Upper

43 100

58 35.1 0.0 67.6

