

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090819\
 Data File : VU034392.D
 Acq On : 07 Sep 2019 19:50
 Operator : JC/SP
 Sample : K4685-13
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFD82

Quant Time: Sep 09 05:45:10 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR090119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Sep 03 14:18:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.86	114	284414	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	289422	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.46	152	136439	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	72652	3.79	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.80%
7) Chloroethane-d5	1.68	69	68047	4.43	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.60%
11) 1,1-Dichloroethene-d2	2.26	63	111651	3.11	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.20%
20) 2-Butanone-d5	4.17	46	207549	46.90	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.80%
24) Chloroform-d	4.63	84	162784	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.20%
26) 1,2-Dichloroethane-d4	5.29	65	77451	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.80%
32) Benzene-d6	5.32	84	335094	4.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.00%
36) 1,2-Dichloropropane-d6	6.31	67	110788	4.73	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.60%
41) Toluene-d8	7.55	98	294088	4.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.20%
43) trans-1,3-Dichloropropene-	7.83	79	34822	4.18	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.60%
46) 2-Hexanone-d5	8.30	63	156100	43.22	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.44%
57) 1,1,2,2-Tetrachloroethane-	10.41	84	84147	4.83	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.60%
64) 1,2-Dichlorobenzene-d4	11.84	152	120667	5.15	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.00%

Target Compounds


					Ovalue
13) Acetone	2.31	43	9814	3.313 ug/L	95
17) Methyl tert-butyl Ether	2.99	73	21445	0.487 ug/L	98
25) Chloroform	4.65	83	53208	1.386 ug/L	99
47) Tetrachloroethene	8.21	164	76101	4.104 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU090819\
Data File : VU034392.D
Acq On : 07 Sep 2019 19:50
Operator : JC/SP
Sample : K4685-13
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFD82

Quant Time: Sep 09 05:45:10 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR090119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Sep 03 14:18:00 2019
Response via : Initial Calibration

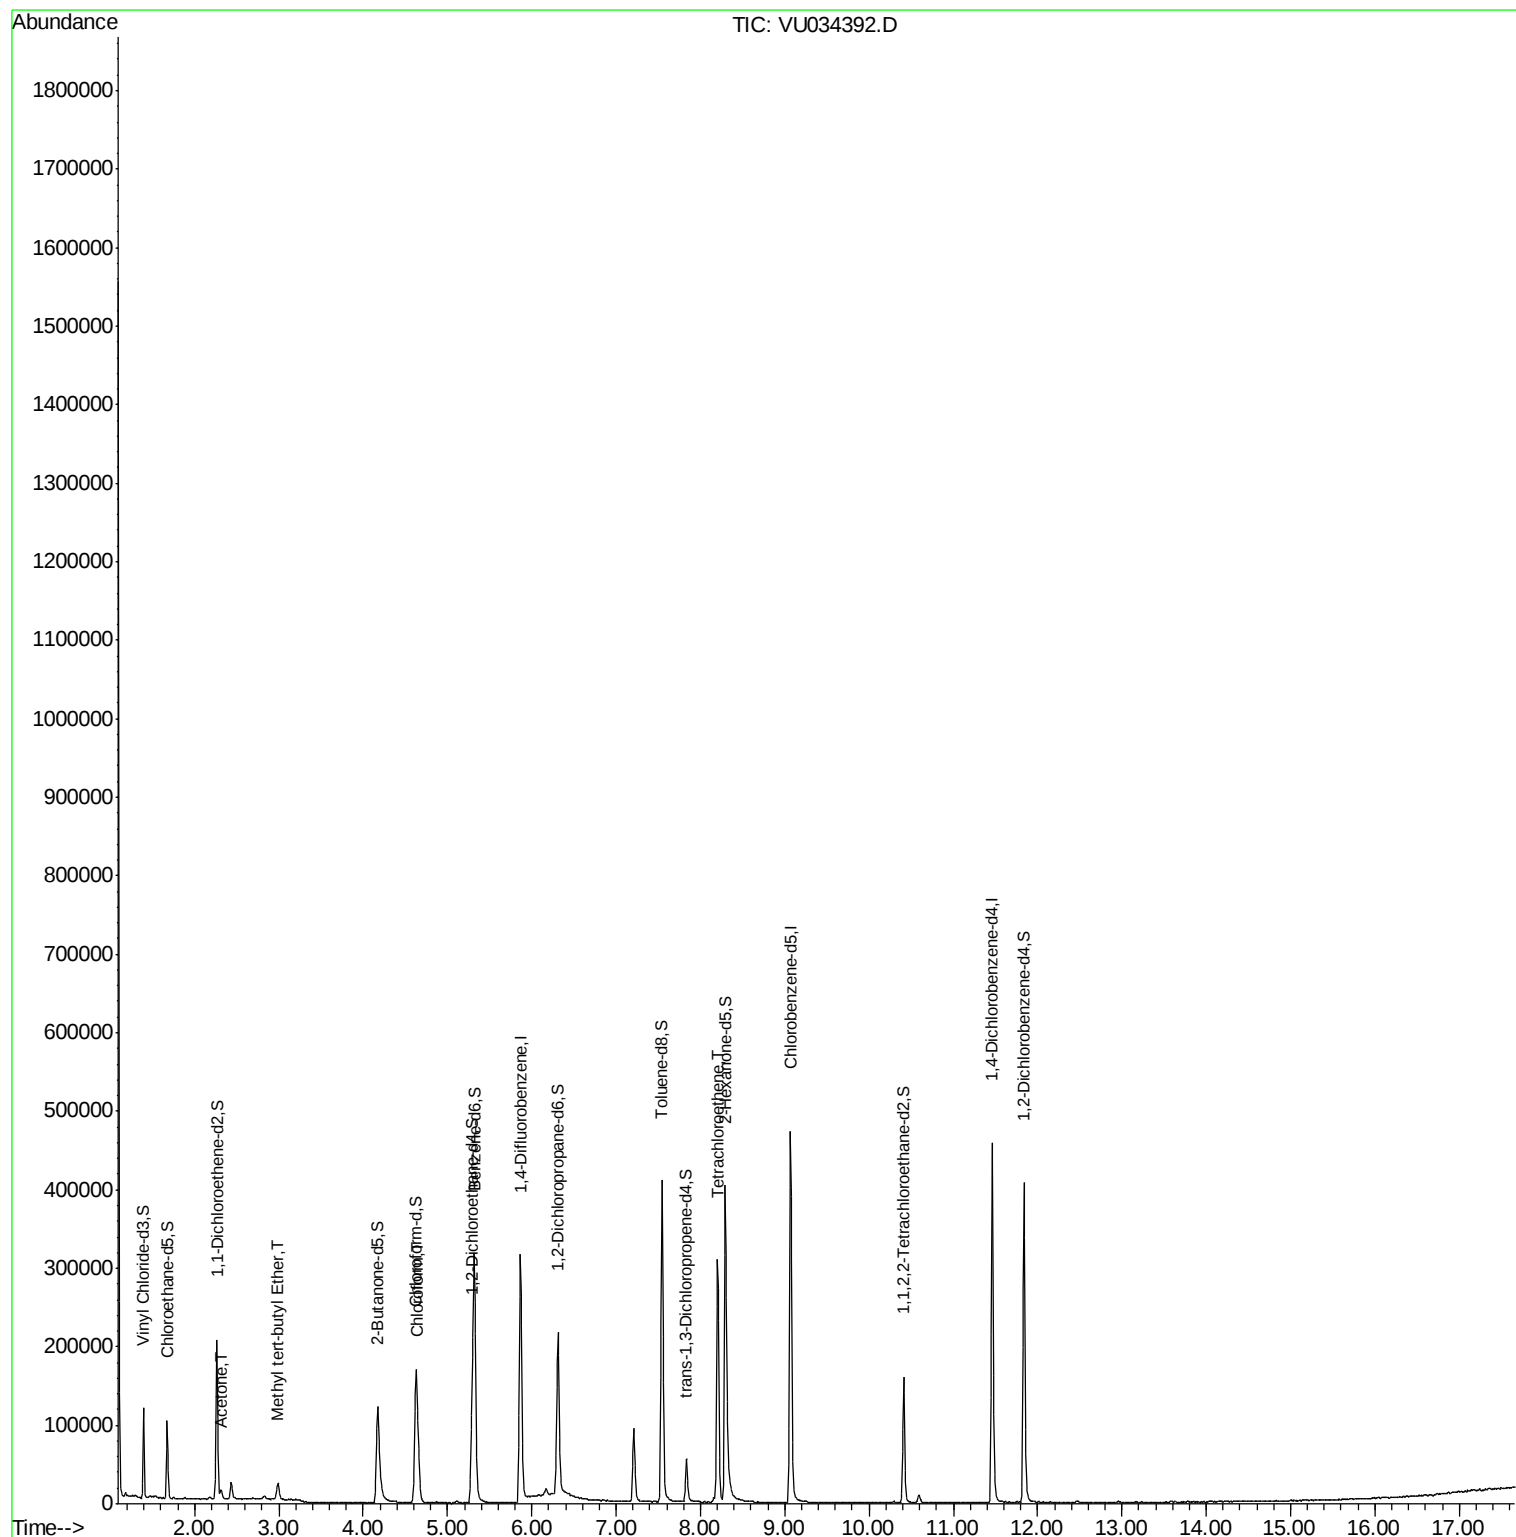

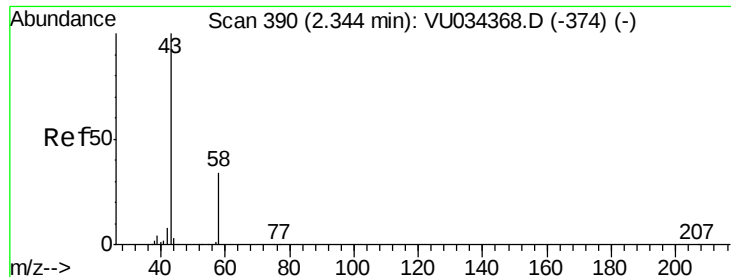

#13

Acetone

Concen: 3.313 ug/L

RT: 2.31 min Scan# 380

Delta R.T. -0.01 min

Lab File: VU034392.D

Acq: 07 Sep 2019 19:50

Instrument :

MSVOA_U

ClientSampleId :





BFD82

Tot Ion: 43 Resp: 9814

Ion Ratio Lower Upper

43 100

58 36.7 0.0 67.6

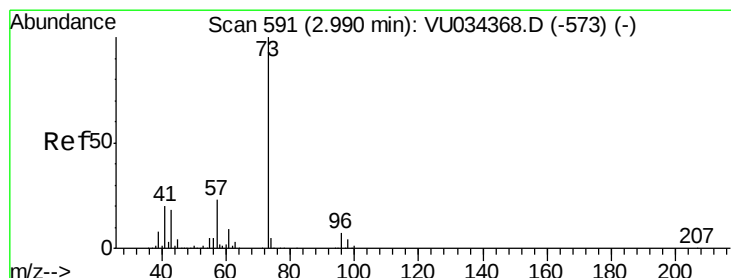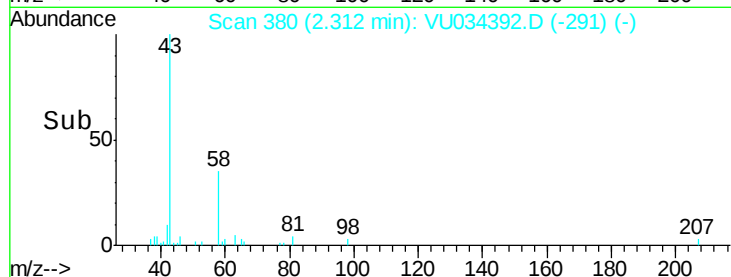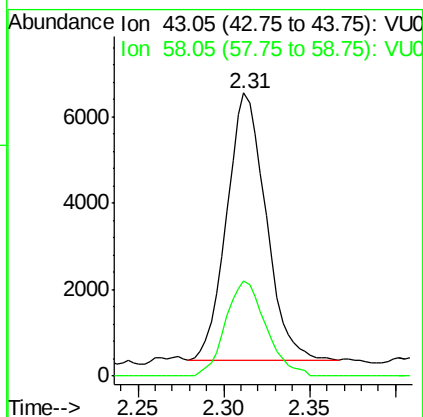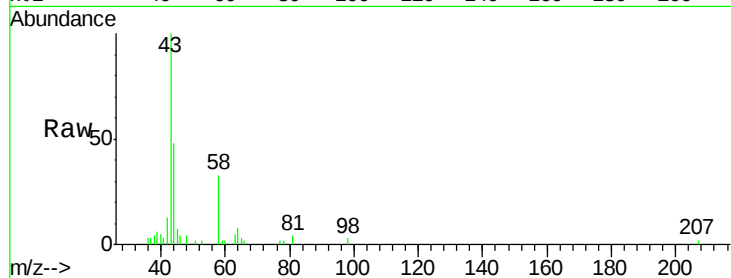

#17

Methyl tert-butyl Ether

Concen: 0.487 ug/L

RT: 2.99 min Scan# 591

Delta R.T. 0.00 min

Lab File: VU034392.D

Acq: 07 Sep 2019 19:50




Tgt Ion: 73 Resp: 21445


Ion Ratio Lower Upper

73 100

43 19.8 14.7 22.1

57 24.1 18.6 27.8

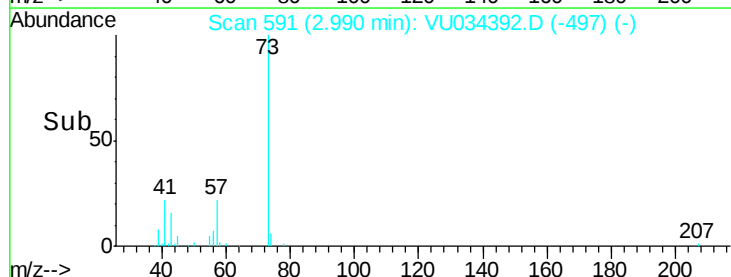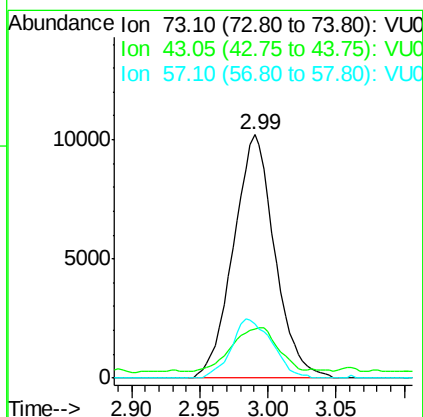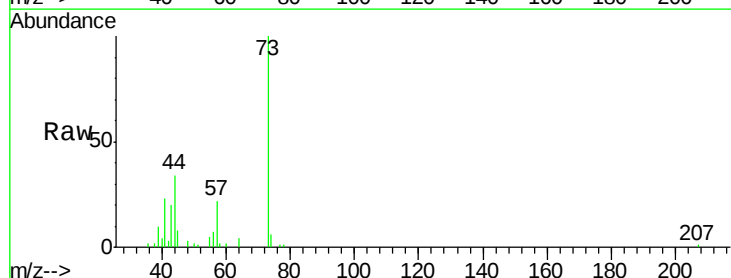

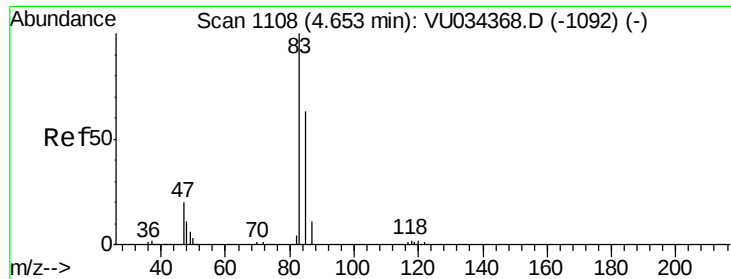

#25

Chloroform

Concen: 1.386 ug/L

RT: 4.65 min Scan# 1108

Delta R.T. 0.00 min

Lab File: VU034392.D

Acq: 07 Sep 2019 19:50

Instrument :

MSVOA_U

ClientSampleId :


BFD82

Tot Ion: 83 Resp: 53208

Ion Ratio Lower Upper

83 100

85 66.2 46.8 86.8

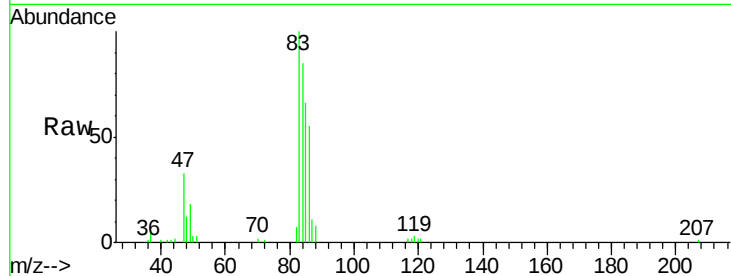

Abundance Ion 83.05 (82.75 to 83.75): VU034392.D (-1014) (-)

Ion 85.00 (84.70 to 85.70): VU034392.D (-1014) (-)

4.65

25000

20000

15000



10000

5000

0

Time-->

4.55 4.60 4.65 4.70 4.75

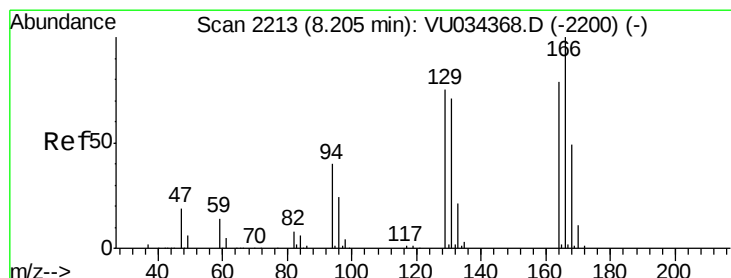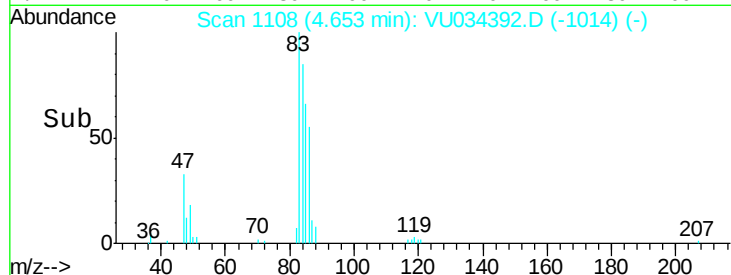

#47

Tetrachloroethene

Concen: 4.104 ug/L

RT: 8.21 min Scan# 2213

Delta R.T. -0.00 min

Lab File: VU034392.D

Acq: 07 Sep 2019 19:50

Tgt Ion: 164 Resp: 76101


Ion Ratio Lower Upper

164 100

129 90.4 68.0 126.2

131 87.4 64.6 120.0

166 125.5 92.0 170.8

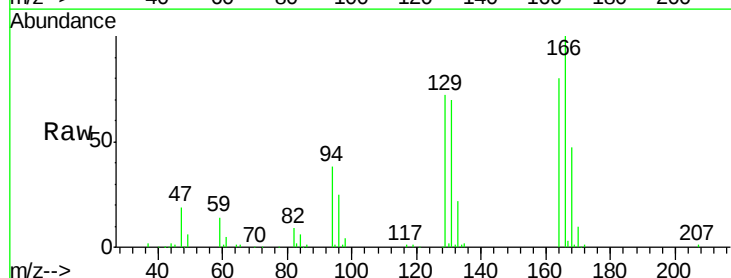

Abundance Ion 163.90 (163.60 to 164.60): VU034392.D (-2121) (-)

Ion 128.95 (128.65 to 129.65): VU034392.D (-2121) (-)

Ion 130.95 (130.65 to 131.65): VU034392.D (-2121) (-)

Ion 165.90 (165.60 to 166.60): VU034392.D (-2121) (-)

80000

60000

40000

20000

0

Time-->

8.15 8.20 8.25 8.30

