


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU090819\
Data File : VU034367.D
Acq On : 07 Sep 2019 09:29
Operator : JC/SP
Sample : BFB07
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB07

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR090119WMA.M
Title : TRACE VOA SOM01.0
Last Update : Sun Sep 08 03:44:03 2019

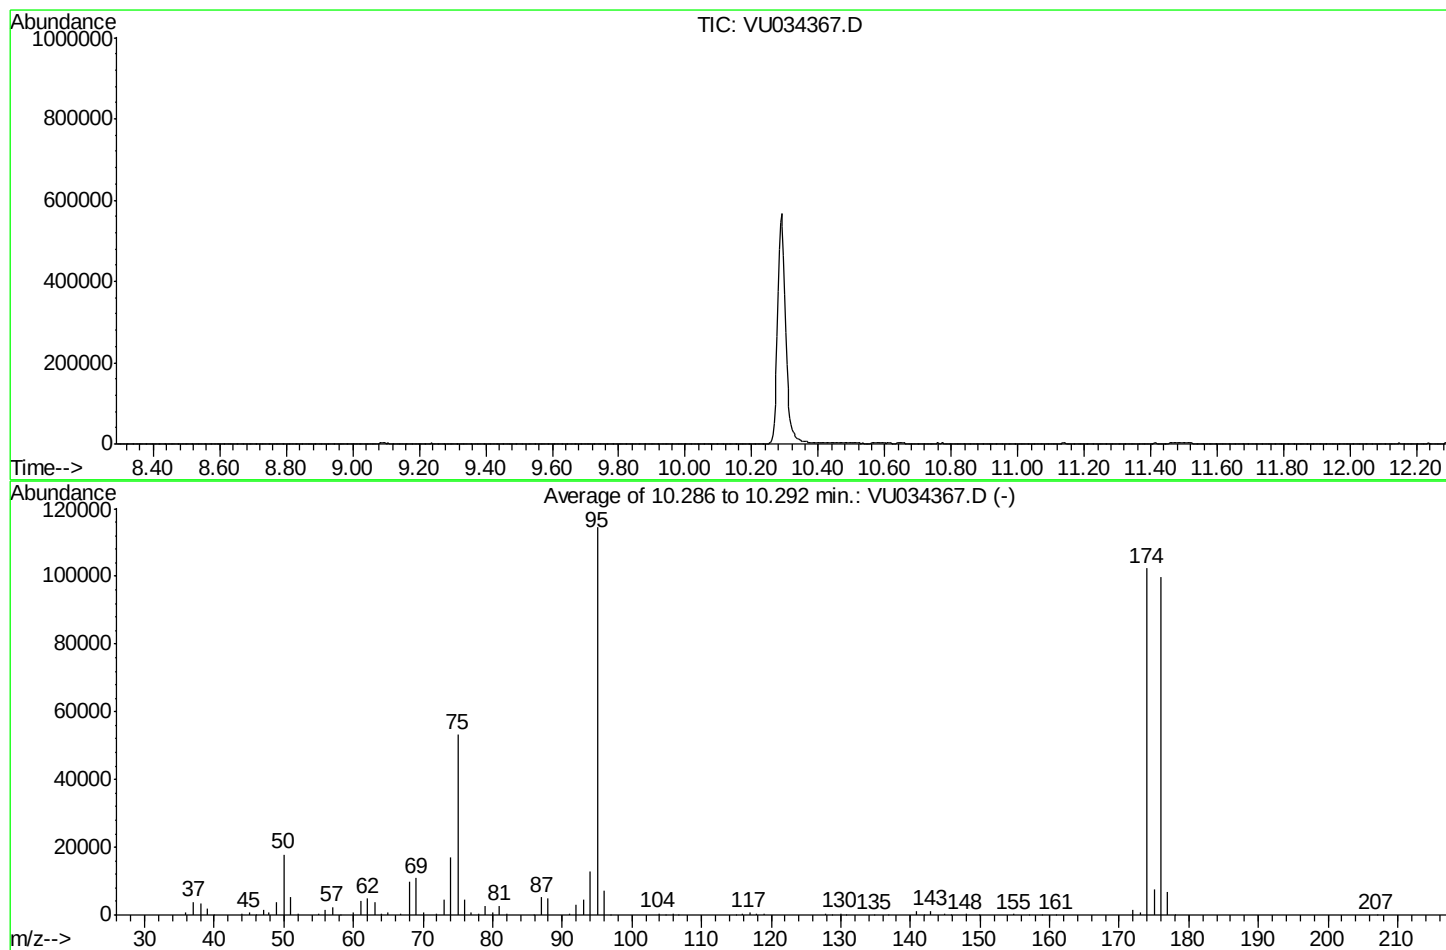

AutoFind: Scans 2860, 2861, 2862; Background Corrected with Scan 2847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	17829	PASS
75	95	30	80	46.5	53184	PASS
95	95	100	100	100.0	114474	PASS
96	95	5	9	6.4	7335	PASS
173	174	0.00	2	0.7	762	PASS
174	95	50	120	89.4	102360	PASS
175	174	5	9	7.4	7554	PASS
176	174	95	101	97.6	99933	PASS
177	176	5	9	6.7	6653	PASS

m/z	Abundance
36.00	796.0
37.00	4205.0
38.00	3530.0
39.00	1767.0
39.90	242.0
44.00	1050.0
45.00	777.0
46.00	140.0
47.00	1416.0
47.90	628.0
49.00	3759.0
50.00	18200.0
51.00	5399.0
52.00	268.0
54.90	220.0
56.00	1547.0
57.00	2475.0
58.10	108.0
60.00	910.0
61.00	4303.0
62.00	4904.0
63.00	3720.0
64.00	429.0
65.00	808.0
66.80	220.0
68.00	9770.0
69.00	11071.0
70.00	951.0
72.00	574.0
73.00	4768.0
74.00	16960.0
75.00	53472.0
76.10	4538.0
77.00	704.0
77.90	468.0
78.90	2735.0
80.00	665.0
81.00	2652.0
82.00	518.0
85.90	122.0
87.00	5047.0
88.00	4937.0
90.90	333.0
92.00	2927.0
93.00	4756.0
94.00	12880.0
95.00	113864.0
96.00	7450.0
96.90	176.0
103.90	439.0
104.90	157.0
105.90	355.0
106.70	109.0
115.90	281.0
116.90	649.0
117.80	445.0
119.00	440.0
127.80	355.0
128.80	126.0
130.00	449.0
130.80	196.0
134.80	128.0
136.90	147.0
140.90	934.0
143.00	1179.0
144.90	295.0
145.90	153.0
148.00	283.0
149.80	114.0
154.90	327.0
157.00	223.0
158.80	115.0
160.90	130.0
171.90	1318.0
174.00	100384.0
175.00	7367.0
176.00	97552.0
177.00	6659.0
178.00	169.0
207.00	214.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

m/z	Abundance
36.00	833.0
37.00	4100.0
38.00	3592.0
39.00	1869.0
39.90	216.0
44.00	1027.0
45.00	773.0
45.90	128.0
47.10	1421.0
47.90	592.0
49.00	4126.0
50.00	18424.0
51.00	5324.0
52.00	292.0
55.00	271.0
56.00	1715.0
57.00	2463.0
58.00	121.0
60.00	941.0
61.00	4363.0
62.00	4953.0
63.10	3896.0
63.90	421.0
65.00	799.0
66.80	240.0
68.00	10212.0
69.00	11261.0
70.00	945.0
72.00	578.0
73.00	4830.0
74.00	17504.0
75.00	54864.0
76.00	4497.0
77.00	715.0
77.90	487.0
78.90	2571.0
80.00	644.0
81.00	2784.0
81.90	555.0
85.90	157.0
87.00	5341.0
88.00	5069.0
91.00	318.0
92.00	3063.0
93.00	4789.0
94.00	13189.0
95.00	117992.0
96.00	7487.0
96.90	156.0
103.90	454.0
104.80	149.0
105.90	396.0
106.70	106.0
114.90	106.0
115.80	244.0
116.90	732.0
117.80	464.0
119.00	475.0
127.80	388.0
128.80	167.0
129.90	424.0
130.80	183.0
134.90	154.0
136.80	161.0
140.90	1062.0
142.00	160.0
142.90	1195.0
144.90	262.0
145.90	170.0
148.00	299.0
149.90	117.0
154.90	405.0
157.00	176.0
158.80	143.0
161.00	120.0
171.90	1427.0
173.00	1163.0
174.00	105464.0
175.00	7744.0
176.00	102960.0
177.00	6882.0
178.00	143.0
207.00	195.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

m/z	Abundance
35.90	821.0
37.00	3640.0
38.00	3520.0
39.00	1714.0
39.90	201.0
44.00	952.0
45.00	715.0
47.10	1354.0
47.90	591.0
49.00	4058.0
50.00	16864.0
51.00	5049.0
52.00	256.0
55.00	268.0
56.00	1561.0
57.00	2242.0
58.00	110.0
60.00	881.0
61.00	4237.0
62.00	4405.0
63.00	3485.0
63.90	370.0
65.00	725.0
66.90	249.0
68.00	9599.0
69.00	10052.0
70.00	853.0
72.00	527.0
73.00	4448.0
74.00	16296.0
75.00	51216.0
76.00	4366.0
76.90	720.0
77.90	457.0
78.90	2214.0
80.00	596.0
81.00	2603.0
81.90	555.0
85.90	153.0
87.00	4977.0
88.00	4805.0
90.90	345.0
92.00	2843.0
93.00	4512.0
94.00	12255.0
95.00	111568.0
96.00	7068.0
96.90	140.0
103.90	453.0
104.80	133.0
105.90	408.0
114.90	129.0
115.70	271.0
116.90	693.0
117.80	380.0
118.90	489.0
127.80	368.0
128.80	206.0
129.90	353.0
130.80	133.0
134.90	204.0
136.80	172.0
140.90	1042.0
142.00	166.0
142.90	1128.0
145.00	197.0
145.90	205.0
148.00	284.0
150.00	116.0
154.90	389.0
157.00	176.0
158.80	136.0
161.00	106.0
172.00	1402.0
173.00	1125.0
174.00	101232.0
175.00	7551.0
176.00	99288.0
177.00	6418.0
177.90	120.0
207.00	155.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

Scan 2847 (10.244 min): VU034367.D
BFB07

m/z	Abundance
39.80	165.0
43.90	774.0
207.00	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07