


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU090820\
Data File : VU040046.D
Acq On : 08 Sep 2020 10:02
Operator : SY/MD
Sample : BFB29
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB29

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Sep 10 14:05:54 2020

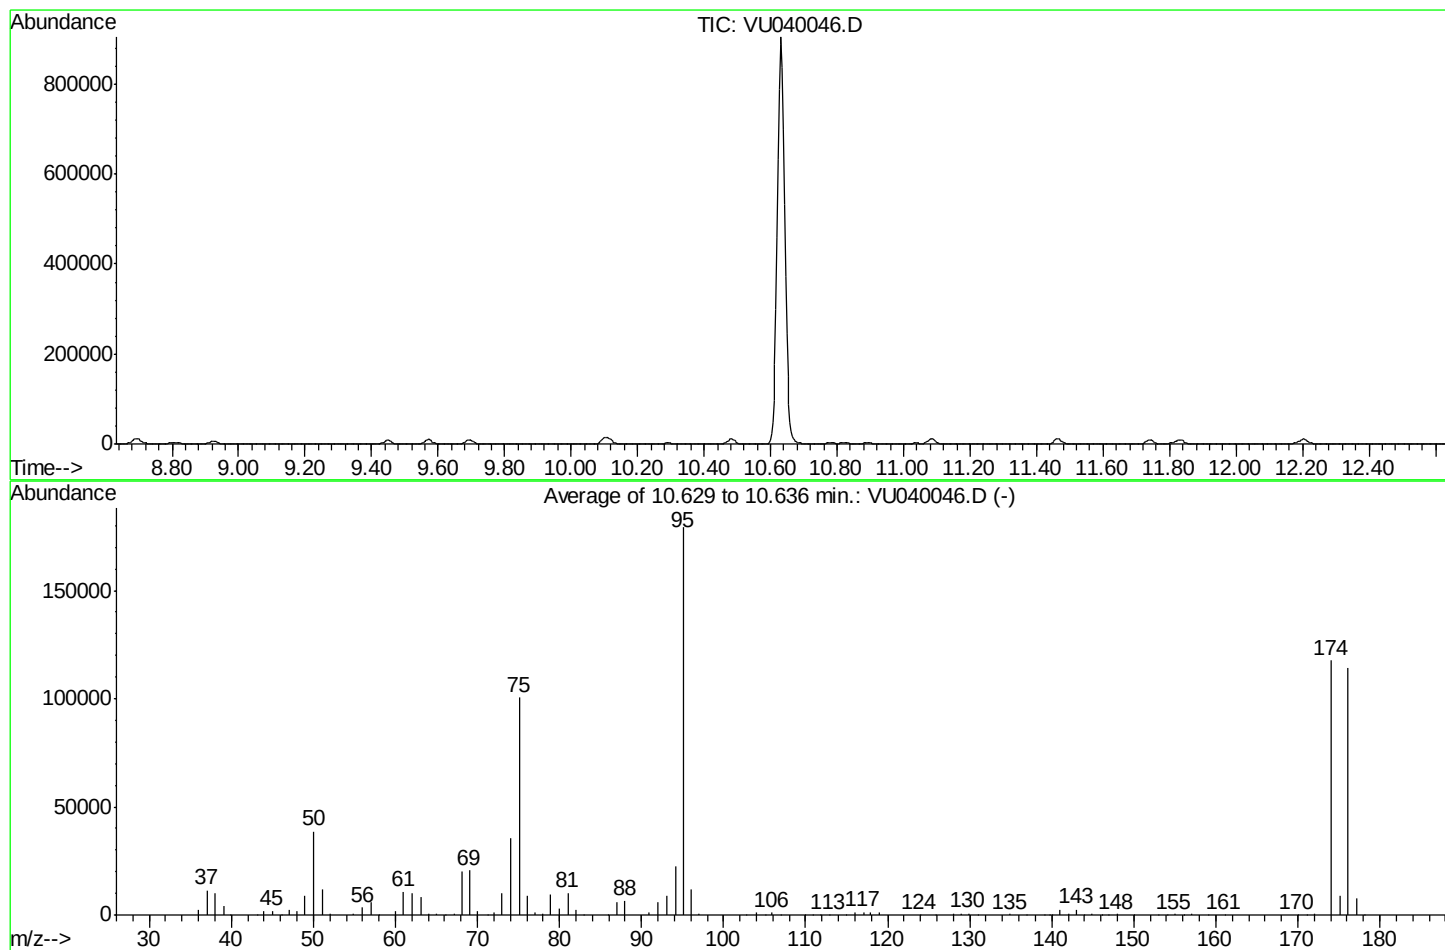

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	38669	PASS
75	95	30	80	56.0	100416	PASS
95	95	100	100	100.0	179242	PASS
96	95	5	9	6.5	11565	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	65.6	117533	PASS
175	174	5	9	7.6	8949	PASS
176	174	95	101	97.1	114069	PASS
177	176	5	9	6.6	7502	PASS

m/z	Abundance
36.00	2406.0
37.00	11939.0
38.00	10383.0
39.00	4311.0
40.00	262.0
44.00	1901.0
45.00	1801.0
46.00	292.0
47.00	2211.0
48.00	1516.0
49.00	9265.0
50.00	40024.0
51.10	12238.0
52.00	652.0
54.90	698.0
56.00	3389.0
57.00	6134.0
58.00	217.0
60.00	1959.0
61.00	10727.0
62.00	10716.0
63.10	8497.0
64.10	819.0
65.10	1014.0
66.10	193.0
67.10	781.0
68.00	20464.0
69.10	20800.0
70.00	1849.0
72.00	1223.0
73.00	10380.0
74.10	36744.0
75.10	102360.0
76.10	8913.0
77.00	1284.0
78.00	843.0
78.90	9807.0
80.00	2726.0
81.00	10201.0
82.00	2147.0
83.00	303.0
85.90	181.0
87.00	6538.0
88.00	6833.0
90.90	1036.0
92.00	6002.0
93.10	8799.0
94.10	22368.0
95.10	180864.0
96.10	11964.0
97.00	325.0
102.80	146.0
104.00	1165.0
105.00	193.0
105.90	1230.0
106.90	204.0
109.90	193.0
110.90	235.0
111.90	186.0
112.90	301.0
114.90	260.0
116.00	961.0
117.00	1469.0
117.90	963.0
119.00	1144.0
123.90	110.0
128.00	656.0
129.00	381.0
129.90	647.0
130.90	212.0
134.90	510.0
137.00	262.0
139.10	158.0
140.10	184.0
141.00	2352.0
142.10	387.0
143.10	2479.0
145.00	370.0
146.10	186.0
146.90	136.0
147.90	471.0
149.90	173.0
153.00	171.0
154.00	189.0
155.00	443.0
156.10	105.0
157.10	318.0
159.00	274.0
161.00	222.0
171.10	204.0
172.10	972.0
174.10	116680.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29

175.10	8919.0
176.10	113168.0
177.10	7465.0
178.10	156.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29

m/z	Abundance
36.00	2288.0
37.00	11620.0
38.00	10251.0
39.10	4243.0
40.00	312.0
44.00	2062.0
45.00	1832.0
46.00	268.0
47.00	2201.0
48.00	1545.0
49.00	9072.0
50.00	39664.0
51.10	11892.0
52.00	622.0
54.90	791.0
56.00	3433.0
57.00	6102.0
58.00	259.0
60.00	1909.0
61.00	11105.0
62.10	10623.0
63.10	8343.0
64.10	814.0
65.10	821.0
66.10	202.0
67.20	783.0
68.10	20648.0
69.00	21232.0
70.00	1654.0
72.00	1273.0
73.00	10754.0
74.10	37024.0
75.10	104280.0
76.10	8997.0
77.00	1247.0
78.00	792.0
79.00	9931.0
80.00	2817.0
81.00	10411.0
82.00	2336.0
83.00	331.0
87.00	6262.0
88.00	6969.0
91.00	1071.0
92.00	6012.0
93.10	9010.0
94.10	23120.0
95.10	185472.0
96.10	12035.0
97.00	320.0
102.80	136.0
104.00	1124.0
105.10	231.0
105.90	1206.0
106.90	186.0
109.90	177.0
110.90	248.0
111.90	183.0
112.90	269.0
114.90	229.0
116.00	1020.0
117.00	1529.0
117.90	979.0
118.90	1174.0
123.90	115.0
125.90	111.0
128.10	605.0
128.90	385.0
129.90	632.0
131.00	281.0
134.90	494.0
137.00	307.0
139.10	160.0
139.80	112.0
141.00	2337.0
142.10	337.0
143.10	2560.0
143.90	143.0
144.90	377.0
146.10	212.0
146.90	186.0
147.90	423.0
150.00	231.0
153.00	151.0
154.00	146.0
155.00	392.0
156.10	135.0
157.10	365.0
159.00	236.0
161.10	262.0
171.10	199.0
172.10	888.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29

174.10	121000.0
175.10	9159.0
176.10	118128.0
177.10	7746.0
178.10	133.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29

m/z	Abundance
36.00	1906.0
37.00	10432.0
38.00	9491.0
39.10	3752.0
39.90	334.0
43.10	104.0
44.00	2046.0
45.00	1737.0
46.10	200.0
47.00	2073.0
48.00	1485.0
49.00	7965.0
50.10	36320.0
51.10	10705.0
52.00	559.0
54.90	802.0
56.00	3180.0
57.00	5465.0
58.10	280.0
60.10	1733.0
61.00	10546.0
62.10	9775.0
63.00	7549.0
64.00	776.0
65.00	623.0
66.10	148.0
67.20	734.0
68.10	18920.0
69.00	19520.0
70.00	1313.0
71.20	108.0
72.00	1227.0
73.00	9634.0
74.10	33656.0
75.10	94608.0
76.10	8089.0
77.00	962.0
78.00	695.0
78.90	9271.0
80.00	2537.0
81.00	9681.0
82.00	2271.0
82.90	269.0
87.00	5722.0
88.00	6125.0
91.00	993.0
92.10	5477.0
93.00	8086.0
94.10	22112.0
95.10	171392.0
96.10	10697.0
97.00	319.0
102.80	132.0
104.00	1038.0
105.10	248.0
105.90	1058.0
106.90	139.0
109.90	172.0
110.90	222.0
111.80	179.0
112.90	224.0
114.90	208.0
116.00	887.0
117.10	1453.0
117.90	921.0
119.00	1128.0
123.90	103.0
128.10	539.0
128.90	333.0
129.90	558.0
131.00	324.0
134.90	404.0
137.00	388.0
139.00	103.0
141.00	2192.0
142.00	292.0
143.00	2389.0
143.90	179.0
144.90	306.0
146.00	198.0
146.90	186.0
148.00	371.0
150.00	267.0
153.00	103.0
154.10	112.0
155.00	338.0
156.10	106.0
157.10	322.0
159.00	183.0
161.10	257.0
170.00	112.0
171.00	180.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29

172.00	759.0
174.10	114920.0
175.10	8771.0
176.10	110912.0
177.10	7295.0
178.10	112.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29

m/z	Abundance
44.00	423.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29