

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090821\
 Data File : VU044603.D
 Acq On : 08 Sep 2021 11:57
 Operator : SY/MD
 Sample : M3596-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F3W34

Quant Time: Sep 09 07:36:44 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 09 07:35:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	111869	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	116259	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	59321	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	35167	3.887	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.800%
7) Chloroethane-d5	1.919	69	37865	4.815	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.400%
11) 1,1-Dichloroethene-d2	2.572	65	15819	4.110	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.200%
20) 2-Butanone-d5	4.642	46	106122	42.411	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	84.820%
24) Chloroform-d	5.073	84	72053	4.504	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.000%
26) 1,2-Dichloroethane-d4	5.710	65	40066	4.592	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.800%
32) Benzene-d6	5.735	84	146393	4.472	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.400%
36) 1,2-Dichloropropane-d6	6.697	67	45478	4.342	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.800%
41) Toluene-d8	7.903	98	130852	4.508	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.200%
43) trans-1,3-Dichloroprop...	8.185	79	15291	4.065	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.400%
46) 2-Hexanone-d5	8.642	63	94368	46.396	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.800%
56) 1,1,2,2-Tetrachloroeth...	10.761	84	40035	4.539	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.800%
66) 1,2-Dichlorobenzene-d4	12.198	152	51502	5.139	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.800%
Target Compounds					Qvalue	
13) Acetone	2.649	43	23701	11.407	ug/L	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090821\
Data File : VU044603.D
Acq On : 08 Sep 2021 11:57
Operator : SY/MD
Sample : M3596-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F3W34

Quant Time: Sep 09 07:36:44 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 09 07:35:45 2021
Response via : Initial Calibration

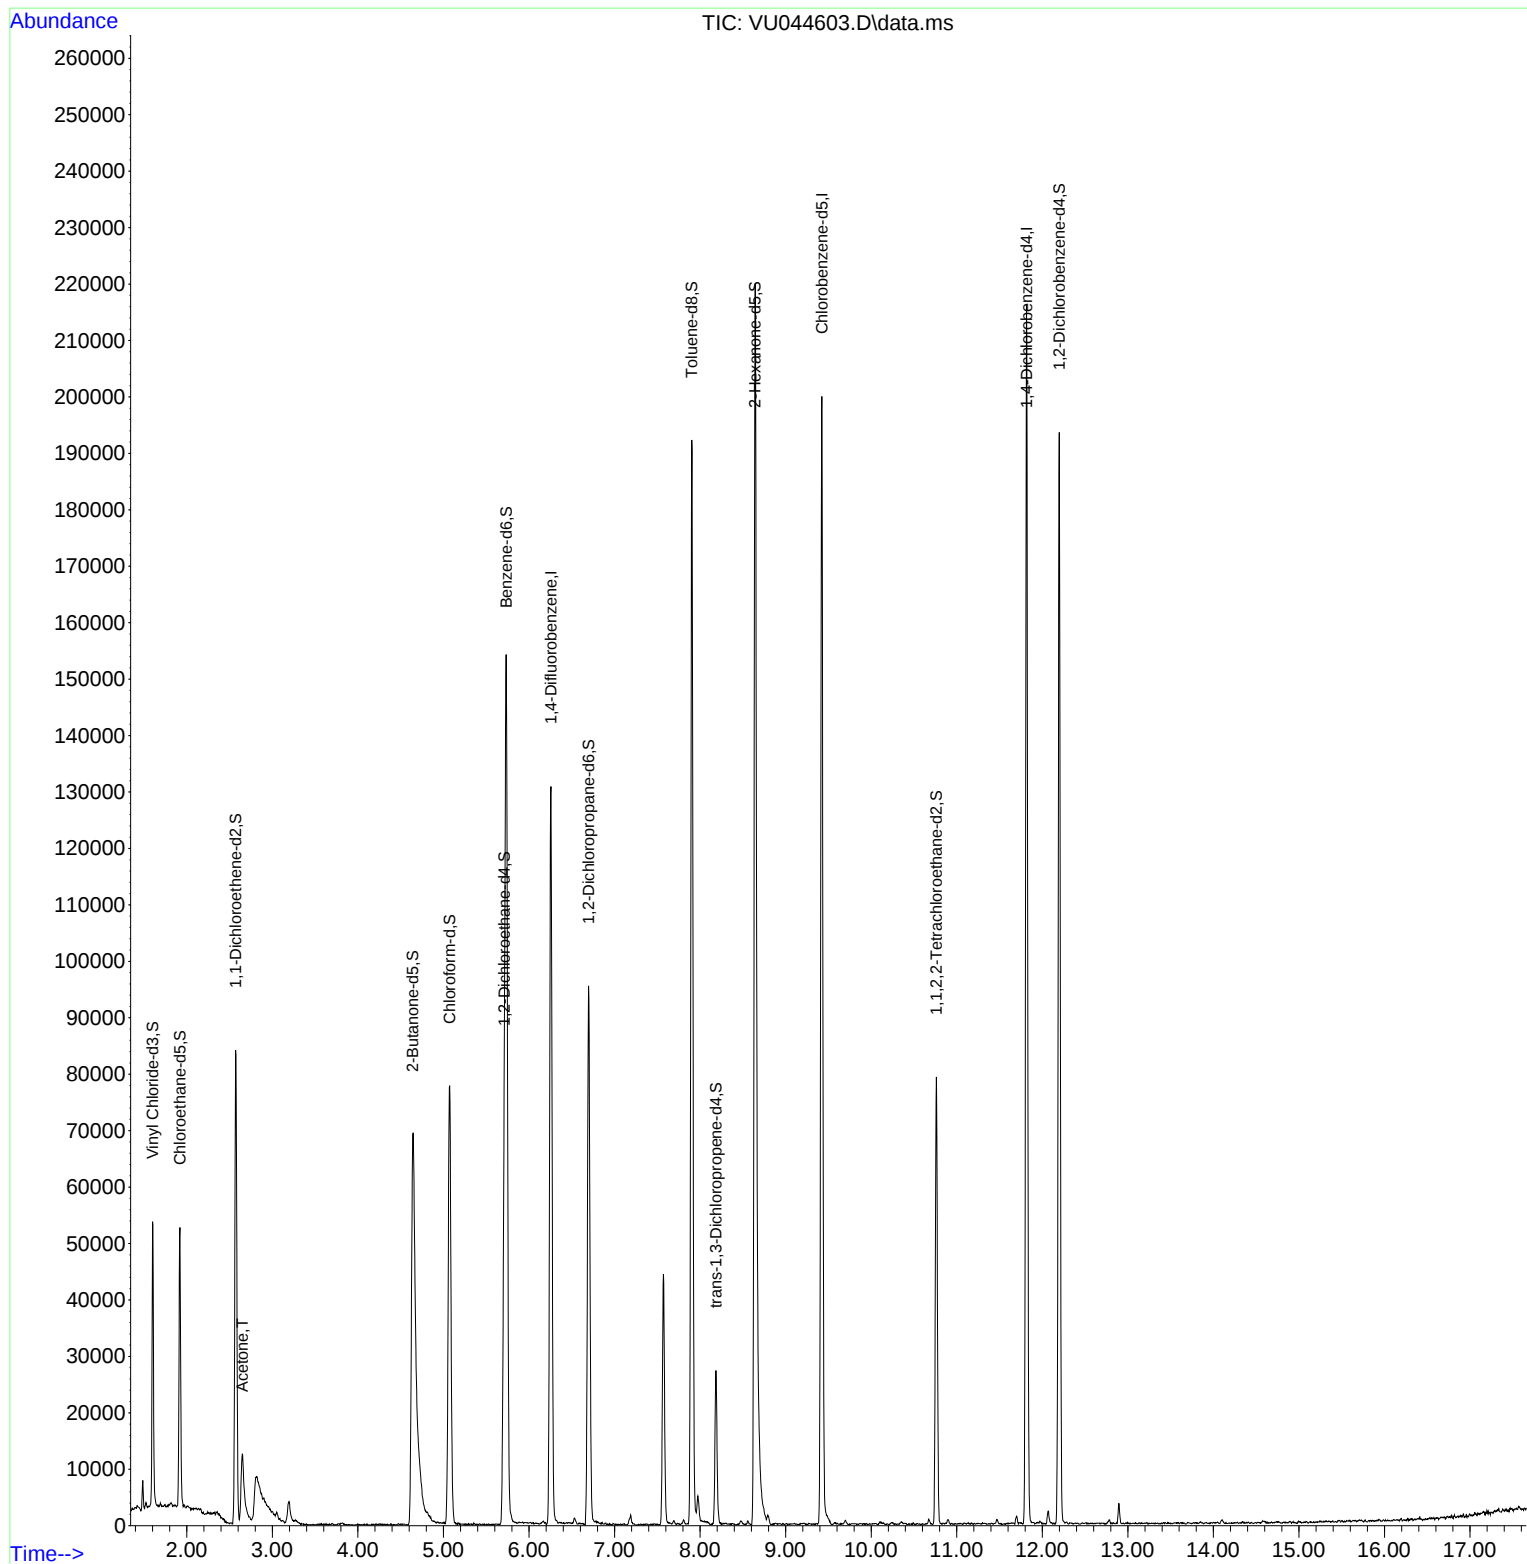

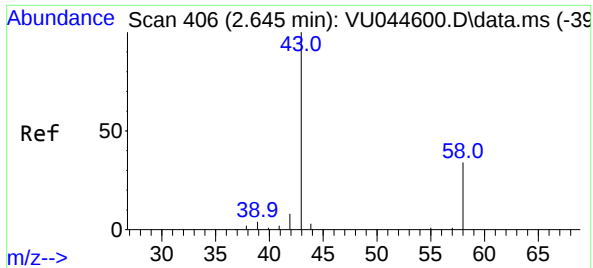

#13
Acetone
Concen: 11.407 ug/L
RT: 2.649 min Scan# 407
Delta R.T. 0.003 min
Lab File: VU044603.D
Acq: 08 Sep 2021 11:57

Instrument :
MSVOA_U
ClientSampleId :
F3W34

Tgt Ion: 43 Resp: 23701
Ion Ratio Lower Upper
43 100
58 33.4 0.0 45.4

