

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090821\
 Data File : VU044606.D
 Acq On : 08 Sep 2021 13:09
 Operator : SY/MD
 Sample : M3596-12
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Quant Time: Sep 09 07:37:23 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 09 07:35:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	112647	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	116173	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	58708	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	35511	3.898	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.000%
7) Chloroethane-d5	1.919	69	36892	4.659	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.200%
11) 1,1-Dichloroethene-d2	2.572	65	15994	4.127	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.600%
20) 2-Butanone-d5	4.642	46	111114	44.099	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	88.200%
24) Chloroform-d	5.073	84	70231	4.360	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.200%
26) 1,2-Dichloroethane-d4	5.710	65	41067	4.675	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.400%
32) Benzene-d6	5.735	84	149815	4.580	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.600%
36) 1,2-Dichloropropane-d6	6.697	67	46337	4.428	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.600%
41) Toluene-d8	7.903	98	130137	4.486	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.800%
43) trans-1,3-Dichloroprop...	8.185	79	15603	4.151	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.000%
46) 2-Hexanone-d5	8.645	63	96568	47.513	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.020%
56) 1,1,2,2-Tetrachloroeth...	10.761	84	41281	4.683	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.600%
66) 1,2-Dichlorobenzene-d4	12.198	152	52175	5.260	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.200%
Target Compounds						Qvalue
16) Methylene chloride	3.054	84	10465	0.814	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090821\
Data File : VU044606.D
Acq On : 08 Sep 2021 13:09
Operator : SY/MD
Sample : M3596-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Time: Sep 09 07:37:23 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 09 07:35:45 2021
Response via : Initial Calibration

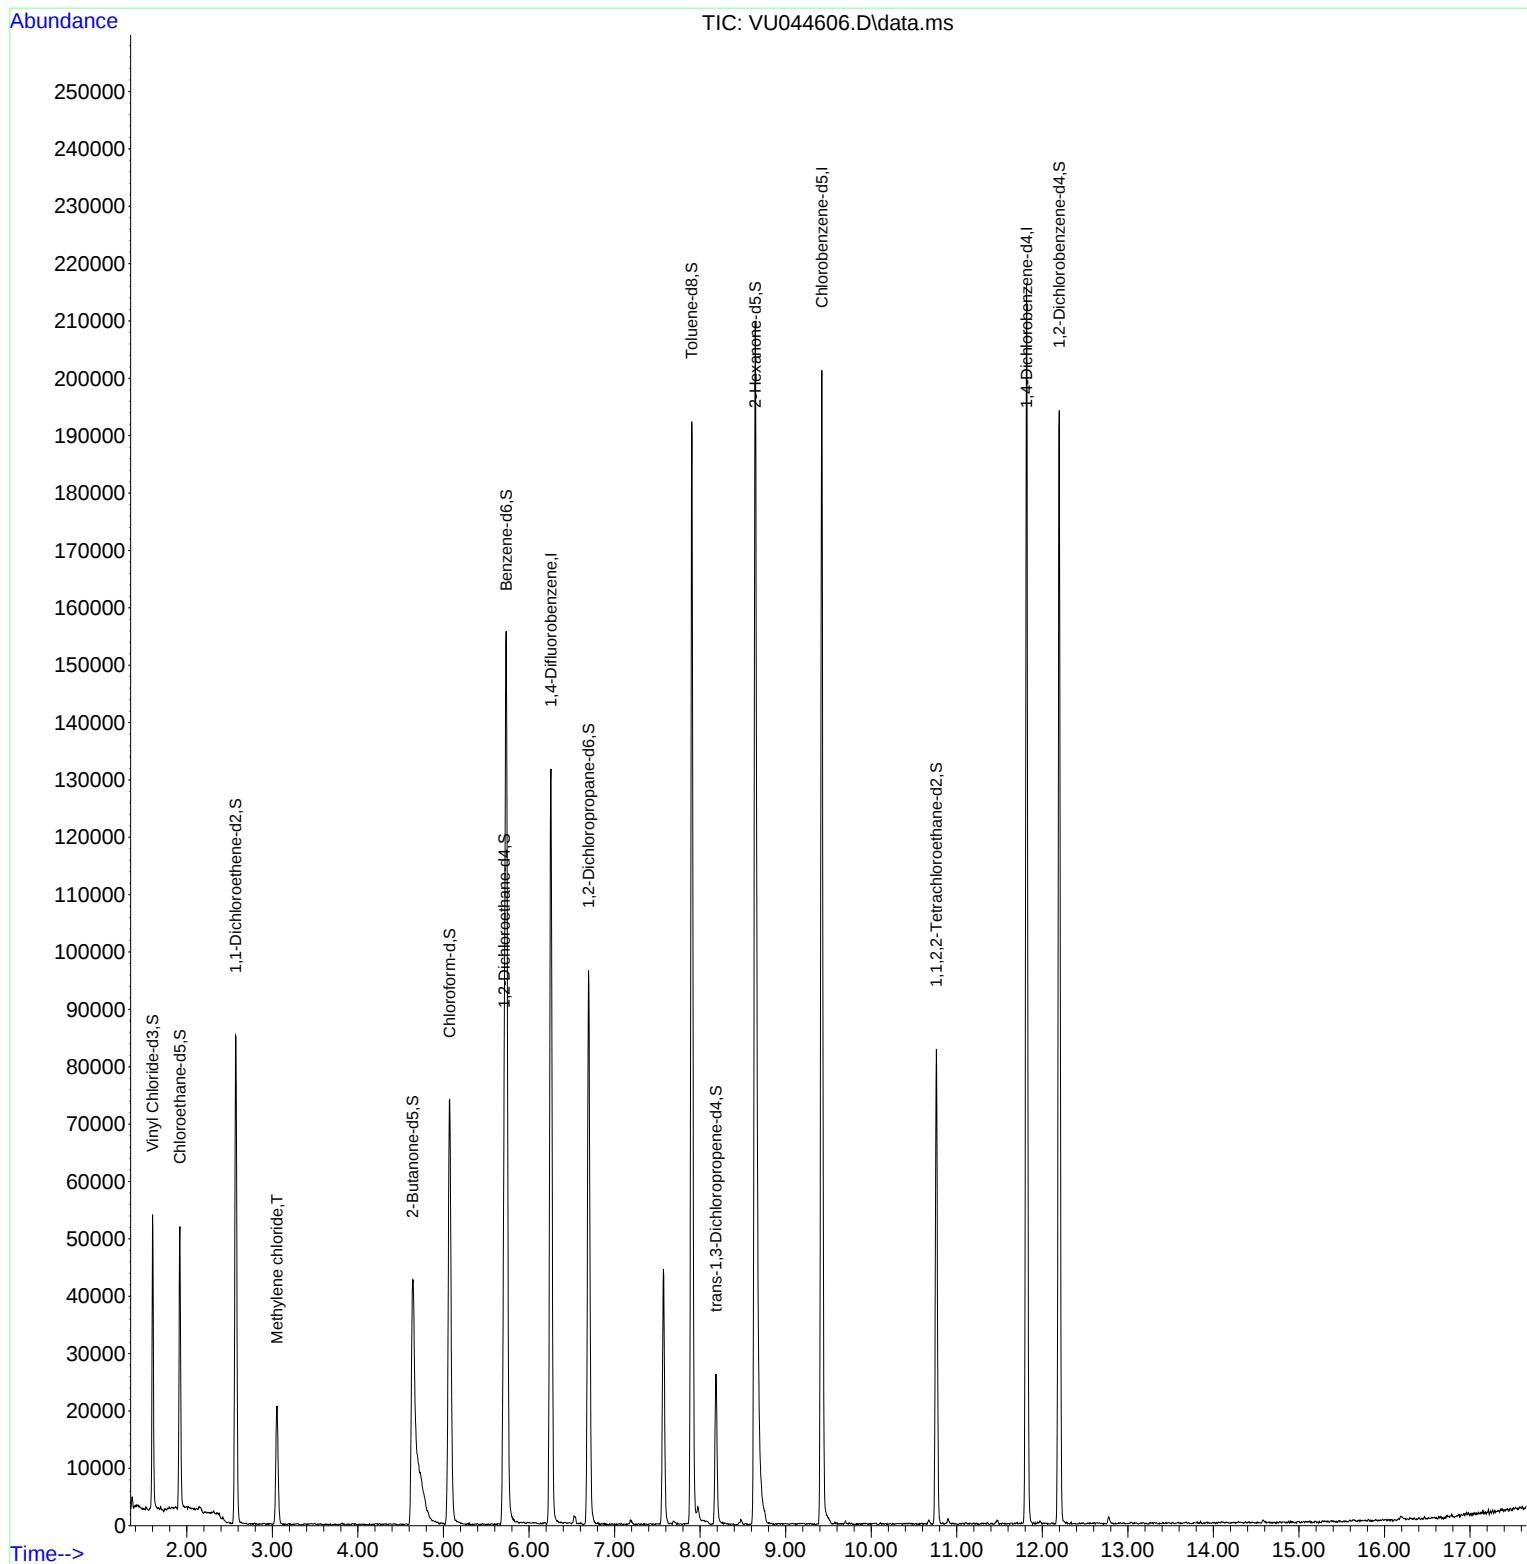

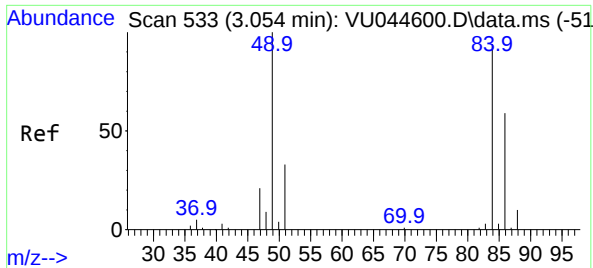

#16
Methylene chloride
Concen: 0.814 ug/L
RT: 3.054 min Scan# 533
Delta R.T. 0.000 min
Lab File: VU044606.D
Acq: 08 Sep 2021 13:09

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Tgt Ion:	84	Resp:	10465
Ion	Ratio	Lower	Upper
84	100		
86	69.2	45.2	84.0
49	112.1	88.8	165.0

