

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090821\
 Data File : VU044603.D
 Acq On : 08 Sep 2021 11:57
 Operator : SY/MD
 Sample : M3596-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F3W34

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU044603.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	39	45	51	rBV	5405	5238	1.13%	0.143%
2	1.601	73	81	97	rVB	50270	58326	12.53%	1.592%
3	1.919	171	180	192	rVB	49370	64533	13.86%	1.762%
4	2.572	371	383	396	rBV	83984	135676	29.14%	3.704%
5	2.649	396	407	430	rVV	11684	30862	6.63%	0.843%
6	2.819	441	460	475	rBV3	7679	32503	6.98%	0.887%
7	3.195	564	577	590	rBV	3623	8314	1.79%	0.227%
8	4.645	1011	1028	1073	rBV2	69462	261838	56.24%	7.148%
9	5.073	1145	1161	1179	rBV	77617	174800	37.55%	4.772%
10	5.732	1344	1366	1390	rBV2	154211	399514	85.81%	10.906%
11	6.256	1512	1529	1547	rBV	130841	250998	53.91%	6.852%
12	6.697	1653	1666	1687	rBV	95514	188457	40.48%	5.145%
13	7.571	1925	1938	1957	rBV	44474	77783	16.71%	2.123%
14	7.903	2028	2041	2057	rBV	192065	333612	71.66%	9.107%
15	7.973	2058	2063	2074	rVB3	4485	7179	1.54%	0.196%
16	8.186	2118	2129	2143	rBV2	27140	44800	9.62%	1.223%
17	8.645	2258	2272	2312	rBV	219920	465570	100.00%	12.710%
18	9.423	2499	2514	2531	rBV	199821	335215	72.00%	9.151%
19	10.761	2915	2930	2946	rBV	79295	128527	27.61%	3.509%
20	11.816	3243	3258	3277	rBV	216026	346814	74.49%	9.468%
21	12.198	3363	3377	3397	rBV	193344	312532	67.13%	8.532%




Sum of corrected areas: 3663091

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090821\
Data File : VU044603.D
Acq On : 08 Sep 2021 11:57
Operator : SY/MD
Sample : M3596-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F3W34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

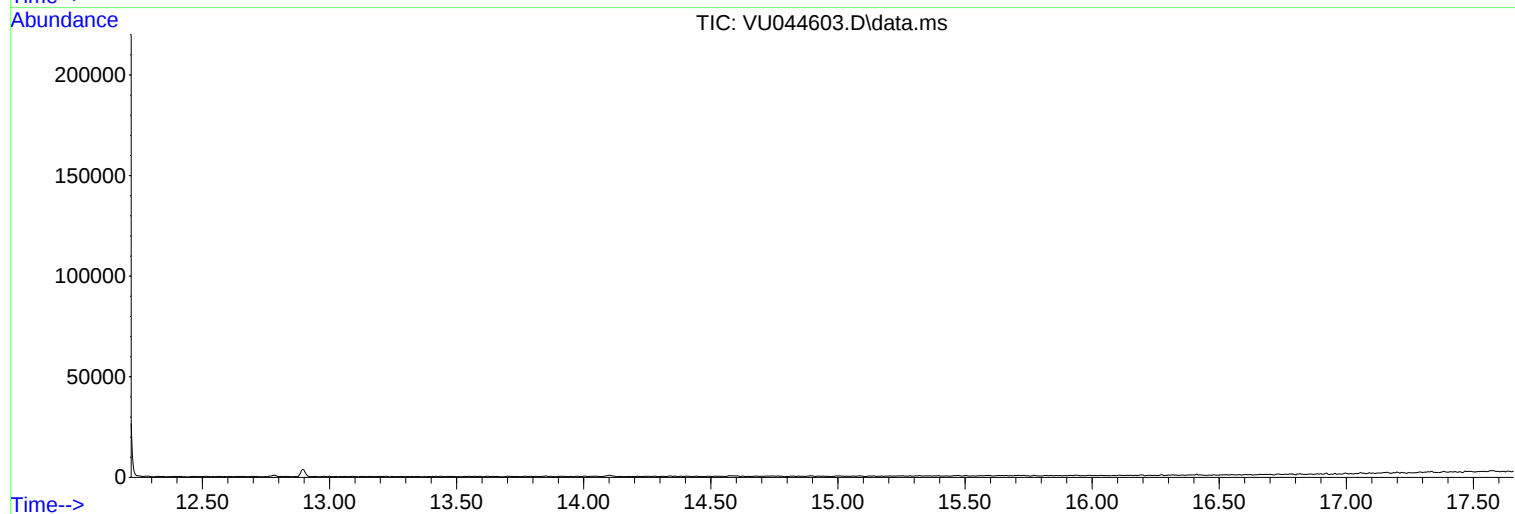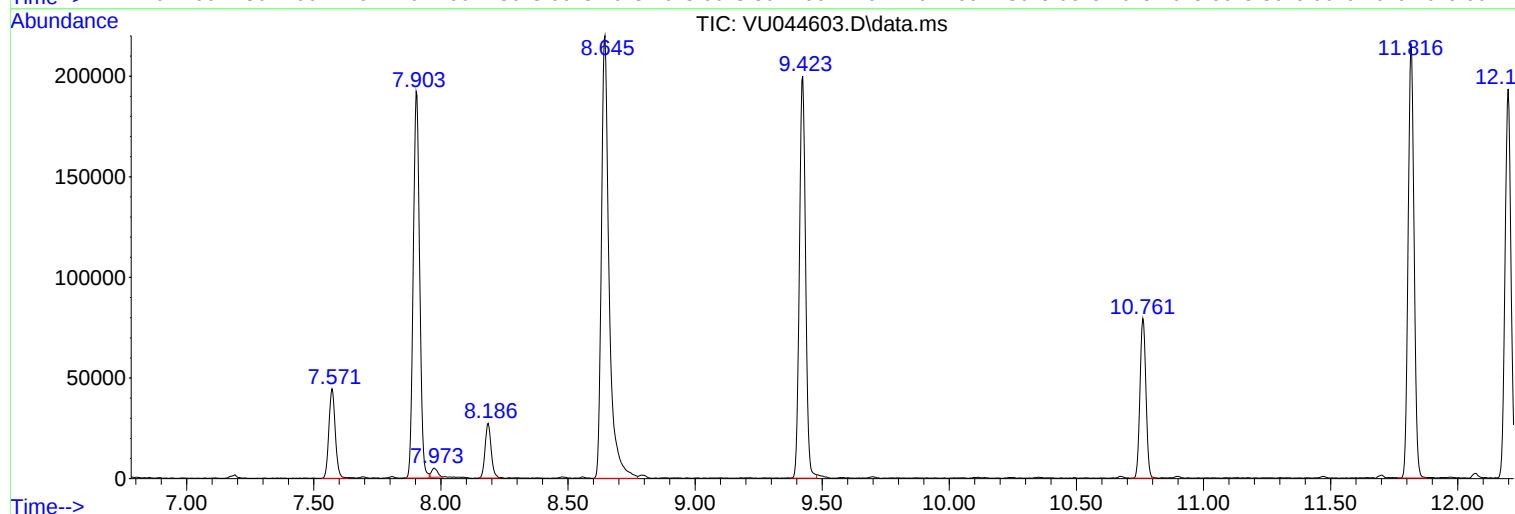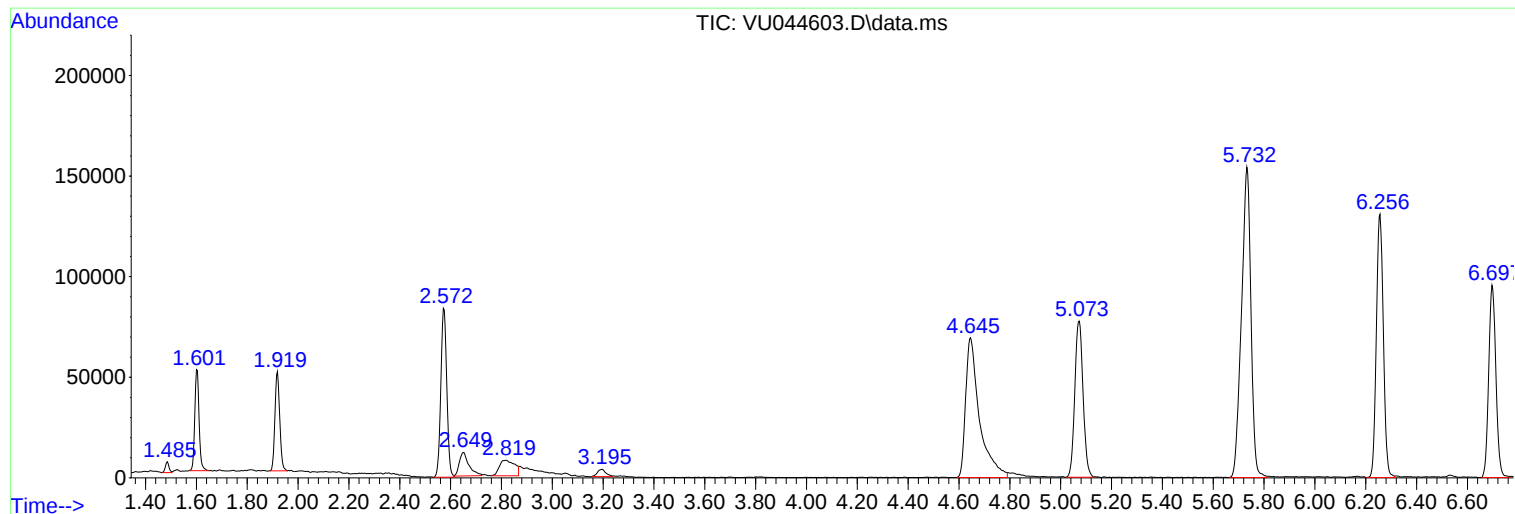

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090821\
Data File : VU044603.D
Acq On : 08 Sep 2021 11:57
Operator : SY/MD
Sample : M3596-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F3W34










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.819	0.65 ug/L	32503	1,4-Difluorobenzene	6.256

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	56
3			2-Pentanol	88	C5H12O	006032-29-7	9
4			4-Penten-2-ol	86	C5H10O	000625-31-0	9
5			Propane, 2-ethoxy-	88	C5H12O	000625-54-7	9

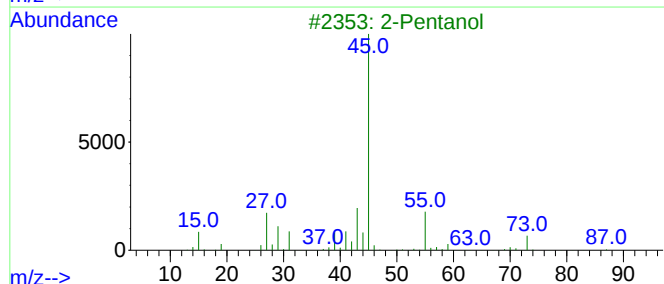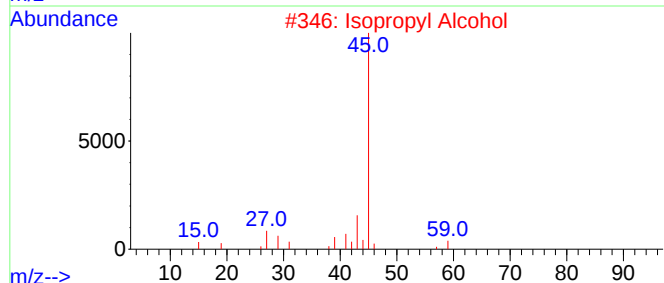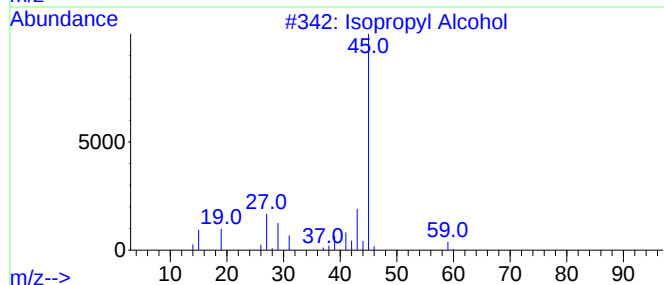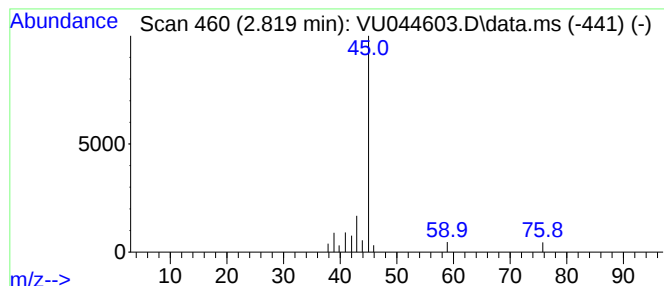

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090821\
Data File : VU044603.D
Acq On : 08 Sep 2021 11:57
Operator : SY/MD
Sample : M3596-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F3W34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.819	0.7	ug/L	32503	1	6.256	250998	5.0