
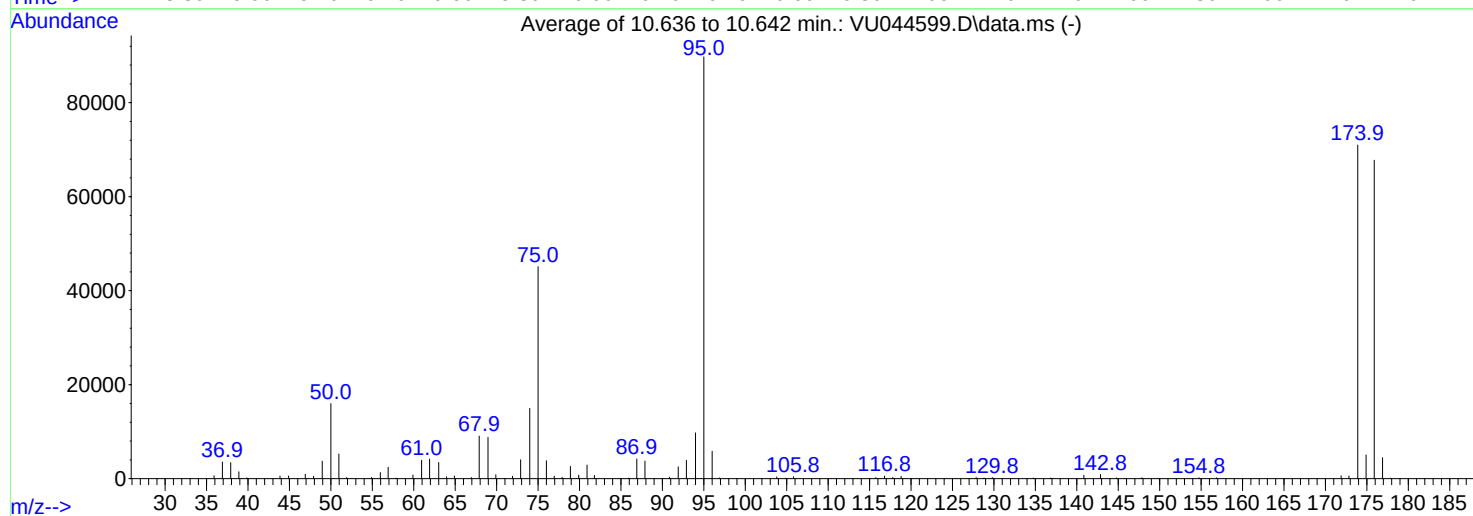


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090821\
 Data File : VU044599.D
 Acq On : 08 Sep 2021 09:18
 Operator : SY/MD
 Sample : BFB014
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB014

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Sep 09 07:35:45 2021

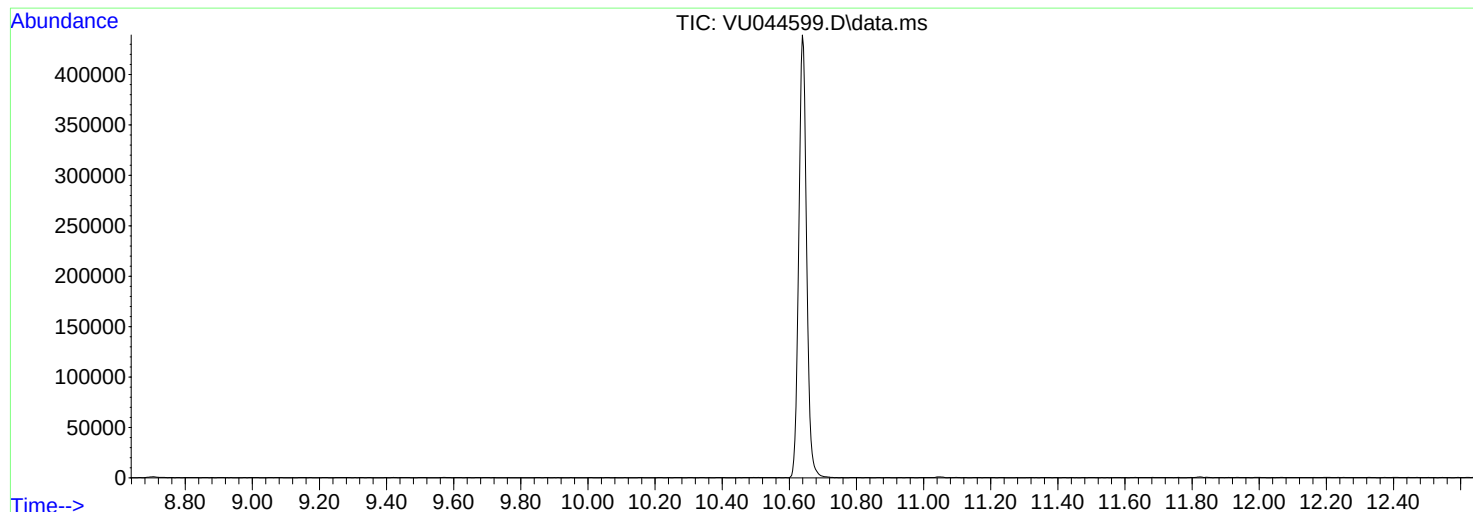

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	15965	PASS
75	95	30	80	50.3	45123	PASS
95	95	100	100	100.0	89752	PASS
96	95	5	9	6.5	5837	PASS
173	174	0.00	2	0.8	587	PASS
174	95	50	120	79.1	70989	PASS
175	174	5	9	7.1	5025	PASS
176	174	95	101	95.5	67765	PASS
177	176	5	9	6.6	4474	PASS

m/z	Abundance
35.90	635.0
36.90	3517.0
37.90	3247.0
38.90	1486.0
39.80	153.0
43.90	760.0
44.90	598.0
46.90	973.0
47.90	468.0
49.00	3820.0
50.00	15652.0
50.90	5132.0
51.90	251.0
54.90	243.0
55.90	1248.0
56.90	2386.0
57.90	115.0
59.90	751.0
61.00	3865.0
61.90	4123.0
63.00	3358.0
64.00	371.0
64.90	581.0
67.00	236.0
67.90	8684.0
68.90	8748.0
69.90	789.0
71.90	494.0
72.90	3866.0
74.00	14419.0
75.00	43992.0
76.00	3803.0
76.90	552.0
77.90	277.0
78.90	2520.0
79.90	722.0
80.90	2856.0
81.80	691.0
85.90	126.0
86.90	4154.0
87.90	3635.0
90.80	318.0
91.90	2369.0
92.90	3774.0
94.00	9710.0
95.00	86800.0
96.00	5700.0
96.90	214.0
103.80	379.0
104.70	100.0
105.80	404.0
115.70	248.0
116.80	530.0
117.80	303.0
118.80	480.0
127.80	189.0
128.80	147.0
129.80	265.0
134.80	114.0
136.80	123.0
140.80	690.0
142.80	881.0
144.80	136.0
145.80	120.0
147.90	220.0
154.70	174.0
156.90	200.0
171.90	693.0
172.80	589.0
173.90	66896.0
174.90	4922.0
175.90	63816.0
176.90	4171.0
177.90	154.0

Instrument :
MSVOA_U
ClientSampleId :
BFB014

m/z	Abundance
43.80	221.0

Instrument :
MSVOA_U
ClientSampleId :
BFB014

m/z	Abundance
35.90	600.0
36.90	3472.0
37.90	3445.0
38.90	1427.0
39.90	171.0
43.90	790.0
44.90	579.0
46.90	899.0
47.90	535.0
48.90	3495.0
50.00	15804.0
51.00	5210.0
51.90	223.0
54.90	244.0
56.00	1296.0
56.90	2361.0
57.80	104.0
59.90	789.0
60.90	3889.0
61.90	4094.0
63.00	3374.0
63.90	443.0
64.90	571.0
66.90	200.0
67.90	9142.0
68.90	8528.0
69.90	789.0
71.90	479.0
72.90	4012.0
74.00	15060.0
75.00	44688.0
76.00	3689.0
77.00	544.0
77.90	336.0
78.90	2606.0
79.90	782.0
80.90	2809.0
81.80	658.0
85.90	104.0
86.90	4032.0
87.90	3656.0
90.90	272.0
91.90	2595.0
92.90	3846.0
94.00	9501.0
95.00	89920.0
96.00	5813.0
96.90	148.0
103.80	350.0
104.90	123.0
105.80	395.0
115.80	256.0
116.80	535.0
117.80	271.0
118.80	442.0
127.90	282.0
128.80	138.0
129.80	242.0
134.70	162.0
136.90	157.0
140.90	755.0
142.90	880.0
144.80	171.0
147.80	212.0
149.80	112.0
154.80	232.0
156.80	174.0
171.90	578.0
172.90	573.0
173.90	72656.0
174.90	4979.0
175.90	69568.0
176.90	4640.0

Instrument :
MSVOA_U
ClientSampleId :
BFB014

m/z	Abundance
35.90	653.0
36.90	3636.0
37.90	3513.0
38.90	1504.0
39.80	163.0
43.90	795.0
44.90	614.0
46.90	1005.0
47.90	541.0
48.90	3853.0
50.00	16440.0
51.00	5417.0
51.90	255.0
54.90	254.0
55.90	1297.0
56.90	2476.0
57.90	116.0
59.90	828.0
61.00	4028.0
61.90	4280.0
63.00	3550.0
63.90	428.0
64.90	590.0
67.00	245.0
67.90	9326.0
69.00	9033.0
69.90	841.0
71.90	540.0
72.90	4159.0
74.00	15384.0
75.00	46688.0
76.00	3962.0
77.00	572.0
77.90	302.0
78.90	2674.0
79.90	768.0
80.90	2981.0
81.80	732.0
85.90	127.0
86.90	4354.0
87.90	3930.0
90.90	288.0
91.90	2590.0
92.90	4045.0
94.00	10050.0
95.00	92536.0
96.00	5999.0
96.90	187.0
103.80	405.0
104.80	126.0
105.80	403.0
115.80	271.0
116.80	542.0
117.80	297.0
118.80	497.0
127.80	235.0
128.80	151.0
129.80	261.0
134.70	141.0
136.90	146.0
140.80	722.0
142.90	944.0
144.80	165.0
145.80	121.0
147.80	236.0
149.80	105.0
154.80	214.0
156.90	193.0
171.90	616.0
172.90	600.0
173.90	73416.0
174.90	5175.0
175.90	69912.0
176.90	4612.0
177.90	123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB014