



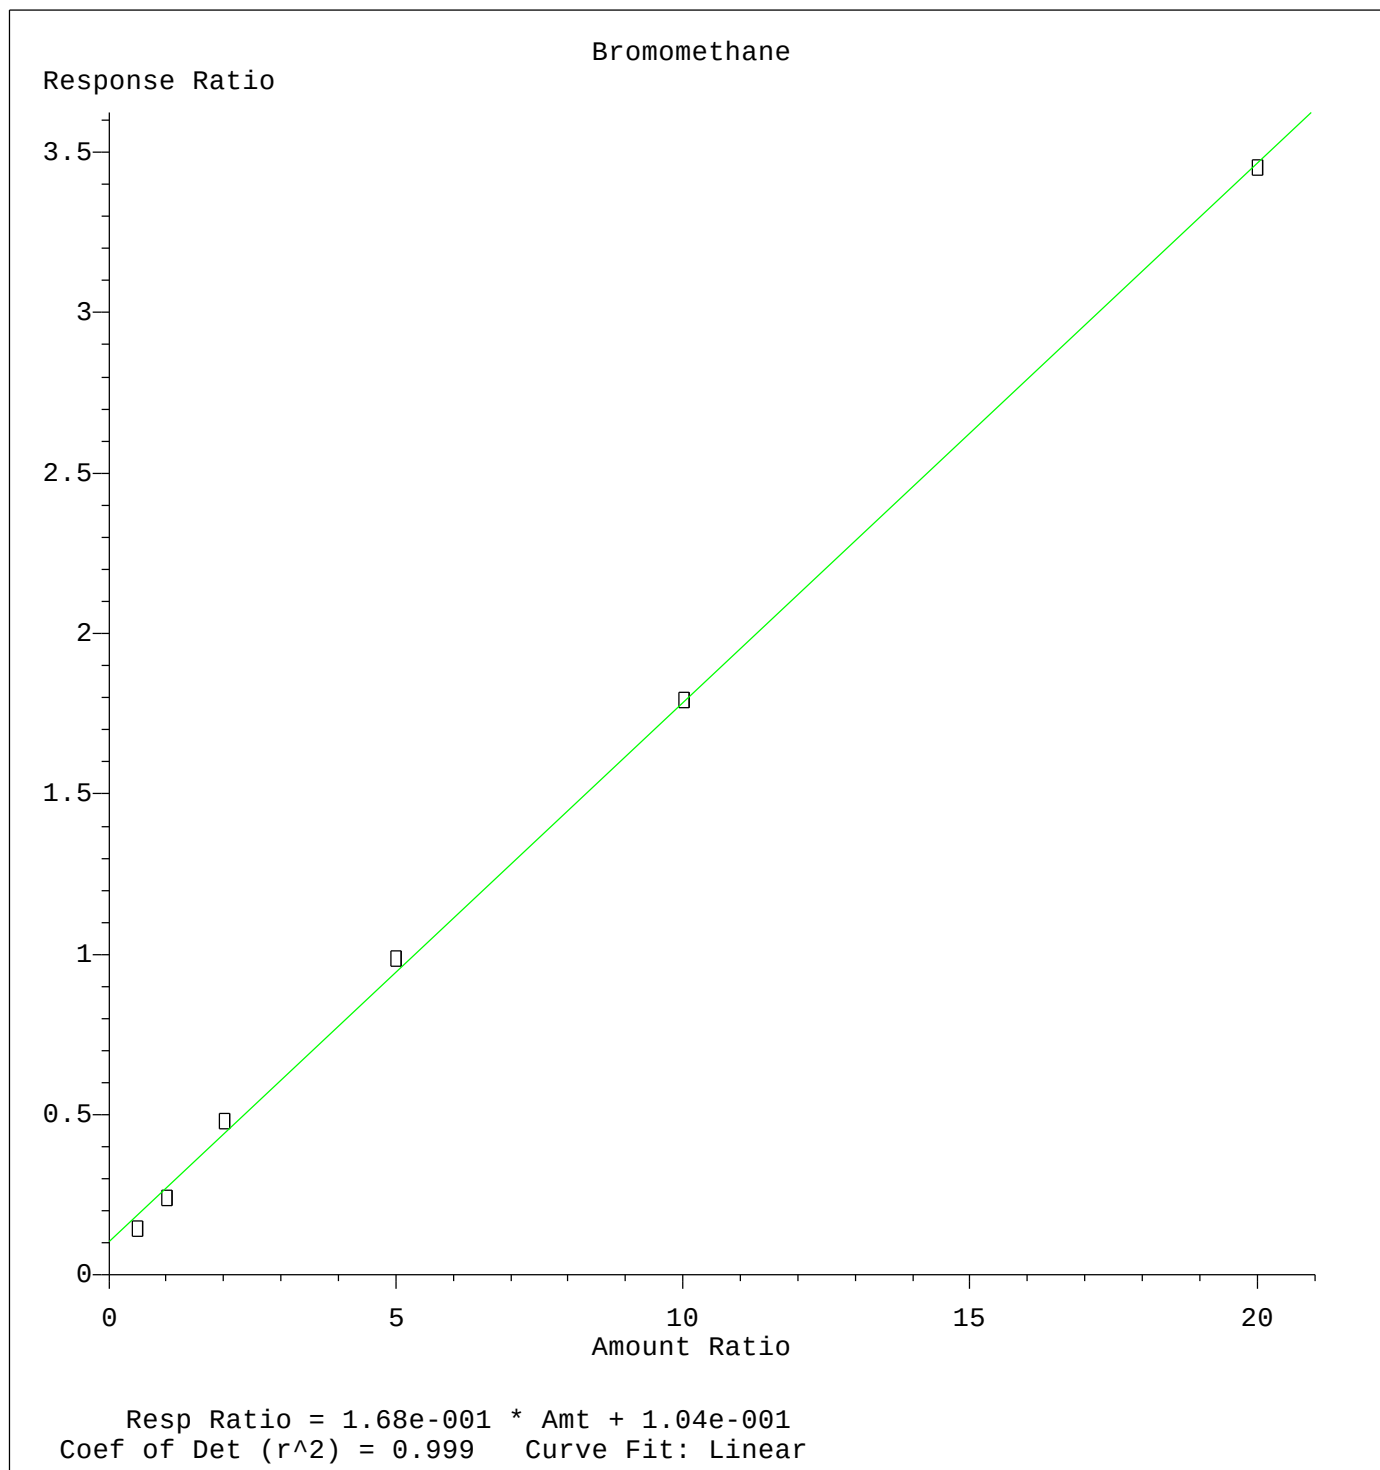

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U090920DW.M
Calibration Table Last Updated: Fri Sep 11 12:52:59 2020

Iodomethane

Response Ratio

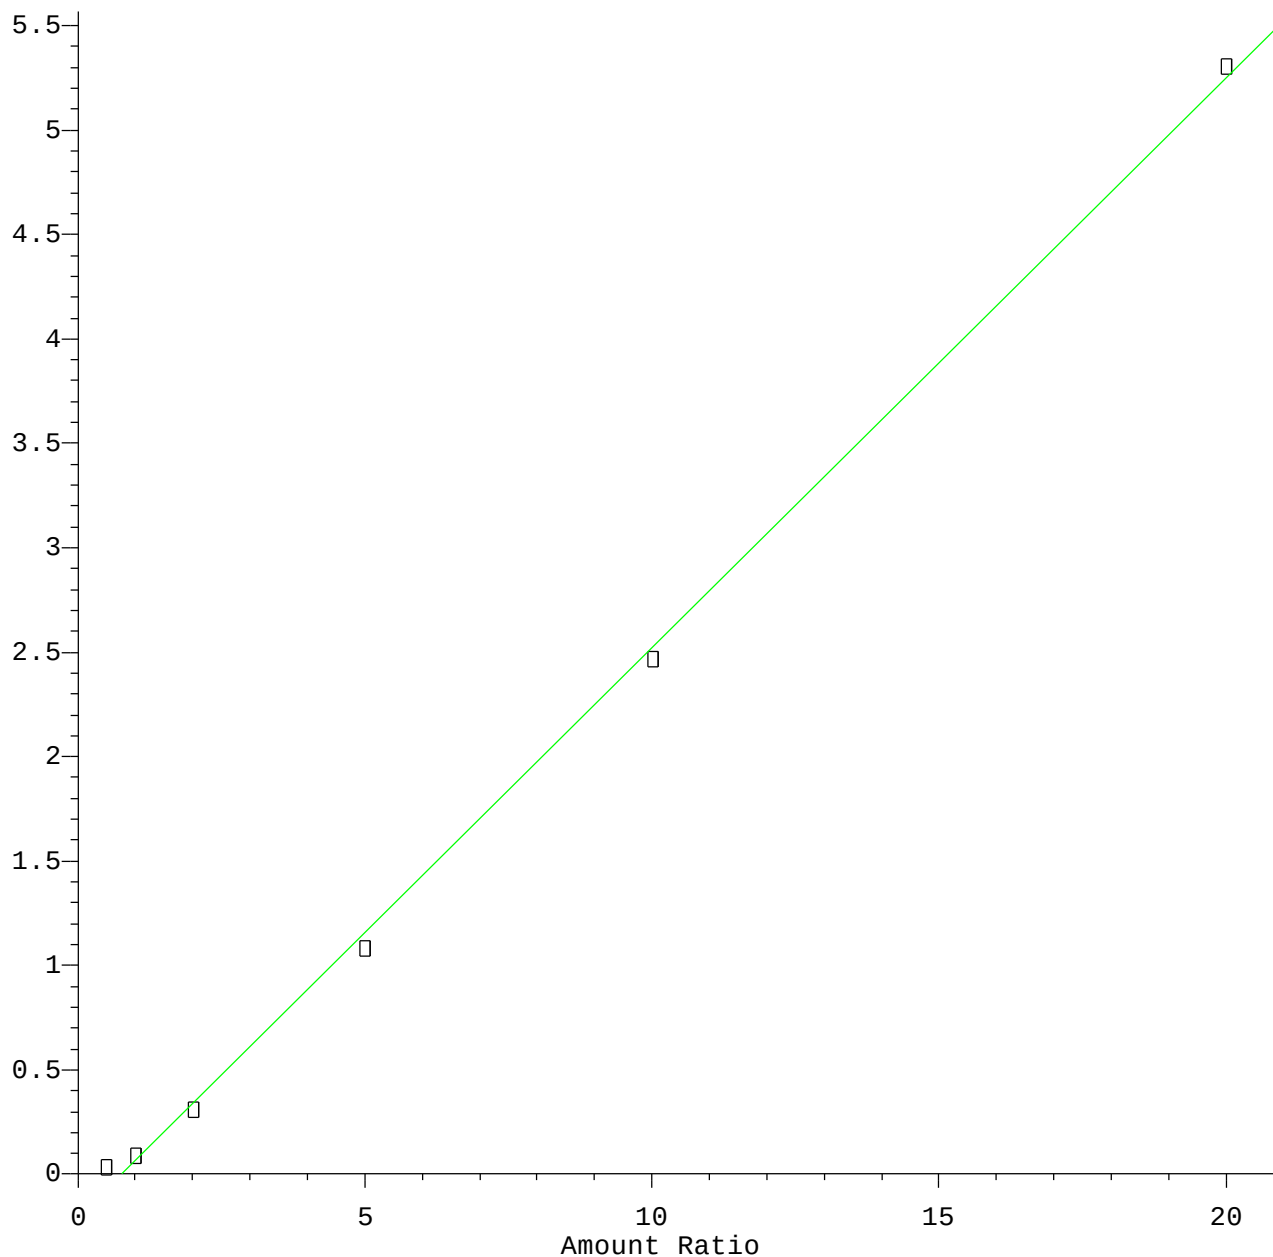


Resp Ratio = $2.73 \times 10^{-1} \times \text{Amt} - 2.06 \times 10^{-1}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U090920DW.M
Calibration Table Last Updated: Fri Sep 11 12:52:59 2020

Methylene Chloride

Response Ratio

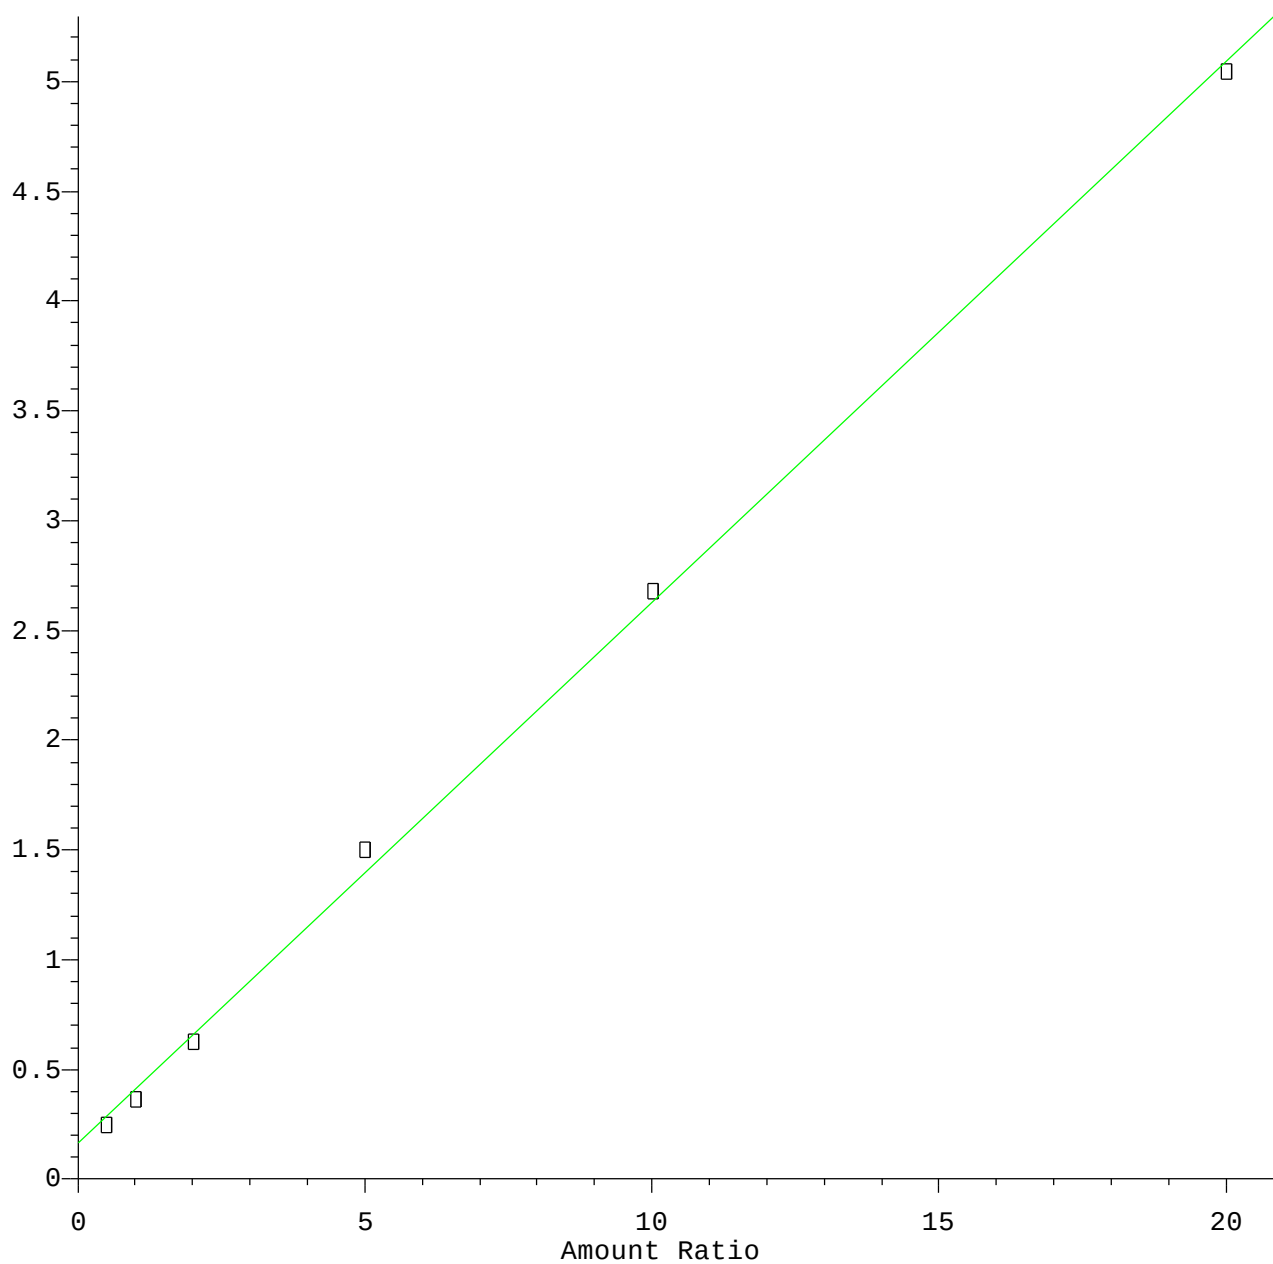

Resp Ratio = $2.46 \times 10^{-1} \times \text{Amt} + 1.61 \times 10^{-1}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U090920DW.M
Calibration Table Last Updated: Fri Sep 11 12:52:59 2020