

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090920\
Data File : VU040065.D
Acq On : 09 Sep 2020 14:58
Operator : SY/MD
Sample : VU0909WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0909WBL01

Quant Time: Sep 10 04:25:39 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U090920DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Sep 10 04:09:54 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene	6.13	96	28109	1.00	ug/l	0.00

System Monitoring Compounds

57) 4-Bromofluorobenzene	10.63	95	9245	0.81	ug/l	0.00
Spiked Amount	1.000		Recovery	=	81.00%	
68) 1,2-Dichlorobenzene-d4	12.19	152	8931	0.85	ug/l	0.00
Spiked Amount	1.000		Recovery	=	85.00%	


Target Compounds	Ovalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU090920\
Data File : VU040065.D
Acq On : 09 Sep 2020 14:58
Operator : SY/MD
Sample : VU0909WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0909WBL01

Quant Time: Sep 10 04:25:39 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U090920DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Sep 10 04:09:54 2020
Response via : Initial Calibration

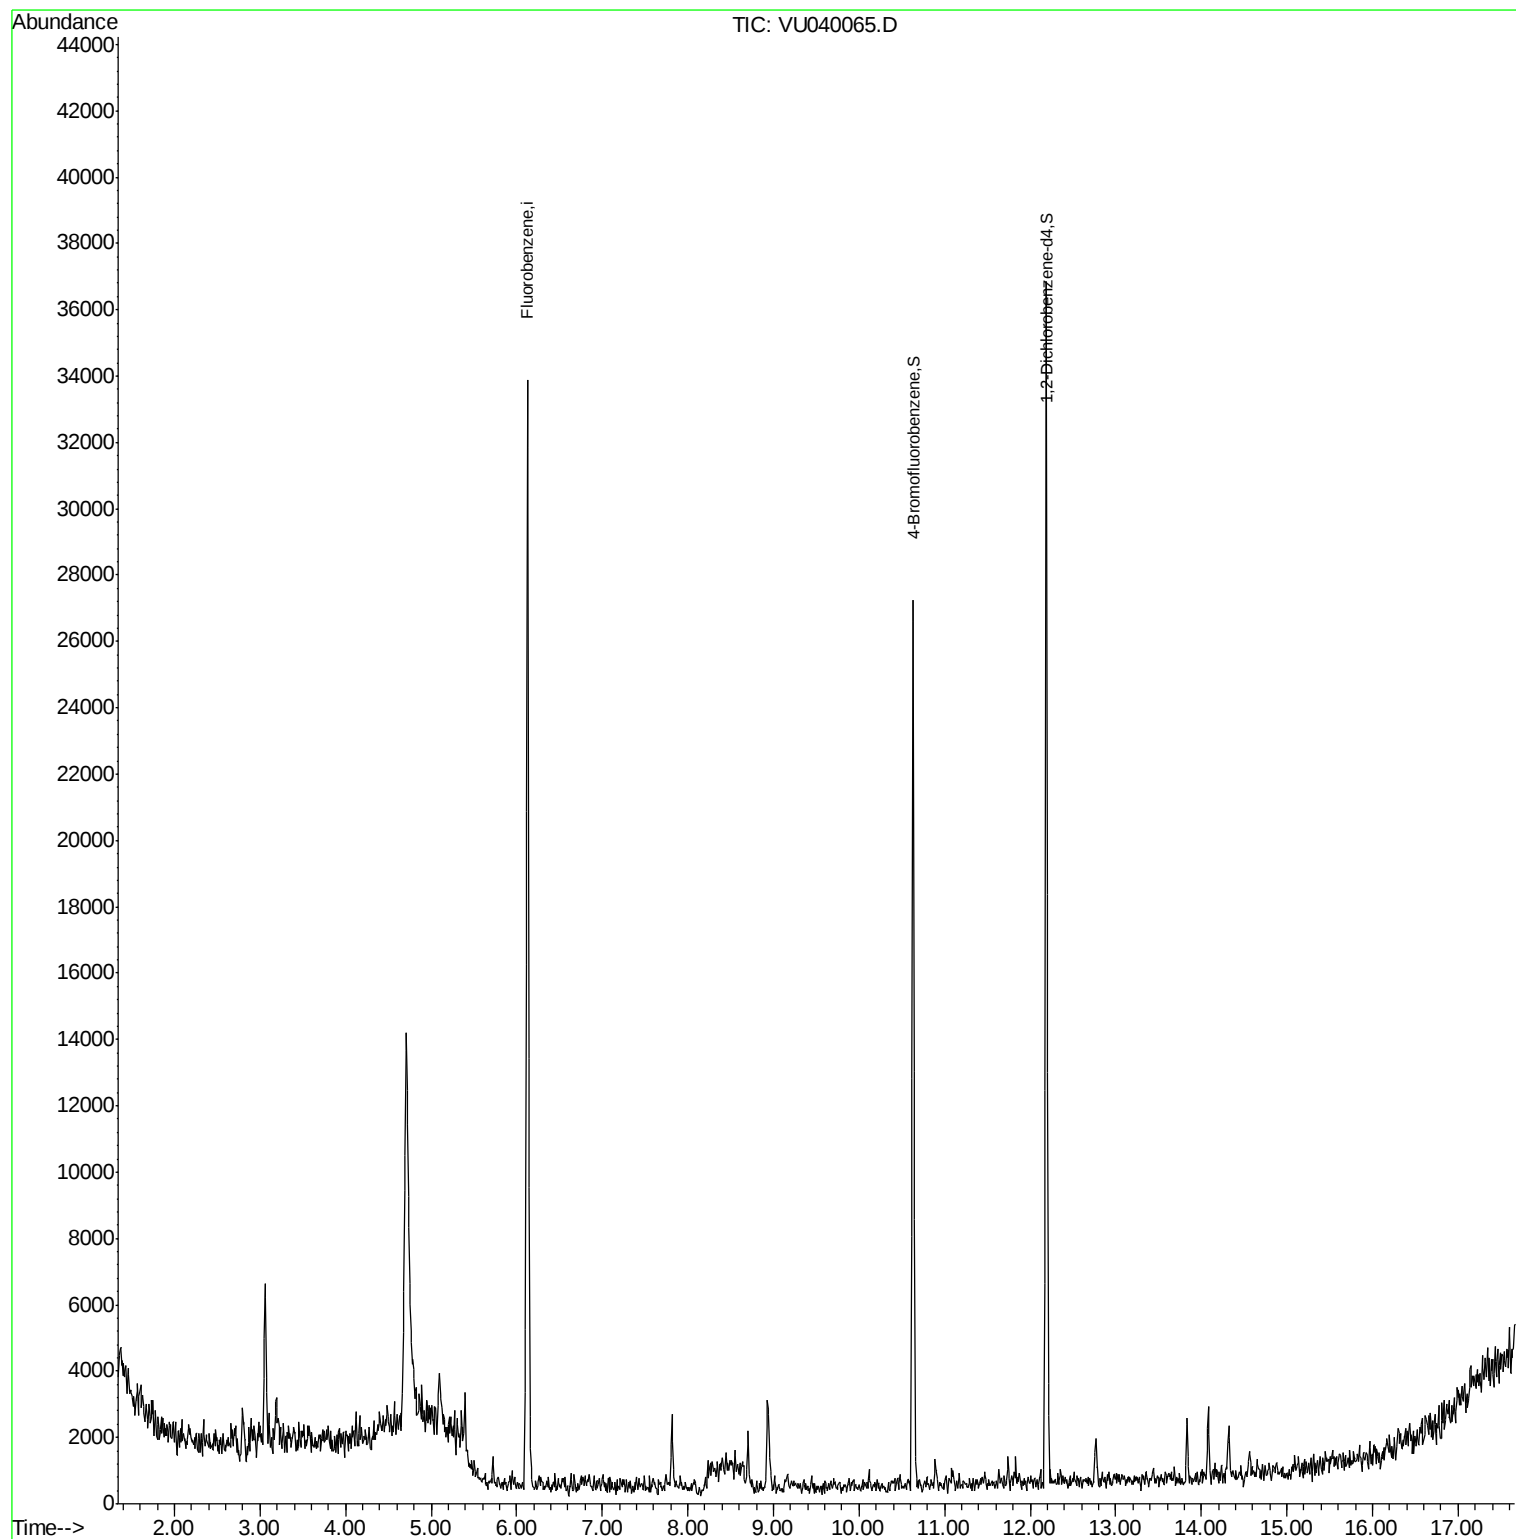

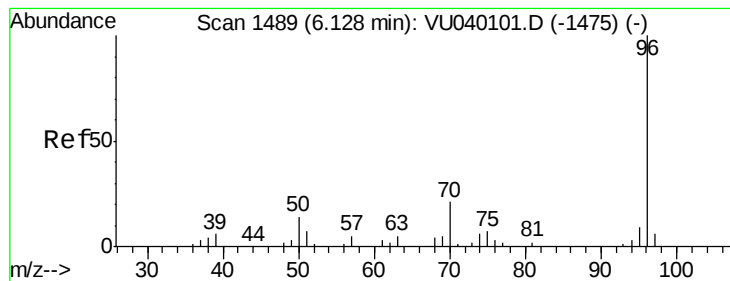

#1

Fluorobenzene

Concen: 1.000 ug/l

RT: 6.13 min Scan# 1489

Delta R.T. -0.00 min

Lab File: VU040065.D

Acq: 09 Sep 2020 14:58

Instrument :

MSVOA_U

ClientSampleId :

VU0909WBL01

Tot Ion: 96 Resp: 28109


Ion Ratio Lower Upper

96 100

70 21.6 17.1 25.7

95 9.6 7.6 11.4

97 6.4 0.0 0.0#



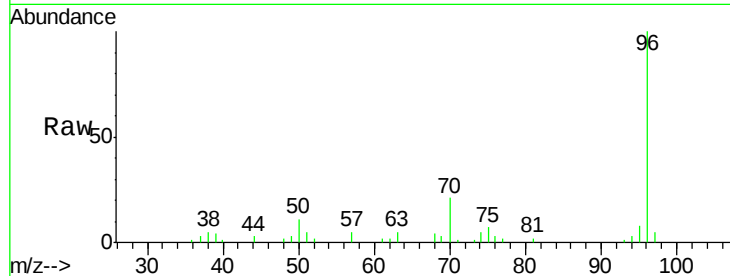


Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 70.00 (69.70 to 70.70): VU0

Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

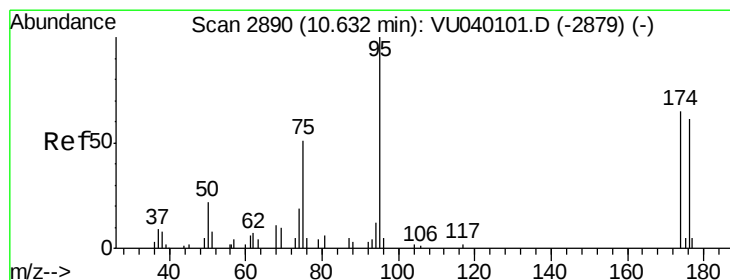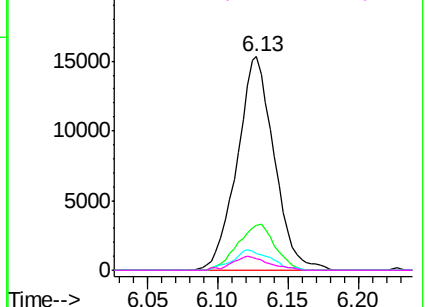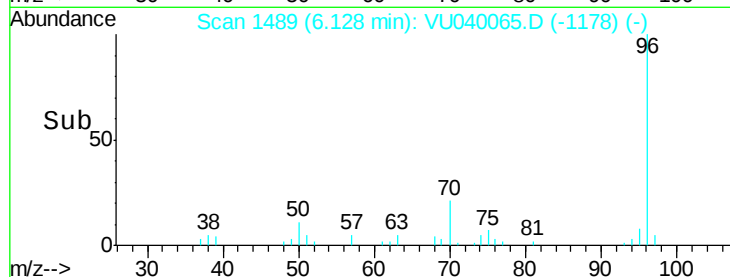

#57

4-Bromofluorobenzene

Concen: 0.806 ug/l

RT: 10.63 min Scan# 2889

Delta R.T. -0.00 min

Lab File: VU040065.D

Acq: 09 Sep 2020 14:58


Tgt Ion: 95 Resp: 9245

Ion Ratio Lower Upper

95 100

174 59.6 49.4 74.0



176 59.8 50.1 75.1

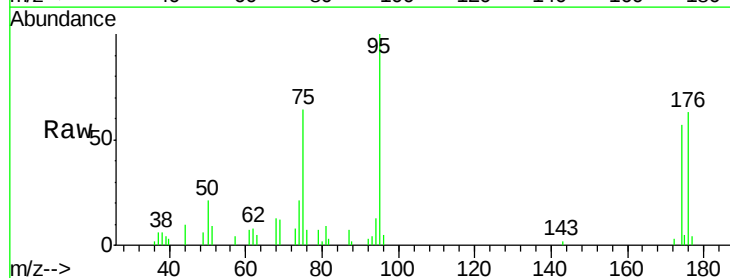


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 174.00 (173.70 to 174.70): V

Ion 176.00 (175.70 to 176.70): V

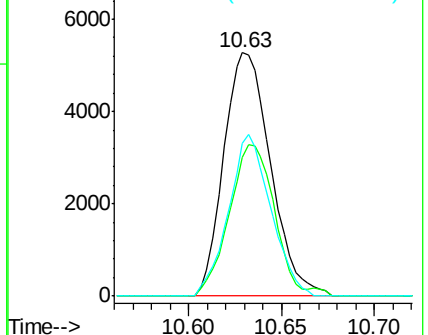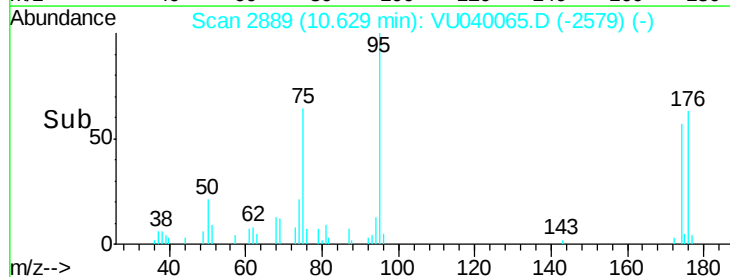

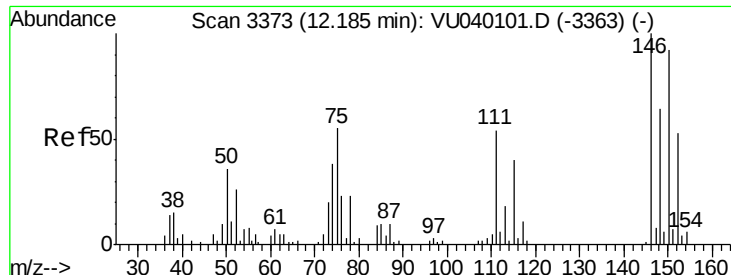

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.851 ug/l
 RT: 12.19 min Scan# 3374
 Delta R.T. -0.00 min
 Lab File: VU040065.D
 Acq: 09 Sep 2020 14:58

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0909WBL01

Tot Ion	Ratio	Lower	Upper
152	100		
115	61.3	0.0	309.0
150	142.8	0.0	658.2

