
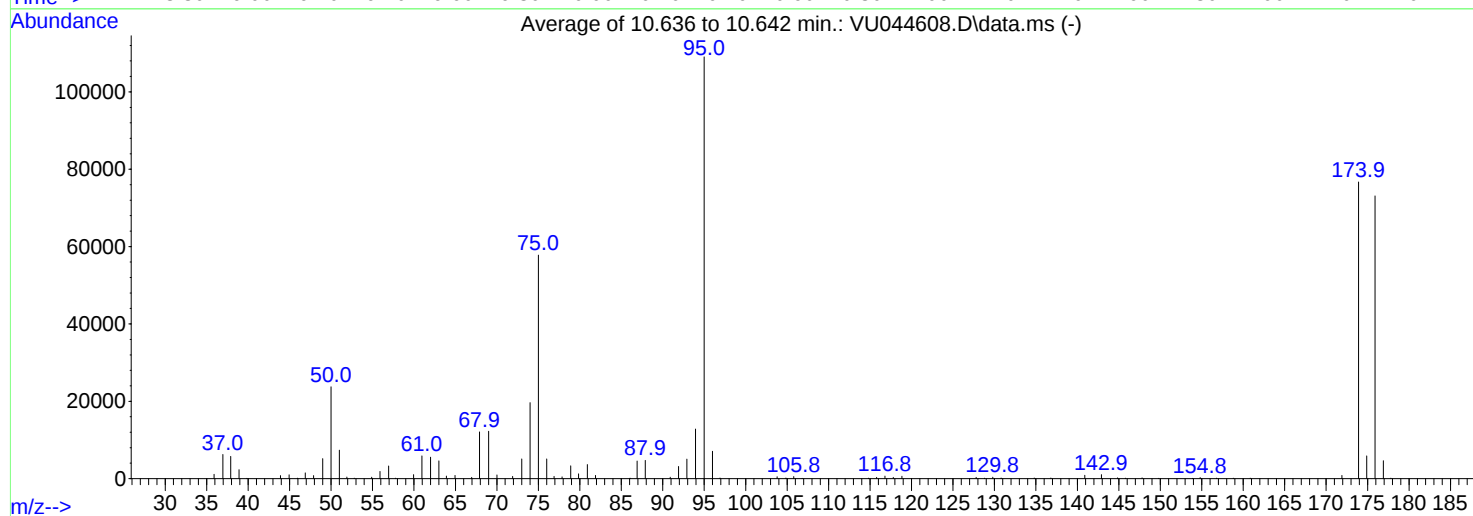


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090921\
 Data File : VU044608.D
 Acq On : 09 Sep 2021 11:58
 Operator : SY/MD
 Sample : BFB015
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB015

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Sep 10 01:38:15 2021

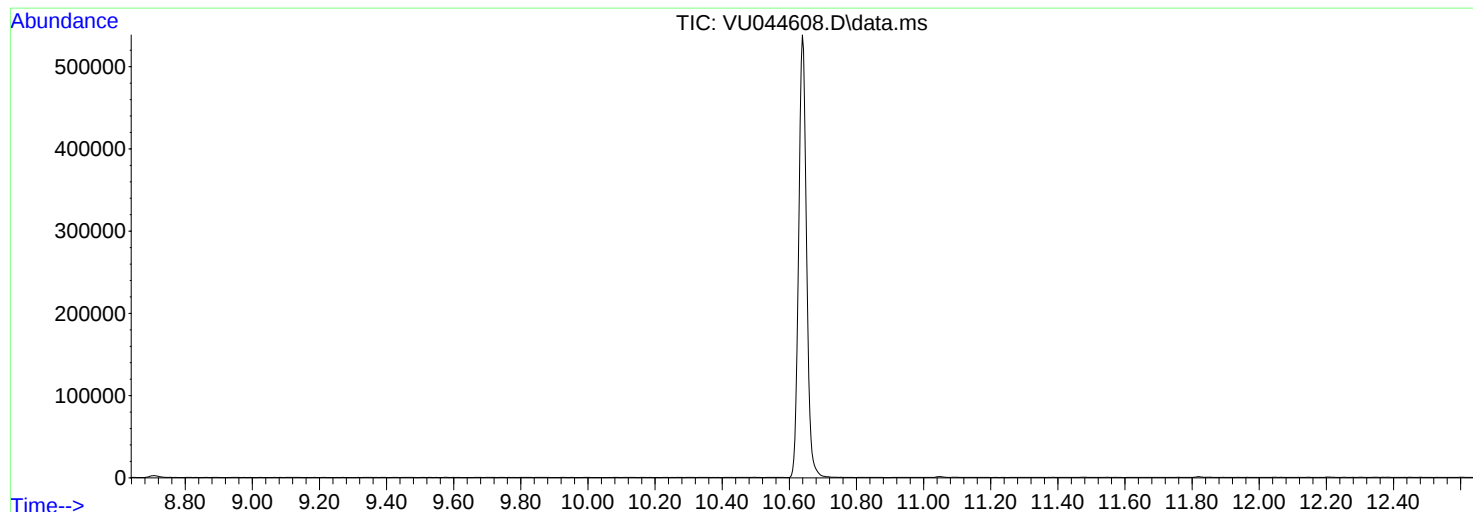

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	23731	PASS
75	95	30	80	53.0	57787	PASS
95	95	100	100	100.0	109059	PASS
96	95	5	9	6.5	7068	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.3	76696	PASS
175	174	5	9	7.7	5896	PASS
176	174	95	101	95.3	73112	PASS
177	176	5	9	6.3	4622	PASS

Scan 2878 (10.594 min): VU044608.D\data.ms
BFB015

m/z	Abundance
39.80	116.0
43.90	326.0

Instrument :
MSVOA_U
ClientSampleId :
BFB015

m/z	Abundance
35.90	1107.0
37.00	6051.0
37.90	5810.0
38.90	2361.0
39.90	222.0
43.90	1077.0
44.90	935.0
45.90	133.0
46.90	1526.0
47.90	813.0
49.00	5103.0
50.00	23336.0
51.00	7037.0
51.90	381.0
52.80	122.0
54.90	350.0
55.90	1752.0
56.90	3223.0
57.80	118.0
60.00	1079.0
61.00	5922.0
62.00	5188.0
63.00	4526.0
63.90	606.0
64.90	752.0
67.00	335.0
67.90	12142.0
69.00	12086.0
70.00	911.0
71.90	556.0
73.00	4972.0
74.00	19416.0
75.00	57096.0
76.00	4916.0
76.90	603.0
77.80	428.0
78.90	3215.0
79.80	1235.0
80.90	3603.0
81.90	816.0
86.10	136.0
86.90	4580.0
87.90	4854.0
90.90	378.0
91.90	3188.0
92.90	5112.0
94.00	12662.0
95.00	108088.0
96.00	6978.0
96.90	160.0
103.80	483.0
104.90	138.0
105.80	534.0
106.80	113.0
114.80	128.0
115.80	338.0
116.80	689.0
117.80	351.0
118.90	657.0
127.80	371.0
128.80	112.0
129.80	380.0
130.80	127.0
134.80	148.0
136.80	149.0
140.90	867.0
142.90	1050.0
144.90	182.0
145.80	145.0
147.80	175.0
149.80	100.0
153.90	107.0
154.80	281.0
156.80	130.0
158.80	114.0
160.80	124.0
171.90	820.0
173.90	78080.0
174.90	6095.0
175.90	74672.0
176.90	4790.0
177.80	148.0

Instrument :
MSVOA_U
ClientSampleId :
BFB015

m/z	Abundance
35.90	1164.0
36.90	6408.0
37.90	5952.0
38.90	2415.0
39.90	220.0
43.90	1140.0
44.90	1006.0
46.00	128.0
46.90	1574.0
47.90	803.0
49.00	5366.0
50.00	24560.0
51.00	7597.0
51.90	419.0
52.80	125.0
54.90	374.0
55.90	1934.0
56.90	3335.0
57.80	118.0
59.90	1093.0
60.90	6140.0
62.00	5710.0
63.00	4688.0
63.90	689.0
65.00	859.0
66.90	350.0
67.90	12536.0
69.00	12670.0
70.00	1015.0
71.90	621.0
73.00	5301.0
74.00	20280.0
75.00	59528.0
76.00	5268.0
76.90	601.0
77.80	444.0
78.90	3405.0
79.90	1276.0
80.90	3771.0
81.90	855.0
86.10	153.0
86.90	4676.0
87.90	4917.0
90.90	397.0
91.90	3263.0
92.90	5258.0
94.00	13216.0
95.00	112880.0
96.00	7259.0
96.90	182.0
103.80	553.0
104.80	156.0
105.80	551.0
106.80	114.0
114.80	135.0
115.80	328.0
116.80	686.0
117.80	363.0
118.90	667.0
127.80	324.0
128.80	140.0
129.80	364.0
130.80	179.0
134.80	165.0
136.80	172.0
140.90	929.0
142.90	1091.0
144.80	206.0
145.80	153.0
147.80	200.0
149.80	104.0
153.90	111.0
154.80	293.0
156.80	128.0
158.80	131.0
160.90	128.0
171.90	877.0
173.90	78944.0
174.90	6093.0
175.90	75408.0
176.90	4715.0
177.80	134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB015

m/z	Abundance
35.90	1098.0
36.90	6278.0
37.90	5482.0
38.90	2222.0
39.90	217.0
43.90	1161.0
45.00	995.0
46.00	125.0
46.90	1415.0
47.90	741.0
49.00	5033.0
50.00	23296.0
51.00	7517.0
51.90	395.0
52.80	120.0
54.90	351.0
55.90	1919.0
57.00	3243.0
57.80	123.0
59.90	987.0
60.90	5631.0
62.00	5744.0
63.00	4529.0
63.90	670.0
65.00	911.0
66.90	364.0
67.90	11599.0
69.00	12012.0
70.00	990.0
71.90	608.0
73.00	5036.0
74.00	19280.0
75.00	56736.0
76.00	5062.0
76.90	595.0
77.90	490.0
78.90	3317.0
79.90	1180.0
80.90	3539.0
81.90	821.0
86.00	149.0
86.90	4412.0
87.90	4423.0
90.90	359.0
91.90	2987.0
92.90	4828.0
93.90	12546.0
95.00	106208.0
96.00	6967.0
96.90	211.0
103.80	517.0
104.80	156.0
105.80	484.0
114.80	129.0
115.80	293.0
116.80	595.0
117.80	324.0
118.80	588.0
127.80	281.0
128.80	151.0
129.80	330.0
130.80	177.0
134.80	167.0
136.80	169.0
140.90	861.0
142.90	999.0
144.80	195.0
145.80	143.0
147.80	196.0
154.80	260.0
156.80	139.0
158.80	140.0
160.90	115.0
171.90	816.0
173.90	73064.0
174.90	5499.0
175.90	69256.0
176.90	4361.0
177.80	112.0

Instrument :
MSVOA_U
ClientSampleId :
BFB015