

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090924\
 Data File : VU060653.D
 Acq On : 09 Sep 2024 12:33
 Operator : MD/SY
 Sample : P3867-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Sep 09 23:46:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.257	114	4722	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.418	117	7063	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	2034	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	3367	0.438	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	88.000%
4) 1,2-Dichloroethane-d4	5.685	65	2049	0.503	ug/L	-0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	100.000%
7) 1,2-Dichloropropane-d6	6.687	67	2182	0.497	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	100.000%
8) Toluene-d8	7.887	98	5009	0.552	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	110.000%
10) 1,1,2,2-Tetrachloroeth...	10.745	84	1737	0.452	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	90.000%
Target Compounds						
6) Trichloroethene	6.544	95	6484	1.454	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090924\
Data File : VU060653.D
Acq On : 09 Sep 2024 12:33
Operator : MD/SY
Sample : P3867-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Sep 09 23:46:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration

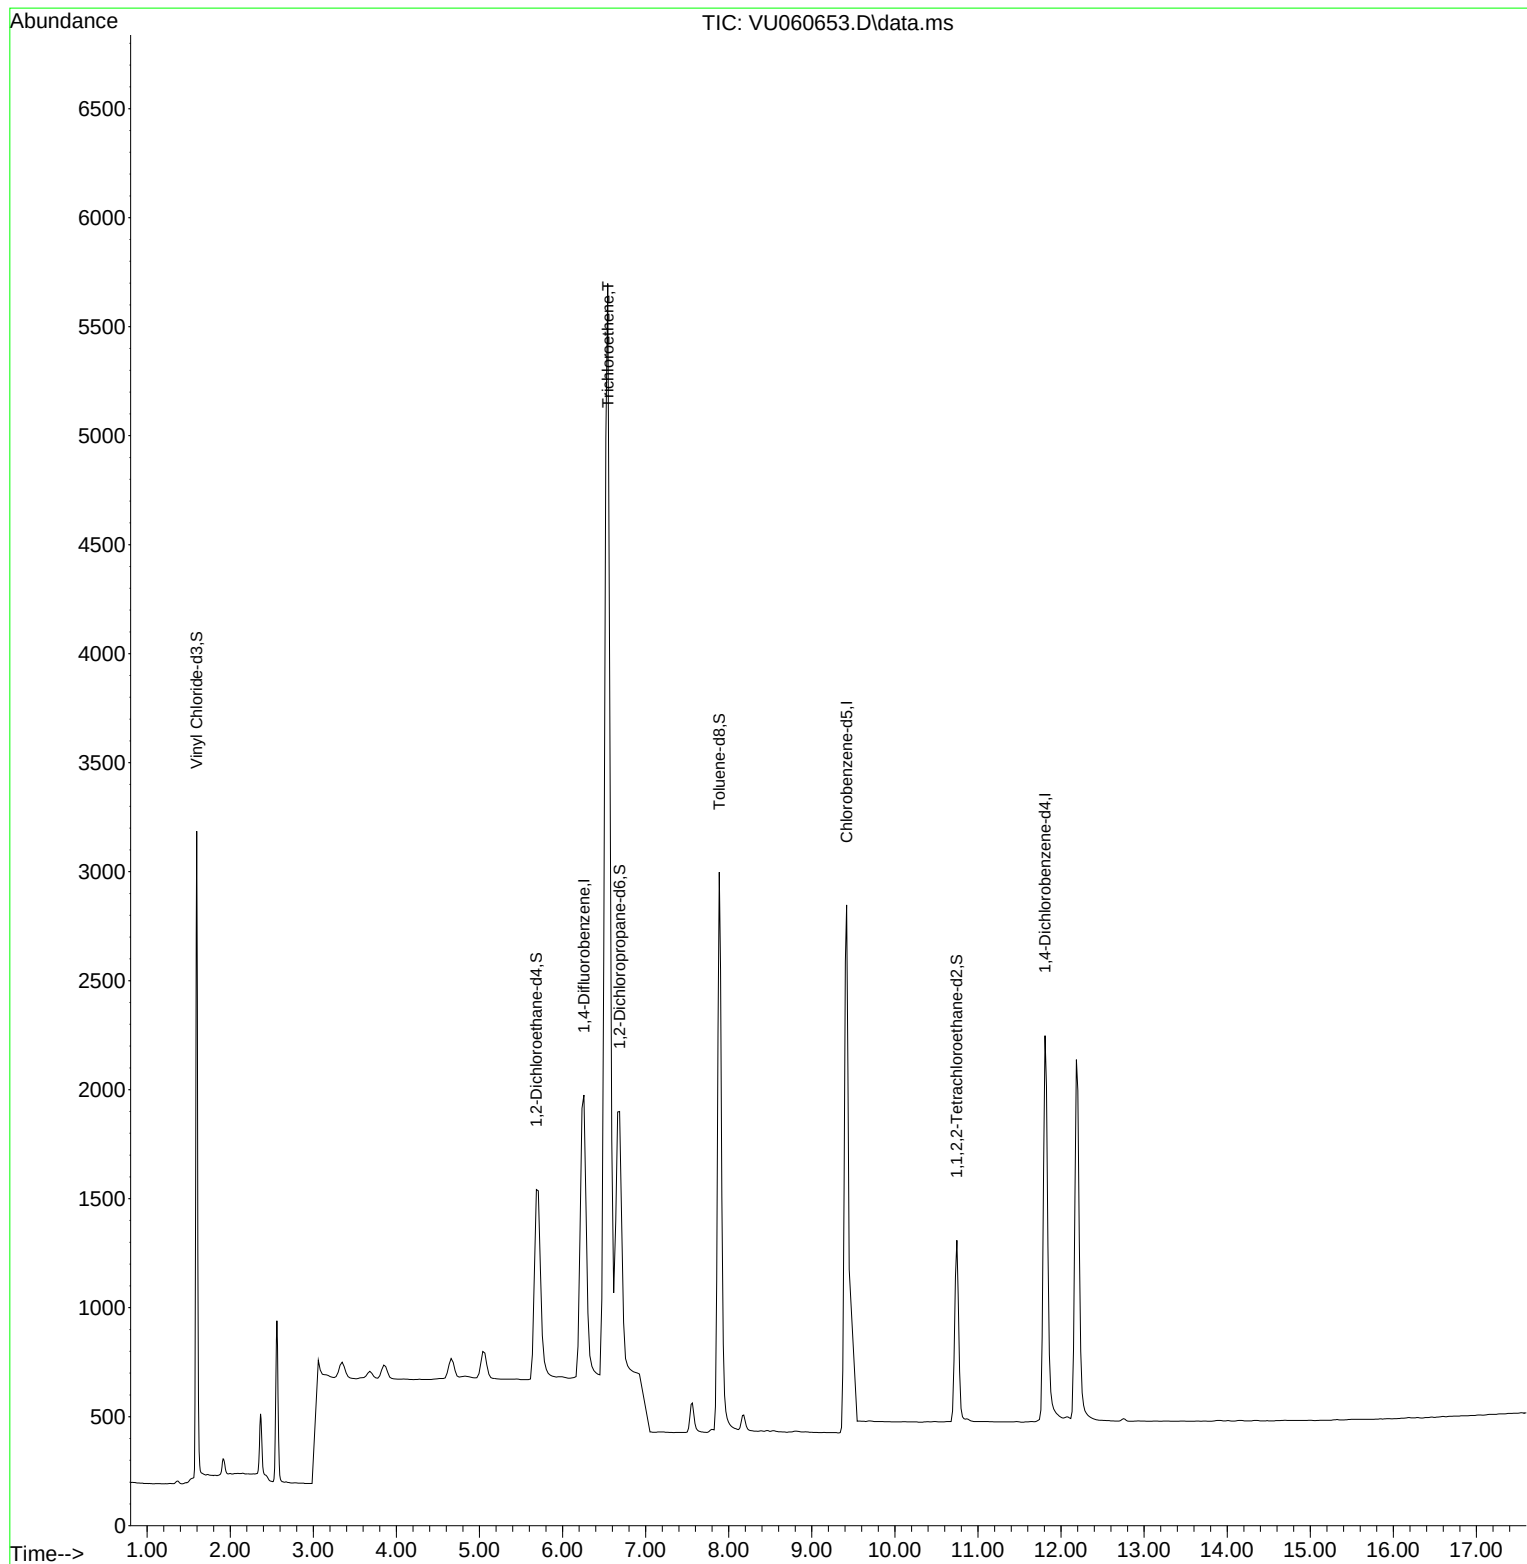

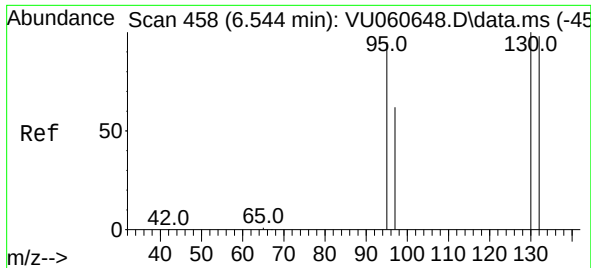

#6
Trichloroethene
Concen: 1.454 ug/L
RT: 6.544 min Scan# 458
Delta R.T. -0.000 min
Lab File: VU060653.D
Acq: 09 Sep 2024 12:33

Instrument :
MSVOA_U
ClientSampleId :

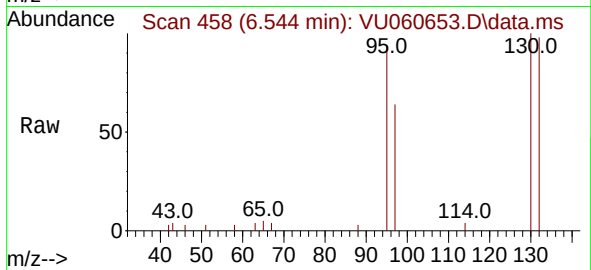

Tgt Ion: 95 Resp: 6484
Ion Ratio Lower Upper
95 100
97 67.3 48.5 90.1
132 103.7 75.5 140.1
130 105.8 76.3 141.7

