


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090924\
Data File : VU060647.D
Acq On : 09 Sep 2024 08:49
Operator : MD/SY
Sample : BFB014
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB014

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Title : TRACE VOA SOM01.0
Last Update : Sat Aug 17 05:03:57 2024

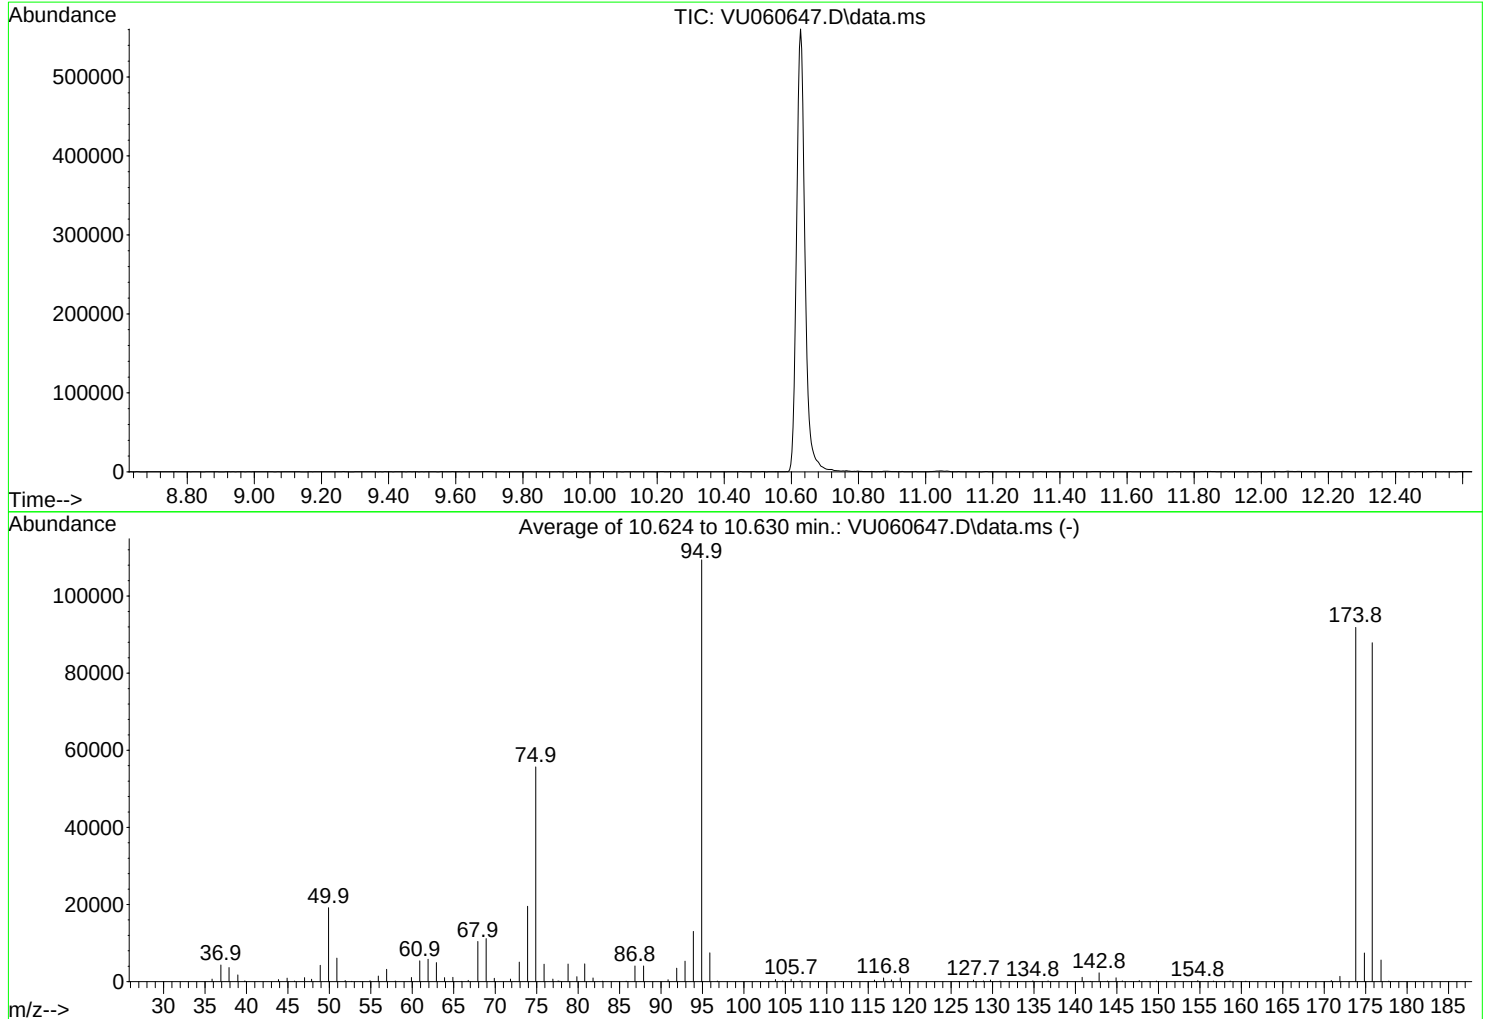

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	19163	PASS
75	95	30	80	50.9	55691	PASS
95	95	100	100	100.0	109392	PASS
96	95	5	9	6.8	7462	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.0	91880	PASS
175	174	5	9	8.1	7442	PASS
176	174	95	101	95.7	87907	PASS
177	176	5	9	6.4	5607	PASS

m/z	Abundance
43.90	245.0

Instrument :
MSVOA_U
ClientSampleId :
BFB014

m/z	Abundance
35.90	767.0
36.90	4296.0
37.90	3625.0
39.00	1760.0
39.70	254.0
43.80	793.0
44.90	921.0
45.80	150.0
47.00	1166.0
47.90	627.0
48.90	4452.0
49.90	19048.0
50.90	5833.0
51.90	339.0
52.70	128.0
54.90	185.0
55.90	1394.0
56.90	3225.0
58.00	180.0
59.90	1019.0
60.90	5328.0
61.90	5980.0
62.90	4878.0
63.90	1163.0
64.90	1051.0
66.80	329.0
67.90	10354.0
68.90	10931.0
69.90	934.0
71.90	653.0
72.90	5153.0
73.90	19712.0
74.90	55224.0
75.90	4500.0
77.00	671.0
77.60	323.0
78.80	4541.0
79.80	1198.0
80.80	4490.0
81.80	897.0
83.00	119.0
85.80	133.0
86.80	4158.0
87.90	3976.0
90.80	517.0
91.90	3210.0
92.90	5213.0
93.90	12524.0
94.90	108696.0
95.90	7102.0
96.80	117.0
103.80	587.0
104.70	201.0
105.70	570.0
106.80	201.0
115.80	443.0
116.90	910.0
117.80	410.0
118.80	903.0
119.90	112.0
127.70	416.0
128.90	165.0
129.80	471.0
130.90	142.0
134.80	235.0
136.70	200.0
140.80	1154.0
142.80	2421.0
143.80	145.0
144.90	1008.0
145.70	157.0
147.70	305.0
148.80	105.0
149.80	141.0
154.80	353.0
156.70	175.0
158.60	126.0
160.70	135.0
170.90	268.0
171.90	1409.0
173.80	89424.0
174.80	7411.0
175.80	85688.0
176.80	5438.0
177.80	163.0

Instrument :
MSVOA_U
ClientSampleId :
BFB014

m/z	Abundance
35.80	675.0
36.90	4476.0
37.90	3663.0
39.00	1802.0
39.80	223.0
43.80	775.0
44.90	913.0
45.80	157.0
47.00	1106.0
47.90	654.0
48.90	4302.0
49.90	19744.0
50.90	6259.0
51.90	305.0
52.70	106.0
54.90	239.0
55.90	1520.0
56.90	3363.0
58.00	187.0
59.90	1150.0
60.90	5578.0
61.90	6035.0
62.90	5149.0
63.90	1053.0
64.90	1174.0
65.90	124.0
66.70	396.0
67.90	10754.0
68.90	11489.0
69.90	867.0
71.80	698.0
72.90	5111.0
73.90	20224.0
74.90	57304.0
75.90	4599.0
76.90	675.0
77.60	370.0
78.80	4727.0
79.90	1335.0
80.80	4688.0
81.80	997.0
82.90	104.0
85.80	137.0
86.80	4197.0
87.90	4163.0
90.80	492.0
91.90	3598.0
92.90	5472.0
93.90	13490.0
94.90	112856.0
95.90	7761.0
96.80	150.0
103.80	568.0
104.70	249.0
105.70	615.0
106.80	212.0
115.80	422.0
116.80	999.0
117.80	461.0
118.90	986.0
125.90	110.0
127.70	447.0
128.90	201.0
129.80	407.0
130.90	155.0
134.80	227.0
136.70	239.0
140.80	1113.0
141.80	143.0
142.80	2327.0
143.80	169.0
144.90	1063.0
145.60	199.0
147.70	287.0
148.90	110.0
149.80	159.0
154.70	307.0
156.70	151.0
158.70	168.0
160.50	131.0
170.90	303.0
171.90	1431.0
173.80	94712.0
174.90	7711.0
175.80	90680.0
176.80	5683.0
177.80	183.0

Instrument :
MSVOA_U
ClientSampleId :
BFB014

m/z	Abundance
35.90	598.0
36.90	4190.0
37.90	3713.0
38.90	1703.0
39.90	209.0
43.90	726.0
44.90	877.0
45.80	178.0
47.00	854.0
47.80	587.0
48.90	3944.0
49.90	18696.0
50.90	6193.0
51.90	250.0
53.80	112.0
54.90	287.0
55.90	1502.0
56.90	2956.0
57.90	150.0
59.90	1012.0
60.90	5298.0
61.90	5425.0
62.90	4812.0
63.90	881.0
64.90	1173.0
65.90	125.0
66.70	320.0
67.90	10189.0
68.90	11029.0
69.90	764.0
71.80	702.0
72.90	4873.0
73.90	18672.0
74.90	54544.0
75.90	4514.0
76.90	661.0
77.80	408.0
78.80	4472.0
79.90	1362.0
80.80	4605.0
81.80	942.0
82.90	116.0
85.80	144.0
86.90	3858.0
87.90	4075.0
90.90	442.0
91.90	3598.0
92.90	5289.0
93.90	13048.0
94.90	106624.0
95.90	7524.0
96.80	186.0
103.00	104.0
103.80	534.0
104.70	237.0
105.70	630.0
106.80	169.0
110.90	107.0
111.80	100.0
112.90	134.0
115.70	367.0
116.80	982.0
117.80	470.0
118.90	989.0
127.70	406.0
128.90	241.0
129.70	373.0
130.90	150.0
134.90	214.0
136.70	229.0
140.80	1094.0
141.80	135.0
142.90	2099.0
143.90	186.0
144.90	961.0
145.70	223.0
146.70	119.0
147.70	248.0
148.90	103.0
149.60	153.0
154.80	244.0
156.60	166.0
158.70	203.0
160.50	114.0
170.80	357.0
171.90	1325.0
173.80	91504.0
174.90	7203.0
175.80	87352.0
176.90	5700.0
177.80	164.0

Instrument :
MSVOA_U
ClientSampleId :
BFB014