

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091018\
 Data File : VU026667.D
 Acq On : 10 Sep 2018 22:19
 Operator : MD/SY
 Sample : J4837-15
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08N3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091018WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.398	63	70	82	rBV	98893	99647	15.01%	1.894%
2	1.678	150	157	174	rVB	75506	95509	14.39%	1.815%
3	2.273	331	342	355	rBV	147724	223953	33.73%	4.256%
4	2.443	385	395	412	rBV2	3714	6730	1.01%	0.128%
5	2.614	443	448	455	rVB2	267	363	0.05%	0.007%
6	2.678	466	468	471	rVB	185	91	0.01%	0.002%
7	2.839	508	518	531	rBB	1419	2926	0.44%	0.056%
8	2.997	564	567	570	rBV	87	70	0.01%	0.001%
9	3.141	609	612	615	rBV	103	75	0.01%	0.001%
10	3.186	623	626	629	rBV2	190	162	0.02%	0.003%
11	3.273	648	653	655	rBV	105	92	0.01%	0.002%
12	3.379	684	686	688	rVV	209	80	0.01%	0.002%
13	3.395	688	691	694	rVB	119	71	0.01%	0.001%
14	3.543	734	737	740	rBV	94	72	0.01%	0.001%
15	3.630	761	764	768	rVV	95	72	0.01%	0.001%
16	3.842	826	830	836	rBB	105	80	0.01%	0.002%
17	3.877	836	841	845	rBV	79	68	0.01%	0.001%
18	3.903	846	849	850	rBV	141	61	0.01%	0.001%
19	4.177	920	934	966	rBV	56406	148766	22.41%	2.827%
20	4.556	1047	1052	1055	rBV	84	86	0.01%	0.002%
21	4.649	1065	1081	1105	rBV	111402	271641	40.92%	5.162%
22	4.762	1114	1116	1119	rBV	251	163	0.02%	0.003%
23	4.829	1133	1137	1141	rBV	215	241	0.04%	0.005%
24	4.877	1150	1152	1154	rBV	223	127	0.02%	0.002%
25	4.974	1178	1182	1188	rBV	93	79	0.01%	0.002%
26	5.074	1210	1213	1217	rVB	89	64	0.01%	0.001%
27	5.135	1217	1232	1244	rBV4	2627	5846	0.88%	0.111%
28	5.344	1272	1297	1328	rBV2	225950	663908	100.00%	12.617%
29	5.492	1341	1343	1345	rVB	138	74	0.01%	0.001%
30	5.591	1372	1374	1377	rVB	208	83	0.01%	0.002%
31	5.784	1431	1434	1436	rBV2	177	145	0.02%	0.003%
32	5.890	1452	1467	1488	rBV	214647	416799	62.78%	7.921%
33	6.038	1512	1513	1516	rVB2	178	91	0.01%	0.002%
34	6.057	1516	1519	1522	rBV	98	65	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091018\
 Data File : VU026667.D
 Acq On : 10 Sep 2018 22:19
 Operator : MD/SY
 Sample : J4837-15
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08N3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091018WMA.M
 Title : VOC Analysis

35	6.186	1557	1559	1560	rBV	334	153	0.02%	0.003%
36	6.334	1590	1605	1625	rVV	153920	306001	46.09%	5.815%
37	6.421	1629	1632	1636	rVB2	200	136	0.02%	0.003%
38	6.466	1643	1646	1649	rVB	279	127	0.02%	0.002%
39	6.514	1656	1661	1673	rBV2	393	647	0.10%	0.012%
40	6.617	1690	1693	1699	rVB	92	82	0.01%	0.002%
41	6.646	1699	1702	1706	rBV2	169	154	0.02%	0.003%
42	6.672	1707	1710	1712	rBV2	134	101	0.02%	0.002%
43	6.736	1729	1730	1733	rVB	136	75	0.01%	0.001%
44	6.758	1733	1737	1739	rBV	189	127	0.02%	0.002%
45	6.829	1751	1759	1768	rVV4	1514	2792	0.42%	0.053%
46	6.864	1768	1770	1773	rVB2	249	122	0.02%	0.002%
47	6.938	1790	1793	1795	rBV	104	65	0.01%	0.001%
48	7.012	1813	1816	1819	rBV	88	70	0.01%	0.001%
49	7.045	1823	1826	1829	rVV	213	141	0.02%	0.003%
50	7.064	1829	1832	1838	rVB2	206	181	0.03%	0.003%
51	7.228	1872	1883	1903	rVV	82363	144215	21.72%	2.741%
52	7.318	1909	1911	1914	rVB	142	60	0.01%	0.001%
53	7.379	1924	1930	1931	rBV	92	87	0.01%	0.002%
54	7.392	1931	1934	1935	rVV	160	117	0.02%	0.002%
55	7.398	1935	1936	1938	rVB	315	80	0.01%	0.002%
56	7.440	1944	1949	1953	rVB	77	84	0.01%	0.002%
57	7.466	1953	1957	1962	rVB	116	101	0.02%	0.002%
58	7.488	1962	1964	1967	rBV	145	102	0.02%	0.002%
59	7.569	1975	1989	2008	rBV	296336	511172	76.99%	9.714%
60	7.729	2037	2039	2042	rVB	184	83	0.01%	0.002%
61	7.762	2046	2049	2053	rVB	90	59	0.01%	0.001%
62	7.787	2053	2057	2059	rBV	75	64	0.01%	0.001%
63	7.852	2066	2077	2098	rBV	57466	96858	14.59%	1.841%
64	7.971	2111	2114	2115	rBV2	219	147	0.02%	0.003%
65	7.987	2117	2119	2123	rVB	153	96	0.01%	0.002%
66	8.022	2125	2130	2134	rBV	207	200	0.03%	0.004%
67	8.045	2134	2137	2138	rBV	160	90	0.01%	0.002%
68	8.186	2167	2181	2188	rBV3	4102	8578	1.29%	0.163%
69	8.311	2210	2220	2247	rVB	184575	310839	46.82%	5.907%
70	8.530	2285	2288	2289	rBV	147	68	0.01%	0.001%
71	8.646	2322	2324	2326	rVV	166	87	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091018\
 Data File : VU026667.D
 Acq On : 10 Sep 2018 22:19
 Operator : MD/SY
 Sample : J4837-15
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08N3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091018WMA.M
 Title : VOC Analysis

72	8.713	2343	2345	2349	rBV	144	84	0.01%	0.002%
73	8.800	2368	2372	2374	rBV	146	84	0.01%	0.002%
74	8.826	2378	2380	2383	rVB	151	71	0.01%	0.001%
75	8.868	2390	2393	2397	rBV	80	67	0.01%	0.001%
76	8.958	2416	2421	2424	rBV	103	109	0.02%	0.002%
77	9.093	2451	2463	2491	rVV2	312700	633846	95.47%	12.046%
78	9.340	2536	2540	2547	rVB	279	241	0.04%	0.005%
79	9.382	2550	2553	2556	rVB2	149	115	0.02%	0.002%
80	9.649	2633	2636	2639	rBV	156	116	0.02%	0.002%
81	9.681	2643	2646	2649	rBV	117	90	0.01%	0.002%
82	9.829	2689	2692	2695	rBV	115	75	0.01%	0.001%
83	9.993	2737	2743	2746	rBV	120	149	0.02%	0.003%
84	10.434	2867	2880	2901	rBV	208322	324648	48.90%	6.170%
85	10.607	2927	2934	2948	rVB2	1687	2841	0.43%	0.054%
86	10.778	2984	2987	2989	rBV	156	102	0.02%	0.002%
87	11.038	3064	3068	3071	rBV2	241	214	0.03%	0.004%
88	11.350	3163	3165	3170	rVB	204	100	0.02%	0.002%
89	11.421	3180	3187	3195	rVV3	3307	4583	0.69%	0.087%
90	11.485	3195	3207	3232	rVB	280185	447985	67.48%	8.514%
91	11.749	3285	3289	3295	rBV3	869	950	0.14%	0.018%
92	11.861	3311	3324	3346	rBV	292684	500659	75.41%	9.515%
93	12.195	3426	3428	3431	rBV2	190	143	0.02%	0.003%
94	12.266	3448	3450	3454	rBV	171	102	0.02%	0.002%
95	12.482	3511	3517	3524	rBV3	521	678	0.10%	0.013%
96	13.189	3735	3737	3740	rBV	189	97	0.01%	0.002%
97	13.292	3767	3769	3773	rBV	261	145	0.02%	0.003%
98	13.507	3828	3836	3849	rBV3	8382	13641	2.05%	0.259%
99	13.658	3882	3883	3884	rBV3	245	83	0.01%	0.002%
100	13.993	3981	3987	4001	rVB6	4759	7500	1.13%	0.143%


Sum of corrected areas: 5261979

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU091018\
Data File : VU026667.D
Acq On : 10 Sep 2018 22:19
Operator : MD/SY
Sample : J4837-15
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C08N3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

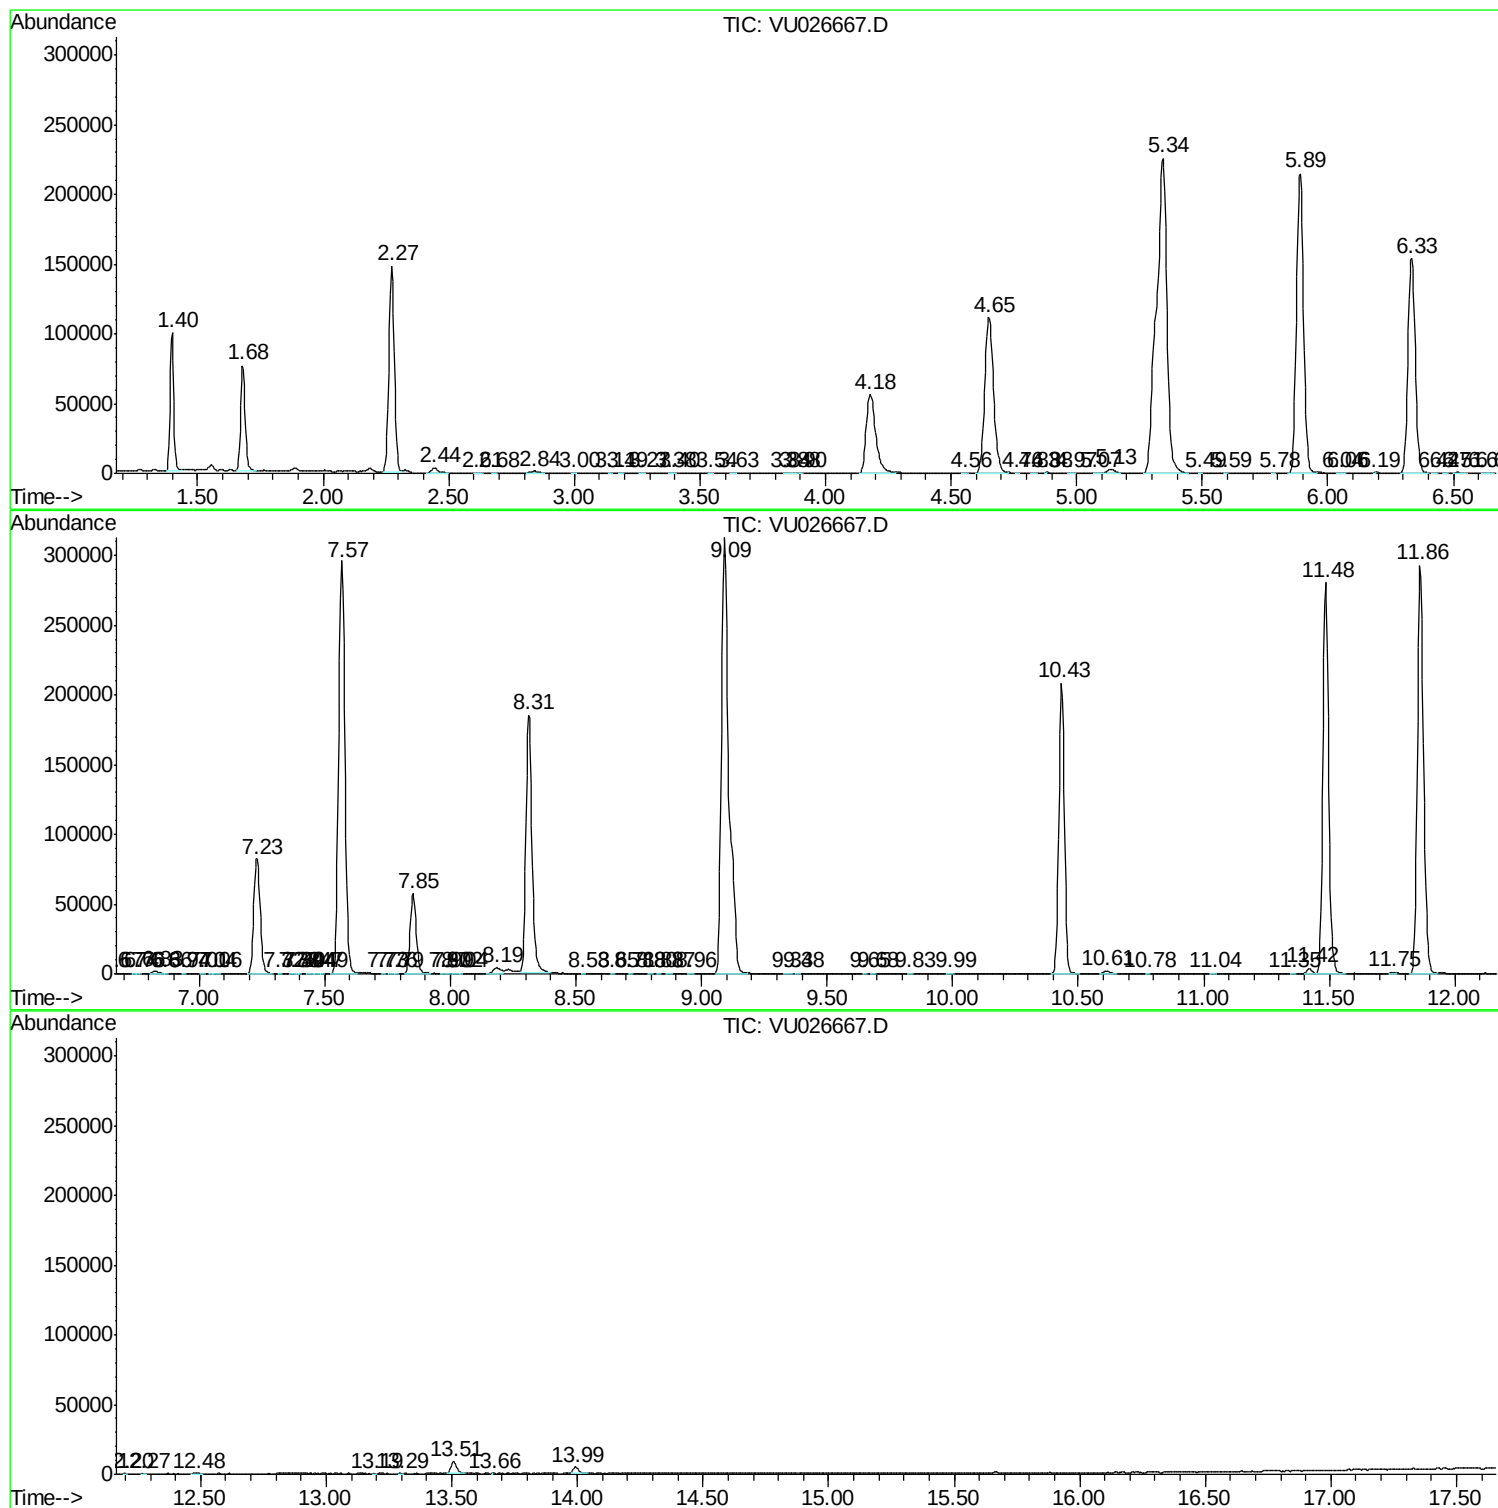

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU091018\
Data File : VU026667.D
Acq On : 10 Sep 2018 22:19
Operator : MD/SY
Sample : J4837-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C08N3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU091018\
Data File : VU026667.D
Acq On : 10 Sep 2018 22:19
Operator : MD/SY
Sample : J4837-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C08N3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc