


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091018\
Data File : VU026633.D
Acq On : 10 Sep 2018 07:28
Operator : MD/SY
Sample : BFB52
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB52

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091018WMA.M
Title : VOC Analysis
Last Update : Tue Sep 11 07:07:03 2018

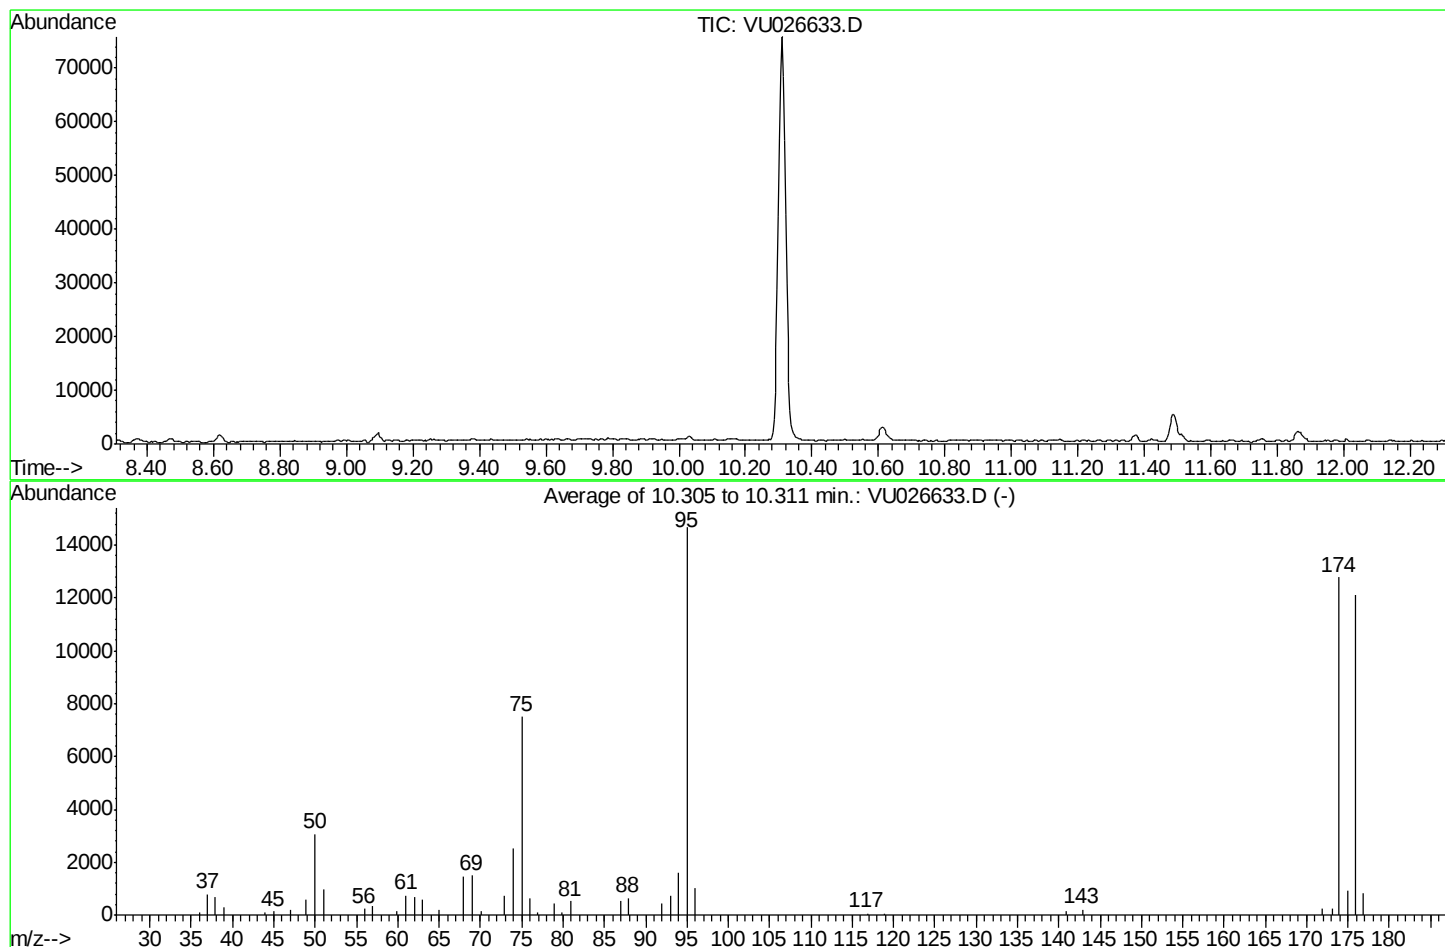

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2830

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	3058	PASS
75	95	30	80	51.1	7499	PASS
95	95	100	100	100.0	14680	PASS
96	95	5	9	6.9	1020	PASS
173	174	0.00	2	1.9	239	PASS
174	95	50	120	87.1	12780	PASS
175	174	5	9	7.3	939	PASS
176	174	95	101	95.0	12142	PASS
177	176	5	9	6.6	803	PASS

Scan 2830 (10.273 min): VU026633.D
BFB52

m/z	Abundance
35.90	493.0
37.90	131.0
39.90	100.0
43.90	187.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
36.00	665.0
37.00	808.0
38.00	752.0
39.00	284.0
43.90	215.0
45.00	146.0
47.00	221.0
48.90	575.0
50.00	2966.0
51.00	835.0
56.00	225.0
56.90	321.0
59.90	143.0
61.00	703.0
62.00	652.0
63.00	508.0
65.00	147.0
68.00	1459.0
69.00	1452.0
70.00	139.0
72.90	657.0
74.00	2316.0
75.00	7165.0
76.00	647.0
78.90	437.0
80.90	481.0
87.00	494.0
87.90	602.0
92.00	458.0
93.00	674.0
94.00	1445.0
95.00	14061.0
96.00	990.0
140.90	123.0
142.90	176.0
171.90	184.0
173.10	227.0
173.90	11774.0
174.90	850.0
175.90	11134.0
176.90	768.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
36.00	616.0
37.00	815.0
38.00	809.0
39.00	318.0
43.90	267.0
45.00	123.0
47.00	203.0
48.90	587.0
50.00	3163.0
51.00	991.0
56.00	249.0
57.00	354.0
59.80	152.0
61.00	783.0
62.00	707.0
63.00	583.0
65.00	188.0
68.00	1507.0
69.00	1531.0
70.10	155.0
73.00	735.0
74.00	2601.0
75.00	7736.0
76.00	658.0
76.90	129.0
78.90	471.0
79.90	121.0
80.90	528.0
86.90	534.0
87.90	645.0
92.00	456.0
92.90	750.0
94.00	1664.0
95.00	15131.0
96.00	1061.0
116.80	106.0
140.90	141.0
142.90	199.0
171.90	226.0
173.10	260.0
173.90	13205.0
174.90	949.0
175.90	12528.0
176.90	845.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
36.00	539.0
37.00	750.0
38.00	821.0
39.00	346.0
44.00	309.0
45.00	103.0
47.00	195.0
48.90	548.0
50.00	3045.0
51.00	1021.0
56.00	242.0
57.00	386.0
59.80	119.0
61.00	766.0
62.00	686.0
63.00	587.0
65.00	210.0
68.00	1430.0
69.00	1486.0
70.00	133.0
73.00	764.0
74.00	2663.0
75.00	7597.0
76.00	580.0
77.00	136.0
78.90	463.0
79.90	152.0
80.90	537.0
86.90	637.0
87.90	659.0
92.00	461.0
92.90	738.0
94.00	1768.0
95.00	14849.0
96.00	1009.0
116.80	107.0
118.90	100.0
140.90	134.0
142.90	210.0
171.90	260.0
173.10	231.0
173.90	13361.0
174.90	1018.0
175.90	12766.0
176.90	798.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52