

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091019\
 Data File : VU034456.D
 Acq On : 10 Sep 2019 17:07
 Operator : JC/SP
 Sample : K4603-20
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PAR-D4-(3.11)

Quant Time: Sep 11 06:57:48 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U090619W.M
 Quant Title : SW846 8260
 QLast Update : Fri Sep 06 05:10:13 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.96	168	223103	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.87	114	355934	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.07	117	365798	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.46	152	187160	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.29	65	194061	57.49	ug/l	0.00
Spiked Amount 50.000			Recovery	=	114.98%	
35) Dibromofluoromethane	4.86	113	167546	50.59	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.18%	
50) Toluene-d8	7.55	98	566969	45.56	ug/l	0.00
Spiked Amount 50.000			Recovery	=	91.12%	
62) 4-Bromofluorobenzene	10.29	95	189790	39.50	ug/l	0.00
Spiked Amount 50.000			Recovery	=	79.00%	
Target Compounds						
16) Acetone	2.31	43	11437	6.547	ug/l	96
20) Methylene Chloride	2.69	84	11829	3.765	ug/l	98
43) Isopropyl Acetate	5.53	43	57626	8.094	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU091019\
Data File : VU034456.D
Acq On : 10 Sep 2019 17:07
Operator : JC/SP
Sample : K4603-20
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PAR-D4-(3.11)

Quant Time: Sep 11 06:57:48 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U090619W.M
Quant Title : SW846 8260
QLast Update : Fri Sep 06 05:10:13 2019
Response via : Initial Calibration

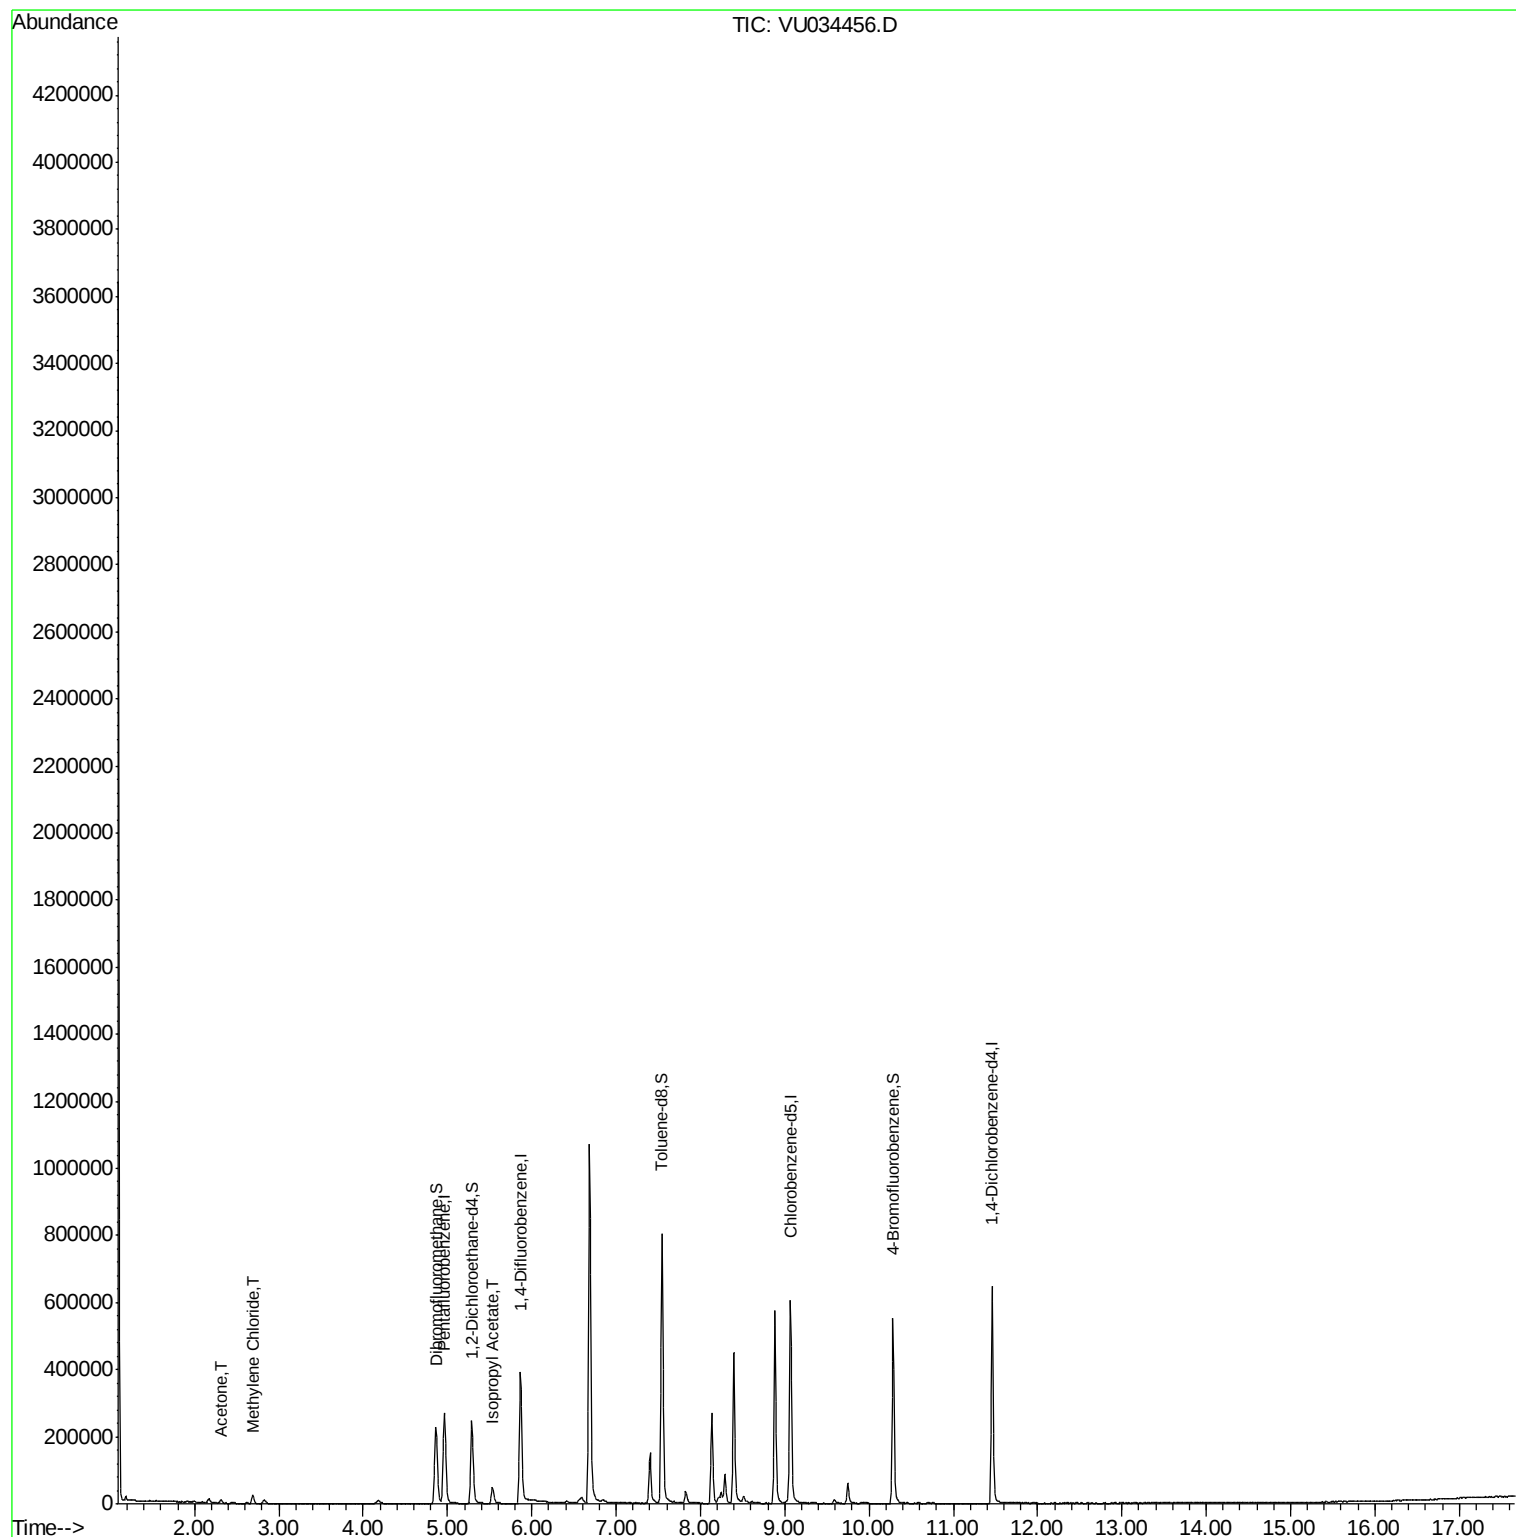

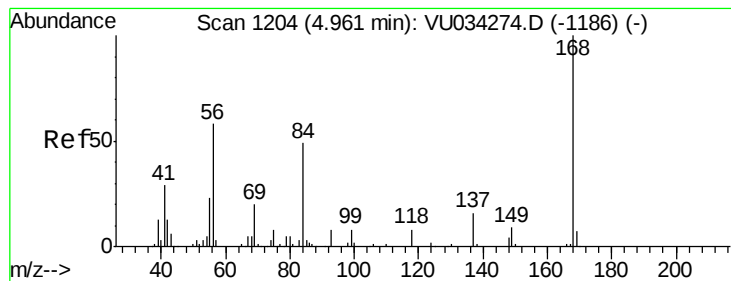

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.96 min Scan# 1205

Delta R.T. 0.00 min

Lab File: VU034456.D

Acq: 10 Sep 2019 17:07

Instrument :

MSVOA_U

ClientSampleId :


PAR-D4-(3.11)

Tot Ion:168 Resp: 223103

Ion Ratio Lower Upper

168 100

99 52.3 41.6 62.4

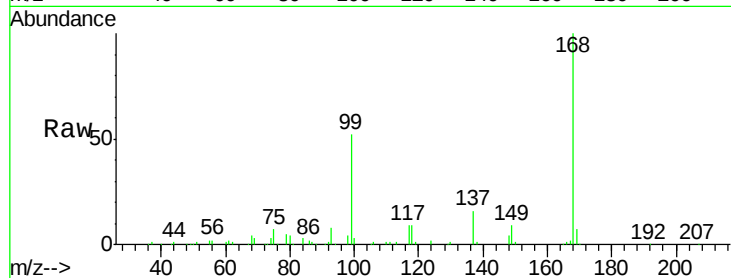

Abundance Ion 167.90 (167.60 to 168.60): VU034456.D (-1186) (-)

Ion 98.90 (98.60 to 99.60): VU034456.D (-1186) (-)

4.96

100000

80000



60000

40000

20000

0

Time-->

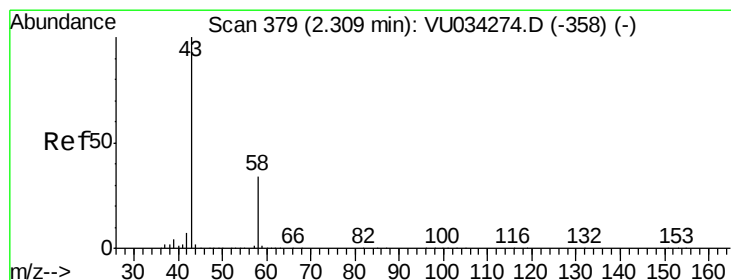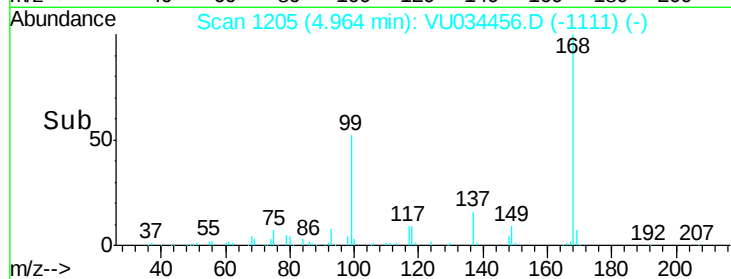

#16

Acetone

Concen: 6.547 ug/l

RT: 2.31 min Scan# 380

Delta R.T. 0.00 min

Lab File: VU034456.D


Acq: 10 Sep 2019 17:07

Tgt Ion: 43 Resp: 11437

Ion Ratio Lower Upper

43 100

58 37.0 27.6 41.4

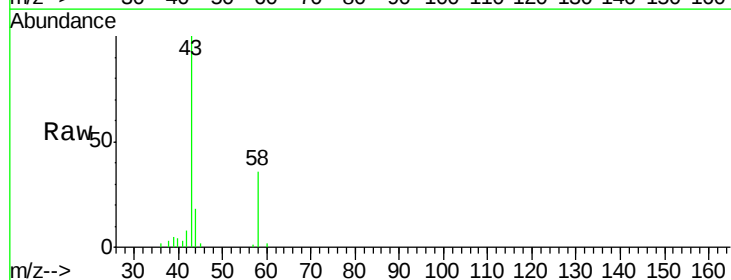

Abundance Ion 43.00 (42.70 to 43.70): VU034456.D (-286) (-)

Ion 58.00 (57.70 to 58.70): VU034456.D (-286) (-)

2.31

8000


6000


4000

2000

0

Time-->




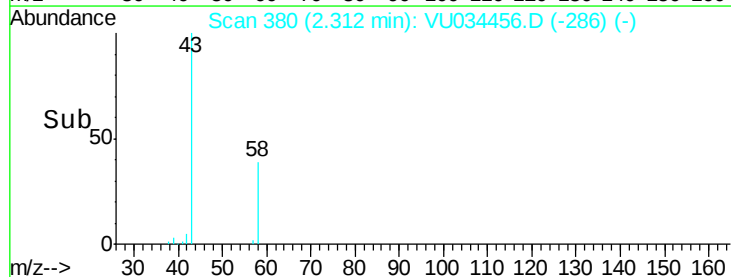


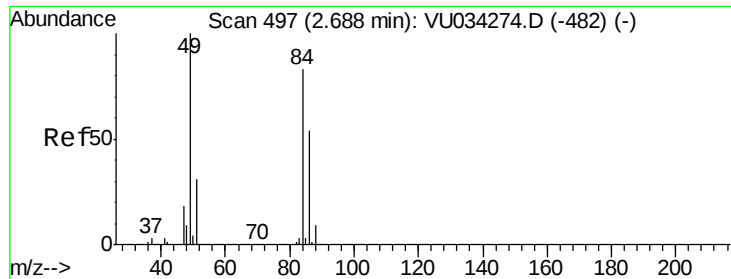

#20
Methvlene Chloride
Concen: 3.765 ug/l
RT: 2.69 min Scan# 498
Delta R.T. 0.00 min
Lab File: VU034456.D
Acq: 10 Sep 2019 17:07




Instrument :
MSVOA_U
ClientSampleId :
PAR-D4-(3.11)


Tot Ion: 84 Resp: 11829
Ion Ratio Lower Upper
84 100
49 123.7 96.0 144.0
51 38.8 30.0 45.0
86 64.7 51.4 77.0

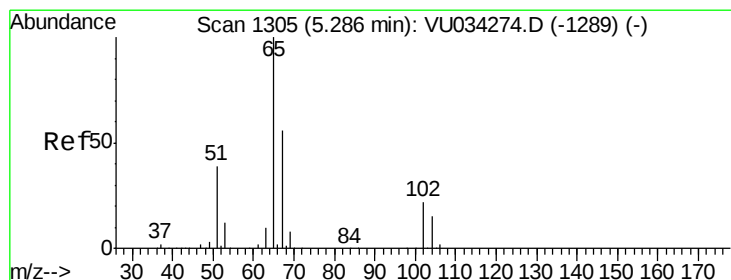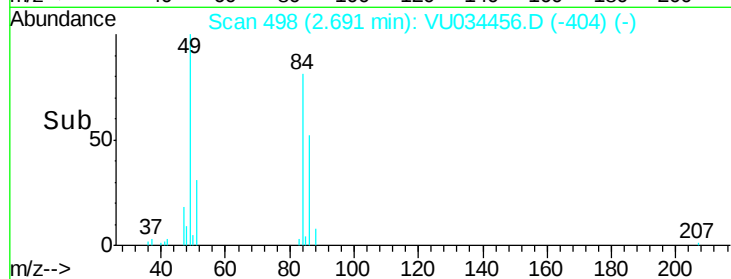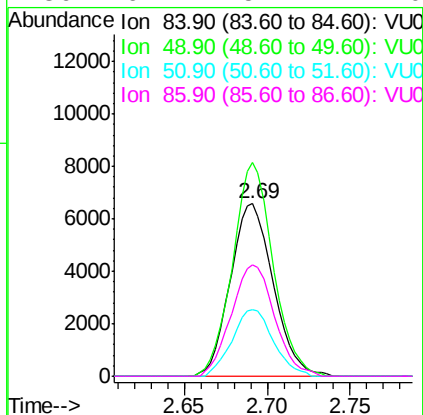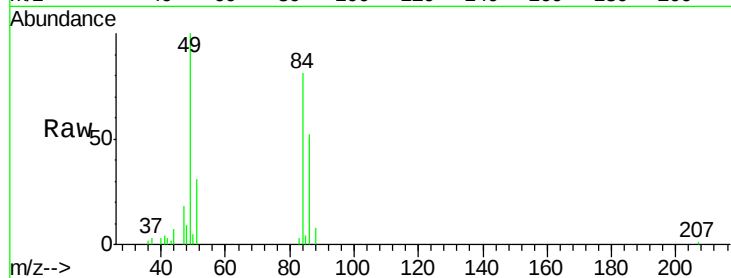

#33
1,2-Dichloroethane-d4
Concen: 57.489 ug/l
RT: 5.29 min Scan# 1306
Delta R.T. 0.00 min
Lab File: VU034456.D
Acq: 10 Sep 2019 17:07

Tgt Ion: 65 Resp: 194061
Ion Ratio Lower Upper
65 100
67 55.1 0.0 112.4

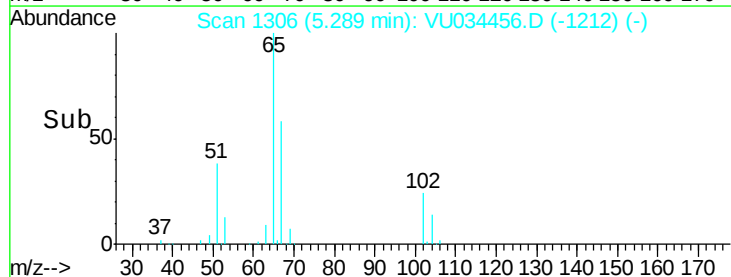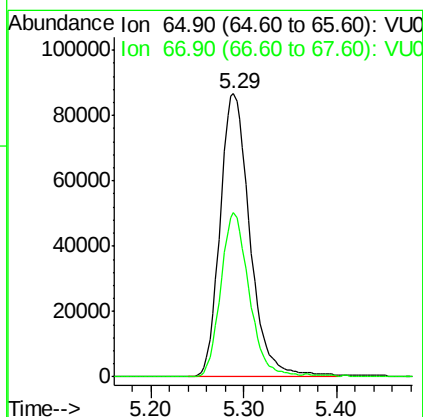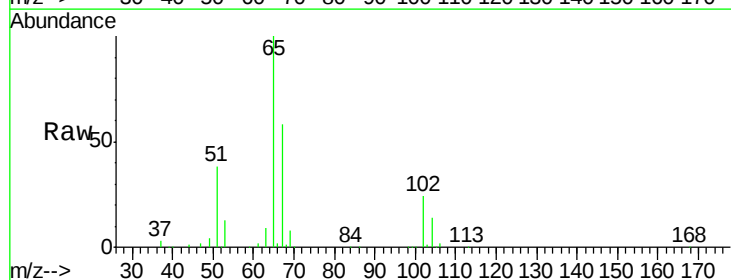

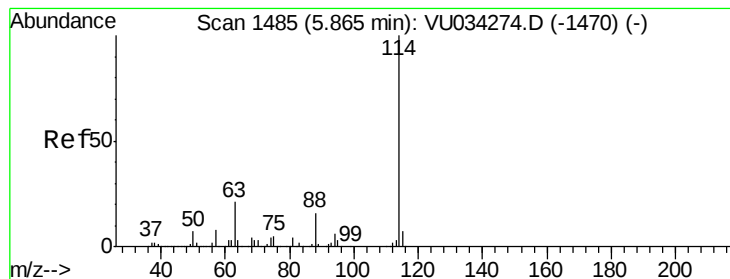

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 5.87 min Scan# 1486

Delta R.T. 0.00 min

Lab File: VU034456.D

Acq: 10 Sep 2019 17:07

Instrument :

MSVOA_U

ClientSampleId :

PAR-D4-(3.11)


Tot Ion:114 Resp: 355934

Ion Ratio Lower Upper

114 100

63 19.9 0.0 42.4




88 15.3 0.0 32.4

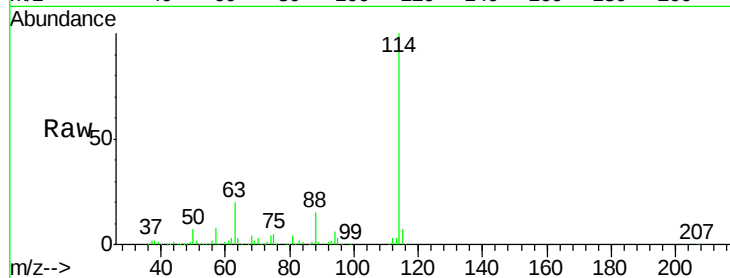

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VU0

Ion 87.90 (87.60 to 88.60): VU0

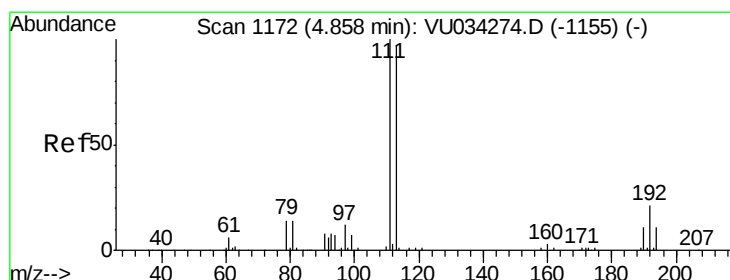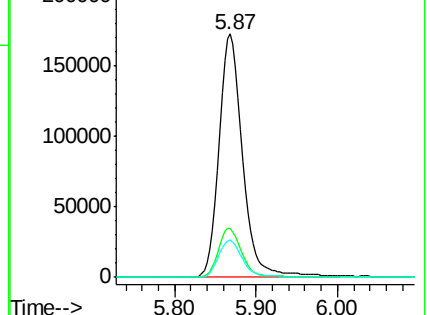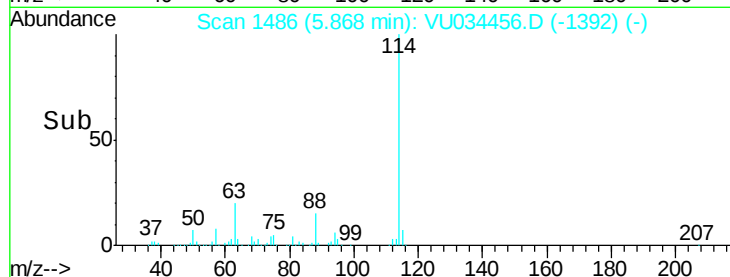

#35

Dibromofluoromethane

Concen: 50.588 ug/l

RT: 4.86 min Scan# 1173

Delta R.T. 0.00 min

Lab File: VU034456.D

Acq: 10 Sep 2019 17:07


Tgt Ion:113 Resp: 167546

Ion Ratio Lower Upper

113 100

111 103.1 81.5 122.3



192 21.5 17.8 26.8

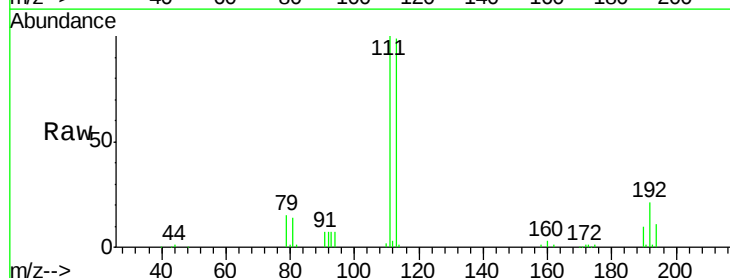


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

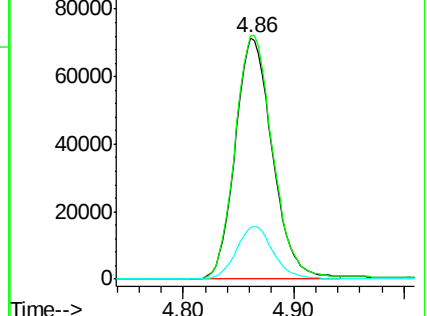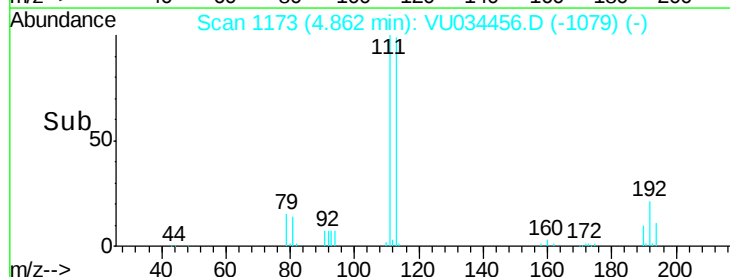

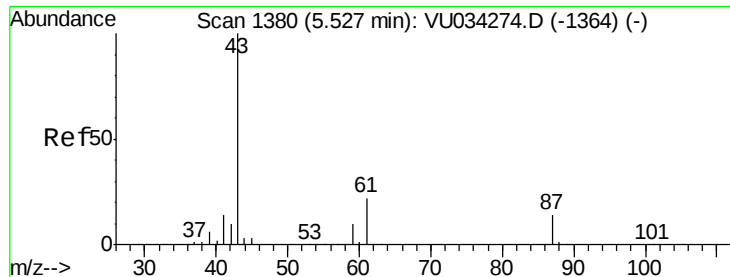

#43

Isopropyl Acetate

Concen: 8.094 ug/l

RT: 5.53 min Scan# 1382

Delta R.T. 0.01 min

Lab File: VU034456.D

Acq: 10 Sep 2019 17:07

Instrument :

MSVOA_U

ClientSampleId :

PAR-D4-(3.11)


Tot Ion: 43 Resp: 57626

Ion Ratio Lower Upper

43 100

61 21.4 17.1 25.7




87 14.5 11.1 16.7

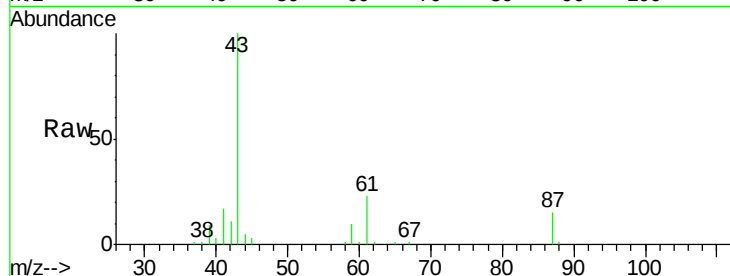

Abundance Ion 43.00 (42.70 to 43.70): VU034456.D (-1287) (-)

Ion 61.00 (60.70 to 61.70): VU034456.D (-1287) (-)

Ion 87.00 (86.70 to 87.70): VU034456.D (-1287) (-)

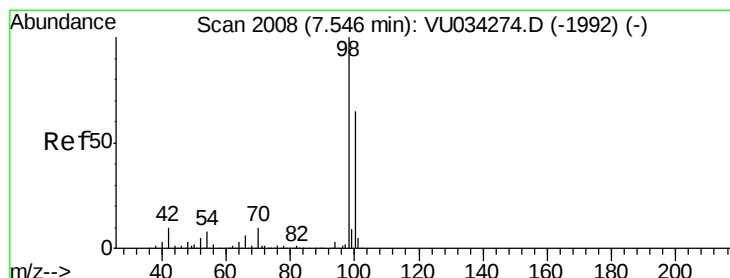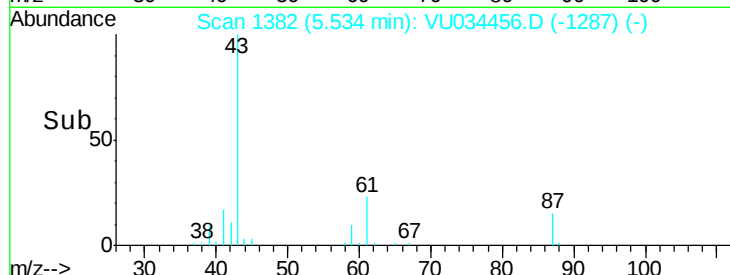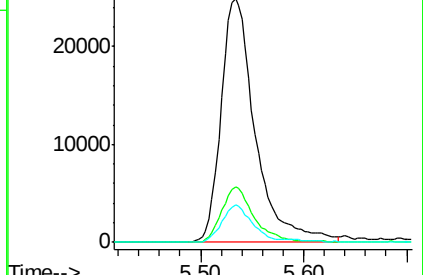

#50

Toluene-d8

Concen: 45.565 ug/l

RT: 7.55 min Scan# 2008

Delta R.T. -0.00 min

Lab File: VU034456.D


Acq: 10 Sep 2019 17:07

Tgt Ion: 98 Resp: 566969

Ion Ratio Lower Upper



98 100


100 64.9 51.7 77.5

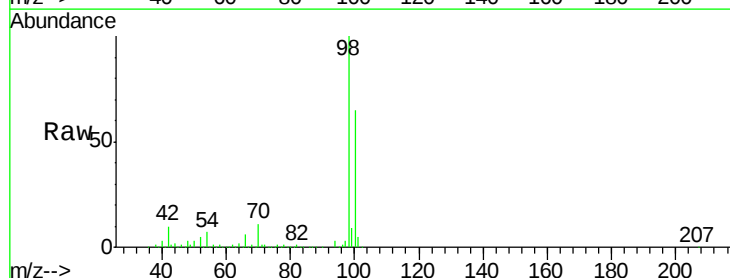

Abundance Ion 98.00 (97.70 to 98.70): VU034456.D (-1915) (-)

Ion 100.00 (99.70 to 100.70): VU034456.D (-1915) (-)

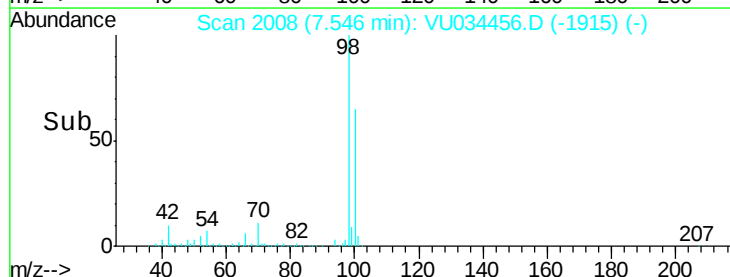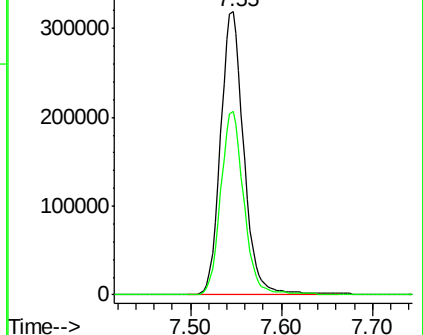

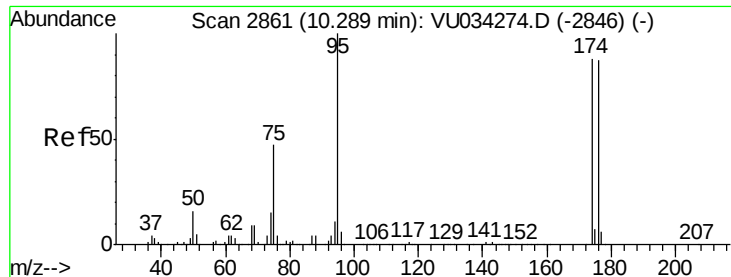

#62

4-Bromofluorobenzene

Concen: 39.505 ug/l

RT: 10.29 min Scan# 2860

Delta R.T. -0.00 min

Lab File: VU034456.D

Acq: 10 Sep 2019 17:07

Instrument :

MSVOA_U

ClientSampleId :

PAR-D4-(3.11)


Tot Ion: 95 Resp: 189790

Ion Ratio Lower Upper

95 100

174 89.5 0.0 175.2




176 84.2 0.0 168.0

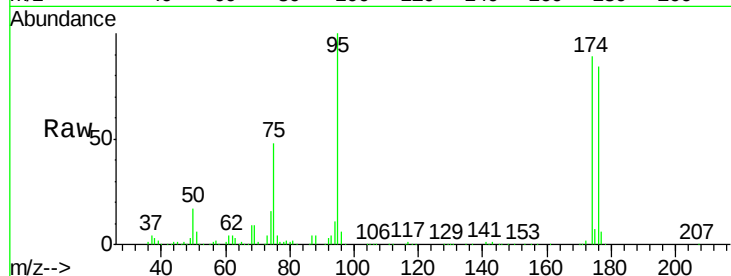

Abundance Ion 94.90 (94.60 to 95.60): VU034274.D (-2846) (-)

Ion 173.80 (173.50 to 174.50): VU034274.D (-2846) (-)

Ion 175.80 (175.50 to 176.50): VU034274.D (-2846) (-)

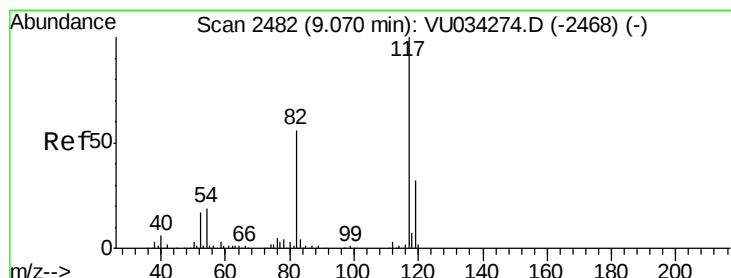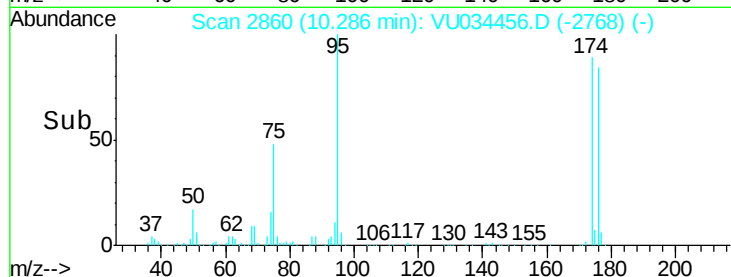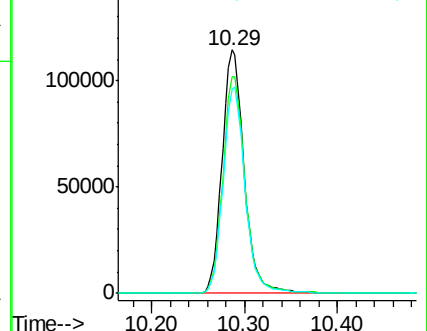

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 9.07 min Scan# 2482

Delta R.T. -0.00 min

Lab File: VU034456.D

Acq: 10 Sep 2019 17:07


Tgt Ion: 117 Resp: 365798

Ion Ratio Lower Upper

117 100

82 55.2 44.6 67.0



119 32.1 25.9 38.9

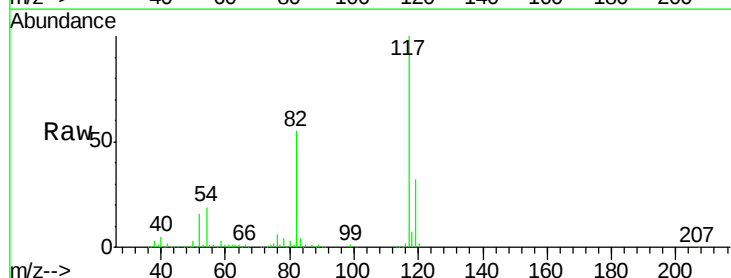


Abundance Ion 116.90 (116.60 to 117.60): VU034274.D (-2468) (-)

Ion 82.00 (81.70 to 82.70): VU034274.D (-2468) (-)

Ion 118.90 (118.60 to 119.60): VU034274.D (-2468) (-)

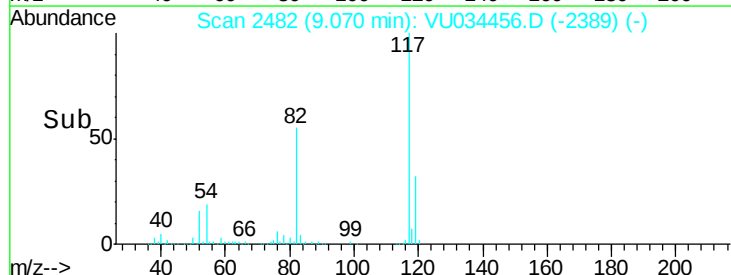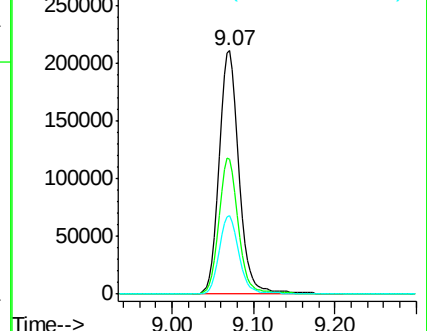

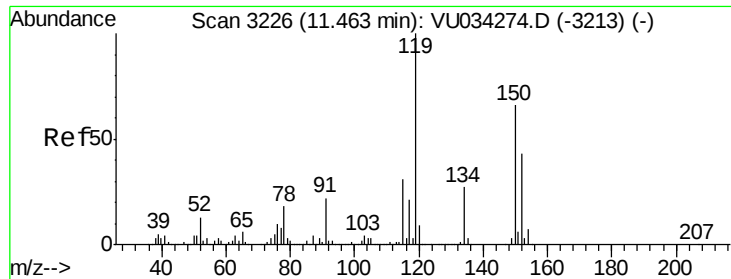

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 11.46 min Scan# 3226

Delta R.T. -0.00 min

Lab File: VU034456.D


Acq: 10 Sep 2019 17:07

Instrument :

MSVOA_U

ClientSampleId :

PAR-D4-(3.11)

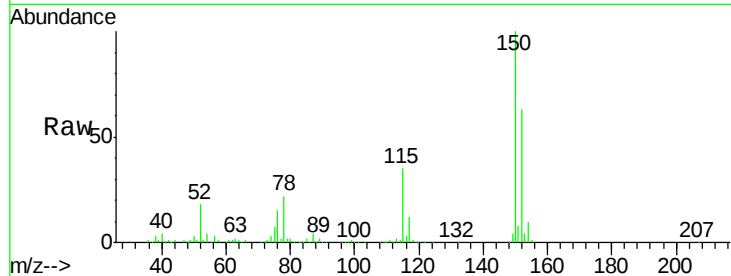

Tot Ion:	152	Resp:	187160
Ion	Ratio	Lower	Upper
152	100		
115	55.8	39.1	117.3
150	156.4	0.0	345.4

