


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU091019\  
 Data File : VU034434.D  
 Acq On : 10 Sep 2019 08:26  
 Operator : JC/SP  
 Sample : BFB  
 Misc : 5.0mL/MSVOA U/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\82U090619W.M  
 Title : SW846 8260  
 Last Update : Fri Sep 06 05:10:13 2019

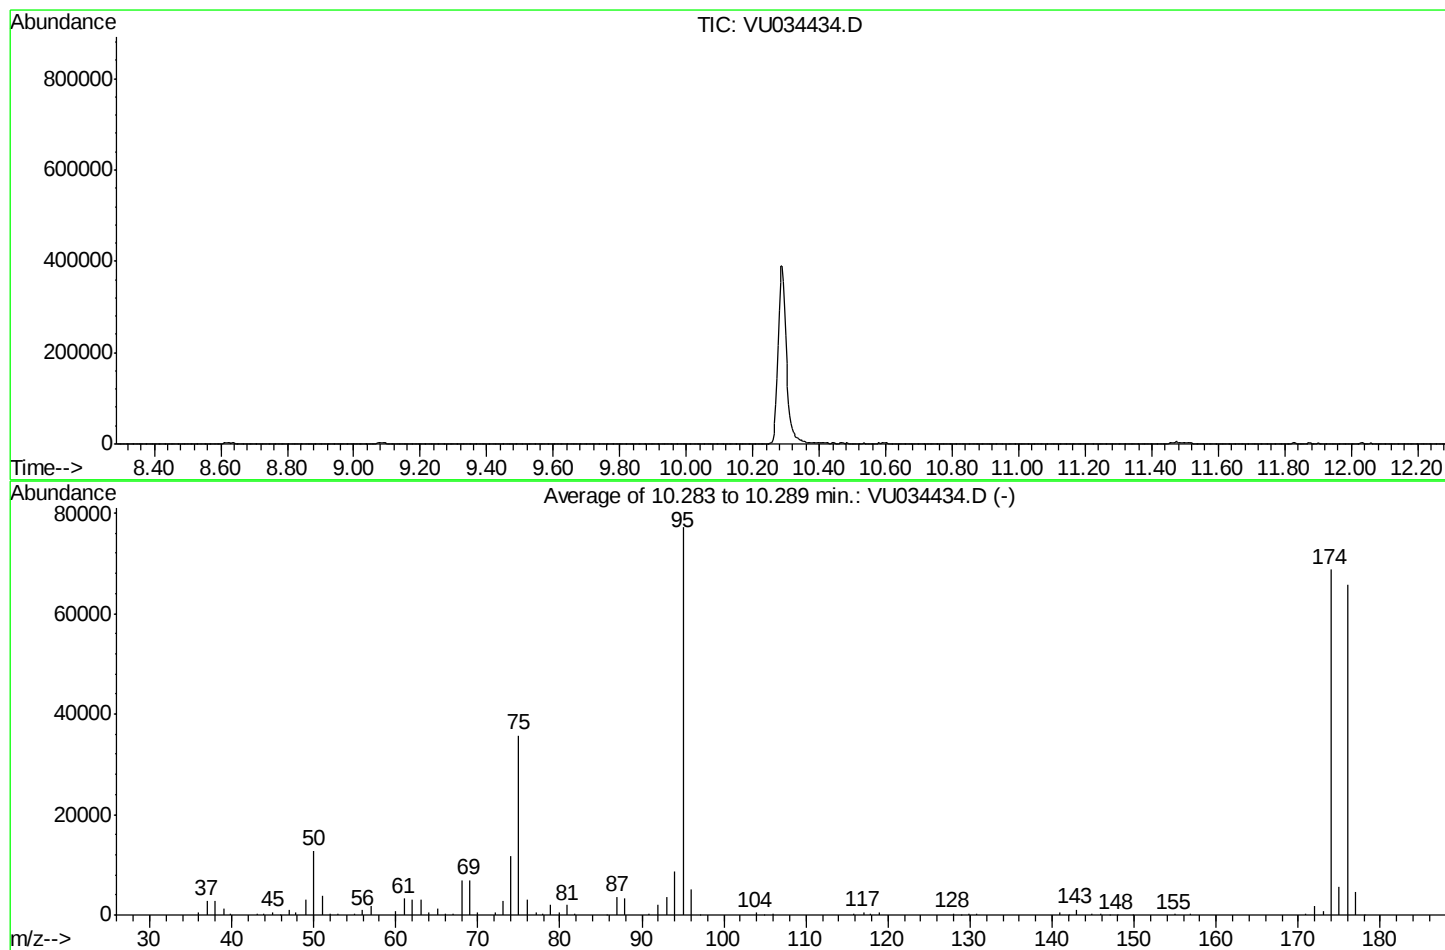

AutoFind: Scans 2859, 2860, 2861; Background Corrected with Scan 2847

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 16.5      | 12752   | PASS             |
| 75          | 95           | 30           | 60           | 46.2      | 35682   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 77178   | PASS             |
| 96          | 95           | 5            | 9            | 6.5       | 5016    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.3       | 871     | PASS             |
| 174         | 95           | 50           | 100          | 89.1      | 68757   | PASS             |
| 175         | 174          | 5            | 9            | 8.0       | 5499    | PASS             |
| 176         | 174          | 95           | 101          | 95.7      | 65784   | PASS             |
| 177         | 176          | 5            | 9            | 7.0       | 4620    | PASS             |