


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU091020\
 Data File : VU040070.D
 Acq On : 10 Sep 2020 09:17
 Operator : SY/MD
 Sample : BFB30
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB30

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Sep 11 10:50:33 2020

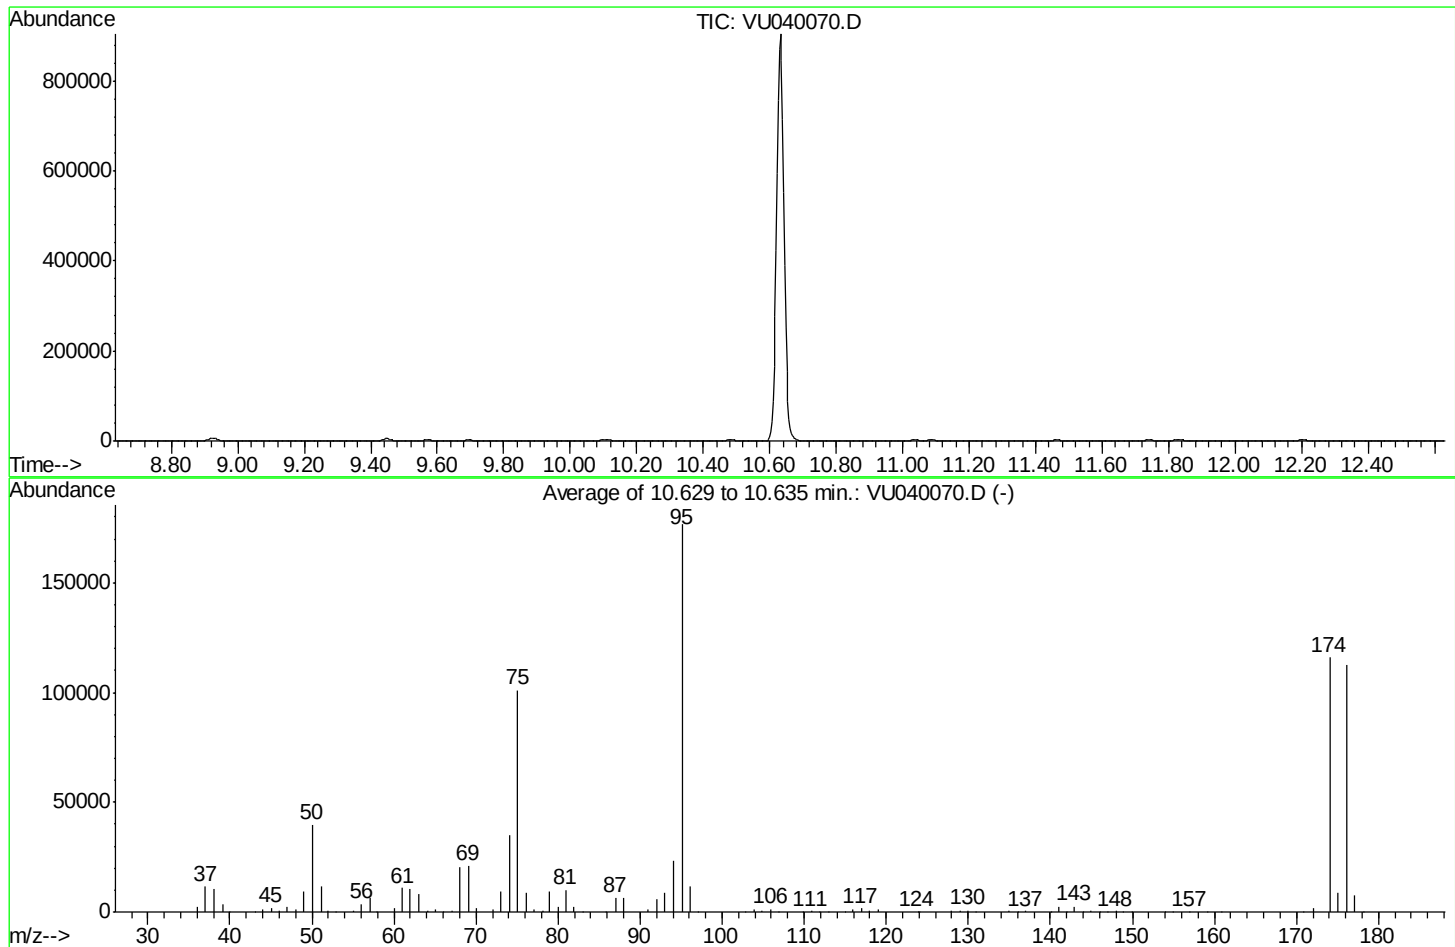

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.6	39965	PASS
75	95	30	80	57.2	100952	PASS
95	95	100	100	100.0	176640	PASS
96	95	5	9	6.6	11648	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	65.6	115920	PASS
175	174	5	9	7.4	8605	PASS
176	174	95	101	97.0	112464	PASS
177	176	5	9	6.7	7517	PASS

m/z	Abundance
36.00	2094.0
37.00	11460.0
38.00	10762.0
39.10	3846.0
40.00	235.0
44.00	1657.0
45.00	2019.0
45.90	328.0
47.00	2307.0
48.00	1441.0
49.00	9377.0
50.00	40152.0
51.10	11826.0
52.00	500.0
52.90	159.0
55.00	610.0
56.10	3755.0
57.10	6255.0
58.00	205.0
60.00	1849.0
61.00	11336.0
62.00	11184.0
63.00	8637.0
64.10	1085.0
65.10	1158.0
66.00	123.0
67.00	651.0
68.10	20896.0
69.00	21168.0
70.00	1454.0
72.00	1104.0
73.00	9830.0
74.10	35432.0
75.10	101416.0
76.10	8693.0
77.00	1112.0
78.10	566.0
79.00	9476.0
79.90	2729.0
80.90	10126.0
81.90	2206.0
83.00	234.0
87.10	6516.0
88.00	6262.0
91.00	1030.0
92.10	5719.0
93.00	8546.0
94.10	23480.0
95.10	176128.0
96.10	11797.0
97.00	281.0
102.80	108.0
103.90	1041.0
104.90	351.0
106.00	1091.0
106.90	207.0
109.80	152.0
110.90	459.0
111.90	172.0
113.00	287.0
115.00	310.0
115.90	868.0
117.00	1545.0
118.00	724.0
119.00	1238.0
123.90	144.0
128.00	644.0
128.90	359.0
130.00	642.0
130.90	241.0
134.90	354.0
137.00	352.0
140.10	134.0
141.00	2224.0
141.90	202.0
143.00	2471.0
144.00	178.0
145.00	390.0
146.00	283.0
148.10	376.0
148.90	147.0
149.90	240.0
154.90	286.0
157.00	333.0
159.10	169.0
160.80	122.0
170.80	217.0
172.10	1671.0
174.10	112808.0
175.10	8397.0
176.10	109912.0
177.10	7515.0

Instrument :
MSVOA_U
ClientSampleId :
BFB30

178.10

209.0

Instrument :
MSVOA_U
ClientSampleId :
BFB30

m/z	Abundance
36.10	2193.0
37.00	11901.0
38.00	10953.0
39.10	3850.0
39.90	275.0
43.00	115.0
44.00	1861.0
45.00	1983.0
45.90	343.0
47.00	2338.0
48.00	1434.0
49.00	9681.0
50.00	41456.0
51.10	12156.0
52.00	523.0
52.90	124.0
55.00	647.0
56.00	3758.0
57.10	6577.0
57.90	192.0
60.00	2003.0
61.00	11325.0
62.00	10910.0
63.00	8616.0
64.00	869.0
65.00	1111.0
66.00	105.0
67.10	595.0
68.10	21088.0
69.10	21696.0
70.00	1549.0
72.00	1238.0
73.00	9845.0
74.10	36216.0
75.10	104728.0
76.10	8906.0
77.00	1071.0
78.10	699.0
79.00	9649.0
80.00	2571.0
80.90	10386.0
81.90	2236.0
83.00	222.0
85.80	165.0
87.00	6636.0
88.00	6611.0
91.00	1120.0
92.10	5819.0
93.00	8906.0
94.10	24240.0
95.10	182528.0
96.10	12010.0
97.00	316.0
102.80	124.0
103.90	1163.0
104.90	340.0
106.00	1292.0
106.90	253.0
109.80	128.0
110.90	448.0
111.90	193.0
113.00	307.0
115.00	310.0
116.00	938.0
117.00	1643.0
117.90	755.0
119.00	1328.0
123.80	180.0
124.10	158.0
128.00	601.0
129.00	339.0
130.00	799.0
130.90	284.0
134.90	370.0
136.10	118.0
137.00	388.0
141.00	2521.0
141.90	222.0
143.00	2754.0
144.00	158.0
145.00	374.0
146.00	304.0
147.00	122.0
148.10	412.0
148.80	161.0
149.90	220.0
154.90	235.0
157.00	309.0
159.10	205.0
160.80	164.0
170.80	172.0
172.10	1569.0

Instrument :
MSVOA_U
ClientSampleId :
BFB30

174.10	119960.0
175.10	8860.0
176.10	116552.0
177.10	7803.0
178.20	187.0

Instrument :
MSVOA_U
ClientSampleId :
BFB30

m/z	Abundance
36.10	2164.0
37.00	10936.0
38.00	9886.0
39.10	3477.0
39.90	326.0
43.00	133.0
44.00	1882.0
45.10	1882.0
46.00	313.0
47.00	2213.0
48.00	1306.0
49.00	8977.0
50.00	38288.0
51.10	11268.0
52.00	486.0
55.00	611.0
56.00	3477.0
57.10	6037.0
58.00	180.0
60.00	2018.0
61.10	10091.0
62.00	9768.0
63.00	7847.0
64.00	721.0
65.00	969.0
67.10	518.0
68.00	19272.0
69.10	20192.0
70.10	1577.0
72.00	1218.0
73.10	8736.0
74.10	33376.0
75.10	96712.0
76.00	8210.0
77.00	959.0
78.10	736.0
78.90	8865.0
80.00	2297.0
80.90	9534.0
81.90	1987.0
83.00	256.0
87.00	6121.0
88.00	6378.0
90.90	1057.0
92.10	5462.0
93.00	8229.0
94.10	22328.0
95.10	171264.0
96.10	11137.0
97.00	288.0
102.90	148.0
103.90	1108.0
104.90	285.0
106.00	1328.0
106.90	252.0
109.80	107.0
110.90	324.0
111.90	173.0
113.00	288.0
115.00	266.0
116.00	920.0
117.00	1527.0
118.00	713.0
119.00	1282.0
123.80	190.0
127.90	541.0
129.00	295.0
130.00	848.0
131.00	289.0
134.90	319.0
137.00	377.0
141.00	2573.0
141.90	209.0
142.90	2691.0
144.00	110.0
145.00	351.0
145.90	286.0
147.00	141.0
148.00	399.0
148.70	131.0
150.00	190.0
154.00	102.0
155.00	270.0
157.00	286.0
159.10	189.0
160.90	183.0
170.70	128.0
172.10	1347.0
174.10	114992.0
175.10	8558.0
176.10	110928.0
177.10	7234.0

Instrument :
MSVOA_U
ClientSampleId :
BFB30

178.10

163.0

Instrument :
MSVOA_U
ClientSampleId :
BFB30

Scan 2875 (10.584 min): VU040070.D
BFB30

m/z	Abundance
39.90	183.0
43.90	352.0

Instrument :
MSVOA_U
ClientSampleId :
BFB30