


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091021\
Data File : VU044620.D
Acq On : 10 Sep 2021 13:49
Operator : SY/MD
Sample : M3712-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JCEP6

Manual Integrations
APPROVED

MMDadoda
9/13/2021 4:30:37 PM

Quant Time: Sep 11 00:26:44 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Sep 11 00:26:11 2021
Response via : Initial Calibration

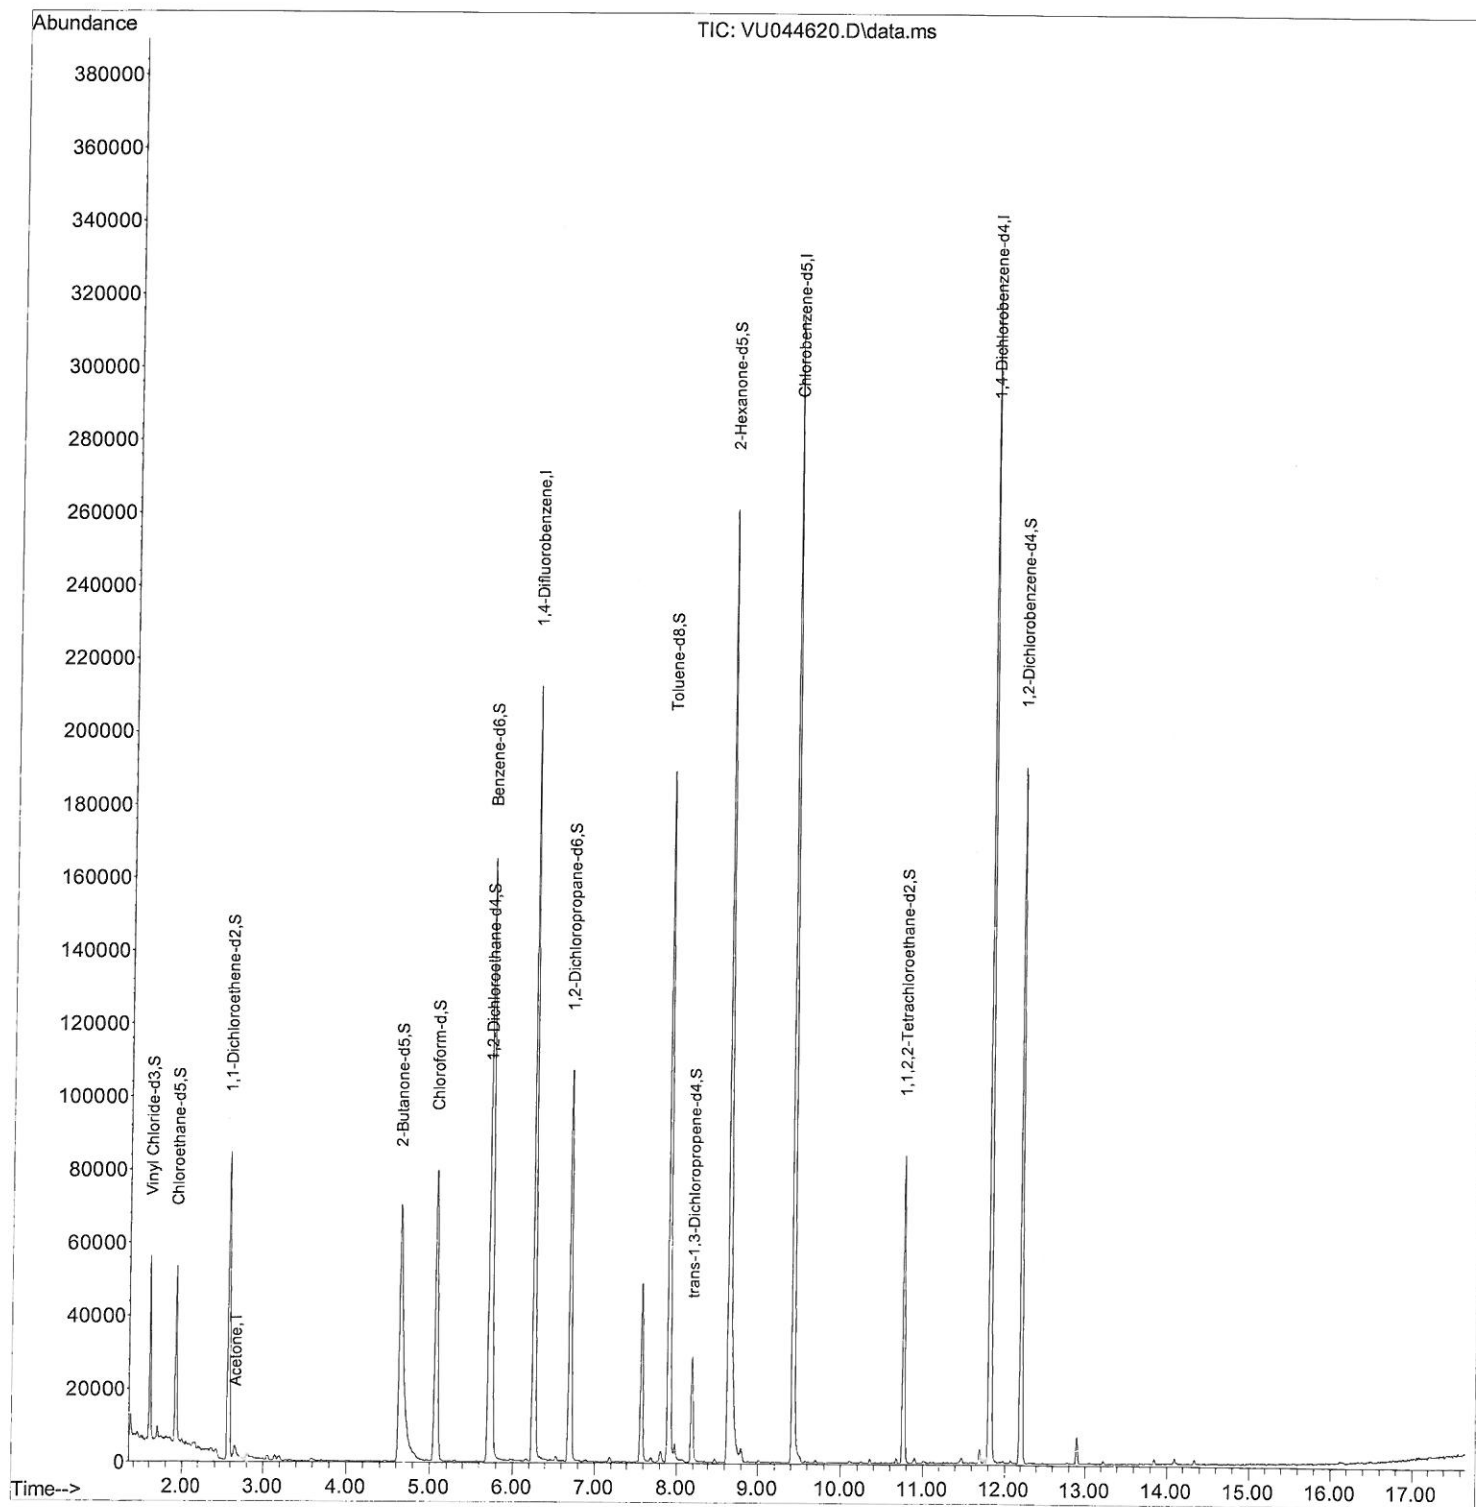

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091021\
 Data File : VU044620.D
 Acq On : 10 Sep 2021 13:49
 Operator : SY/MD
 Sample : M3712-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JCEP6

Manual Integrations
 APPROVED

MMDadoda
 9/13/2021 4:30:37 PM

Quant Time: Sep 11 00:26:44 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Sep 11 00:26:11 2021
 Response via : Initial Calibration

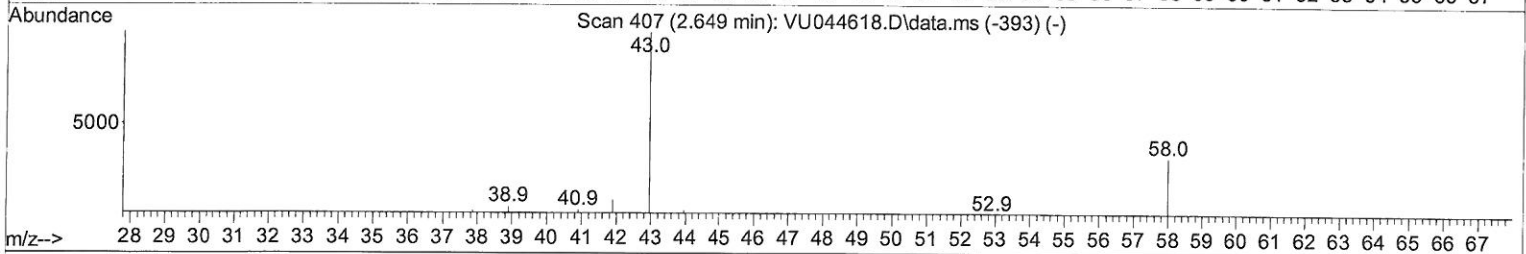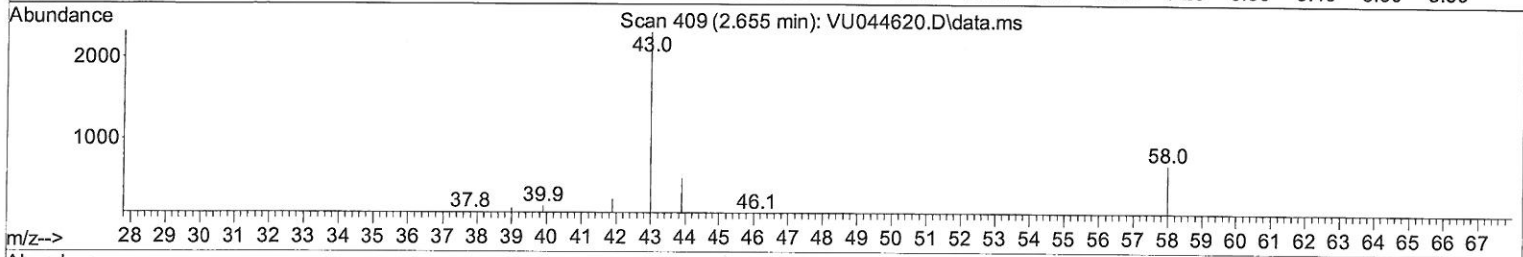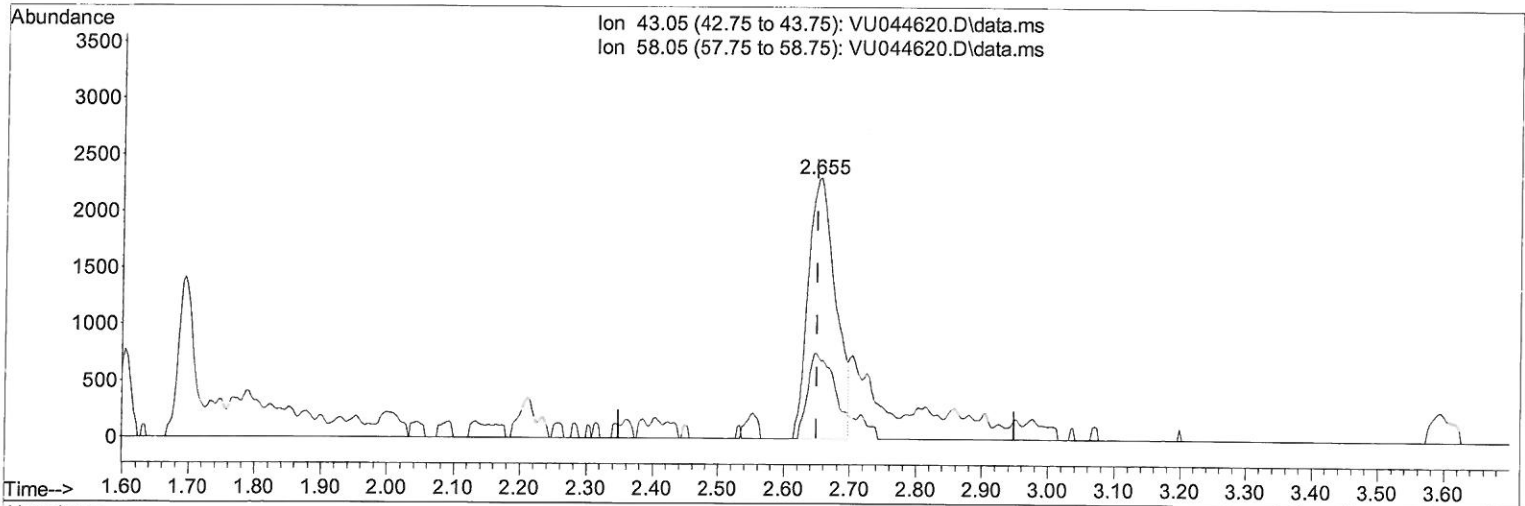

TIC: VU044620.D\data.ms

(13) Acetone (T)

2.655min (+ 0.006) 2.49 ug/L

response 6651

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	21.20	34.51
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091021\
Data File : VU044620.D
Acq On : 10 Sep 2021 13:49
Operator : SY/MD
Sample : M3712-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JCEP6

Manual Integrations
APPROVED

MMDadoda
9/13/2021 4:30:37 PM

Quant Time: Sep 11 00:26:44 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Sep 11 00:26:11 2021
Response via : Initial Calibration

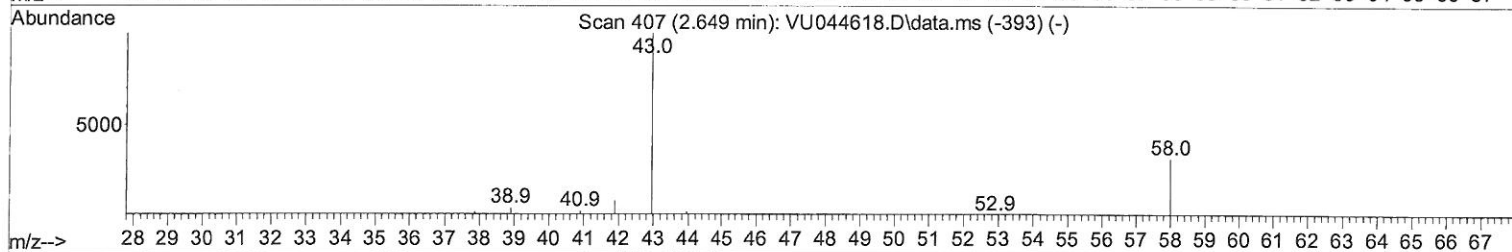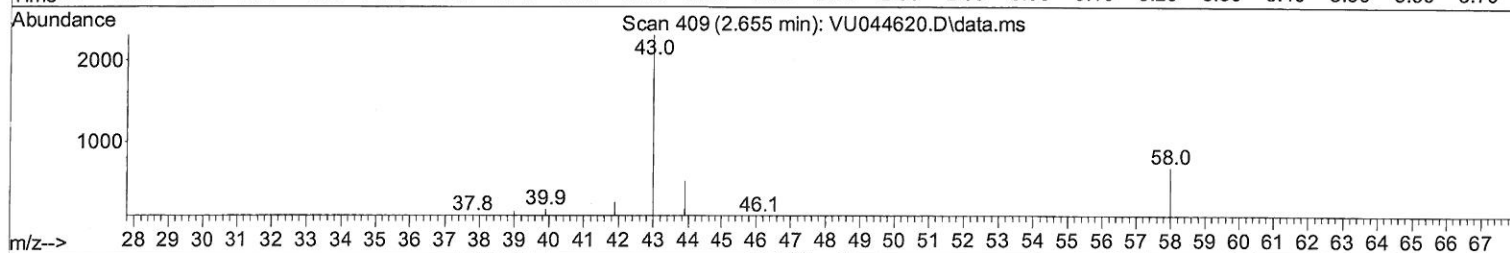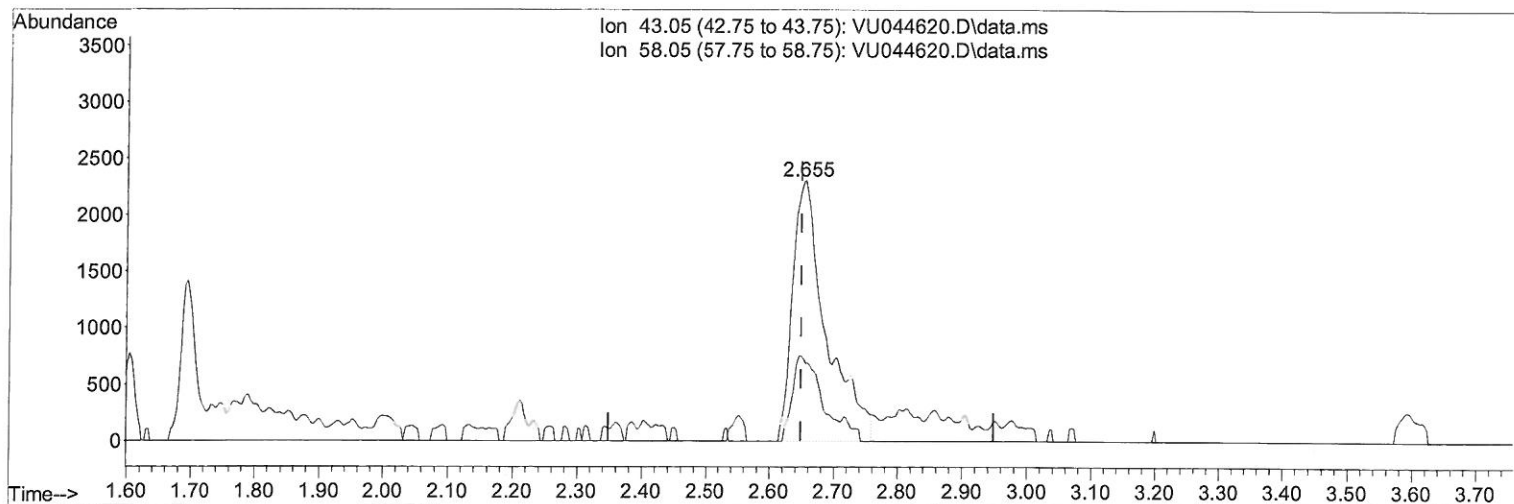

TIC: VU044620.D\data.ms

(13) Acetone (T)

2.655min (+ 0.006) 3.13 ug/L m

response 8349

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	21.20	27.49
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091021\
 Data File : VU044620.D
 Acq On : 10 Sep 2021 13:49
 Operator : SY/MD
 Sample : M3712-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JCEP6

Manual Integrations
 APPROVED

MMDadoda
 9/13/2021 4:30:37 PM

Quant Time: Sep 11 00:26:44 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Sep 11 00:26:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	165705	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	167154	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	80201	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	32858	3.361	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	67.200%		
7) Chloroethane-d5	1.919	69	35071	3.515	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	70.200%		
11) 1,1-Dichloroethene-d2	2.572	65	16295	3.300	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	66.000%		
20) 2-Butanone-d5	4.642	46	148370	36.201	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	72.400%		
24) Chloroform-d	5.073	84	74002	3.598	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	72.000%		
26) 1,2-Dichloroethane-d4	5.713	65	44228	3.607	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	72.200%		
32) Benzene-d6	5.736	84	148516	3.485	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	69.600%#		
36) 1,2-Dichloropropane-d6	6.700	67	50248	3.590	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	71.800%		
41) Toluene-d8	7.906	98	121474	3.274	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	65.400%#		
43) trans-1,3-Dichloroprop...	8.189	79	16608	3.366	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	67.400%		
46) 2-Hexanone-d5	8.645	63	109625	34.570	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	69.140%		
56) 1,1,2,2-Tetrachloroeth...	10.764	84	43111	3.474	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	69.400%		
66) 1,2-Dichlorobenzene-d4	12.198	152	46742	3.532	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	70.600%#		
Target Compounds						
13) Acetone	2.655	43	8349m	3.128	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed