

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091021\
 Data File : VU044620.D
 Acq On : 10 Sep 2021 13:49
 Operator : SY/MD
 Sample : M3712-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JCEP6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU044620.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.363	3	7	16	rVB3	6126	6512	1.12%	0.150%
2	1.601	74	81	96	rVB	50378	58771	10.08%	1.351%
3	1.919	172	180	193	rVB	47827	62166	10.66%	1.429%
4	2.575	372	384	397	rBV	84032	138596	23.77%	3.186%
5	2.649	397	407	439	rVB2	3574	11221	1.92%	0.258%
6	4.646	1012	1028	1077	rBV	70156	264304	45.34%	6.076%
7	5.073	1142	1161	1180	rBV	79457	181177	31.08%	4.165%
8	5.732	1346	1366	1390	rBV2	165231	433129	74.30%	9.957%
9	6.256	1515	1529	1549	rBV	212415	402870	69.11%	9.261%
10	6.700	1651	1667	1689	rBV	107141	212281	36.41%	4.880%
11	7.575	1926	1939	1957	rBV	48810	85866	14.73%	1.974%
12	7.906	2028	2042	2058	rBV	189364	330617	56.71%	7.600%
13	7.977	2058	2064	2080	rVB3	4403	7649	1.31%	0.176%
14	8.186	2118	2129	2150	rBV2	28795	51240	8.79%	1.178%
15	8.645	2259	2272	2312	rBV	261088	582977	100.00%	13.401%
16	8.796	2312	2319	2331	rVB5	3816	7496	1.29%	0.172%
17	9.423	2502	2514	2547	rBV	314855	532892	91.41%	12.250%
18	10.764	2916	2931	2950	rBV	84120	137420	23.57%	3.159%
19	11.819	3246	3259	3278	rBV	324250	520989	89.37%	11.976%
20	12.198	3363	3377	3396	rBV	190638	311790	53.48%	7.167%
21	12.896	3587	3594	3606	rVB4	7270	10141	1.74%	0.233%




Sum of corrected areas: 4350104

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091021\
Data File : VU044620.D
Acq On : 10 Sep 2021 13:49
Operator : SY/MD
Sample : M3712-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JCEP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

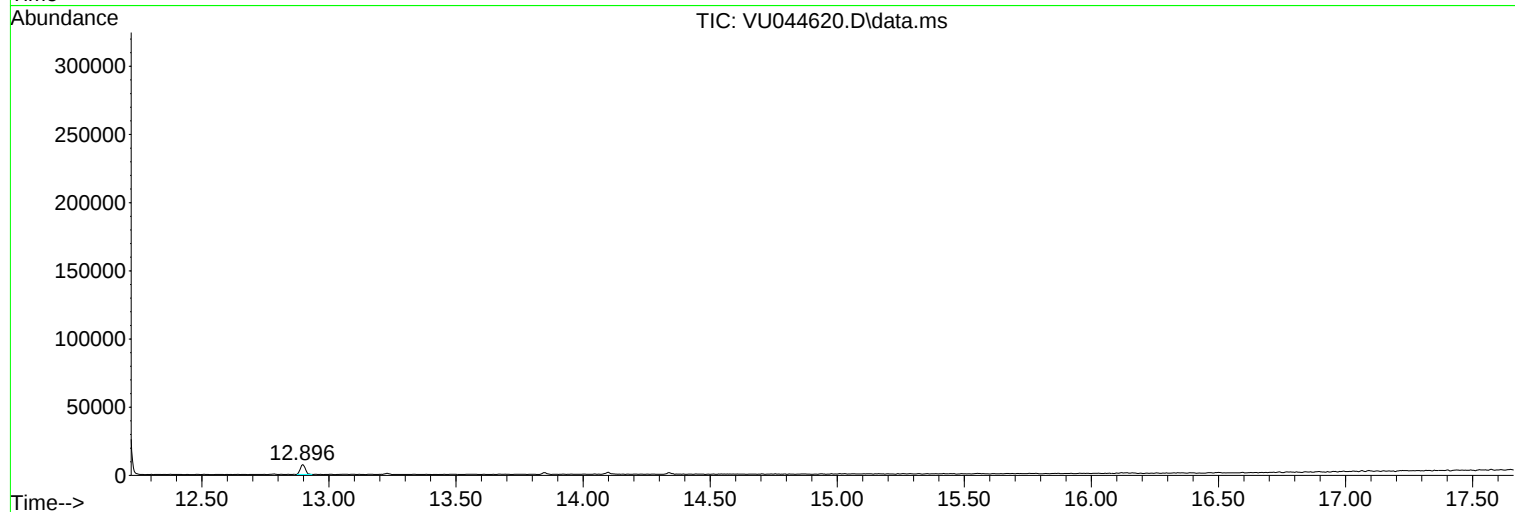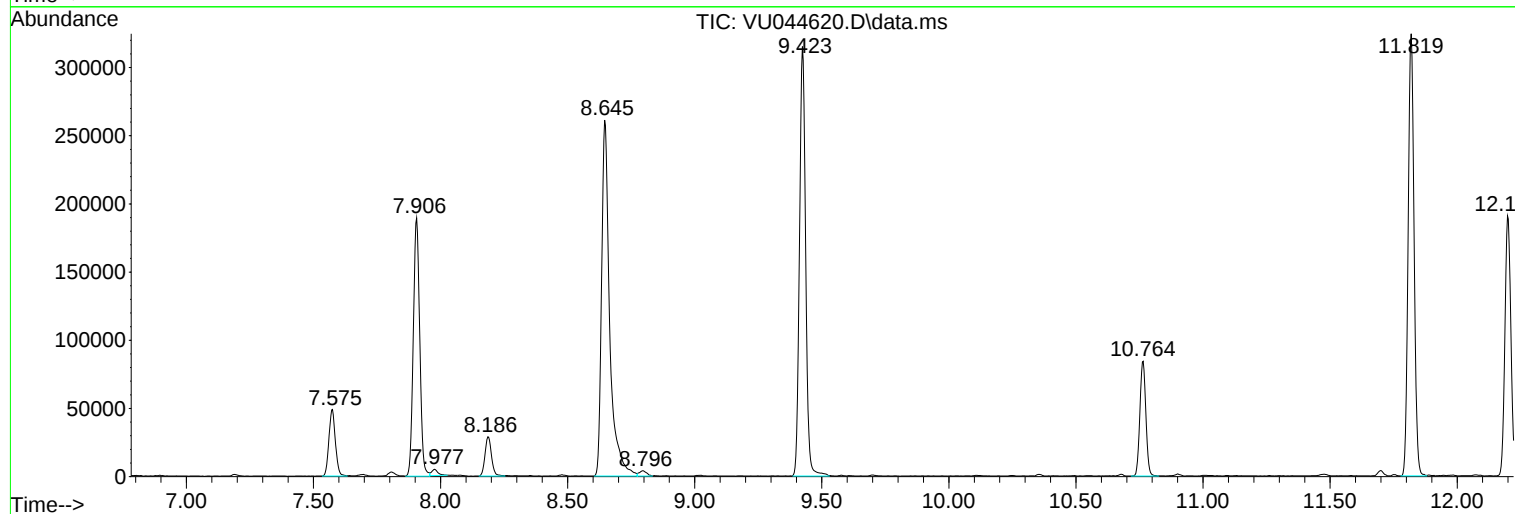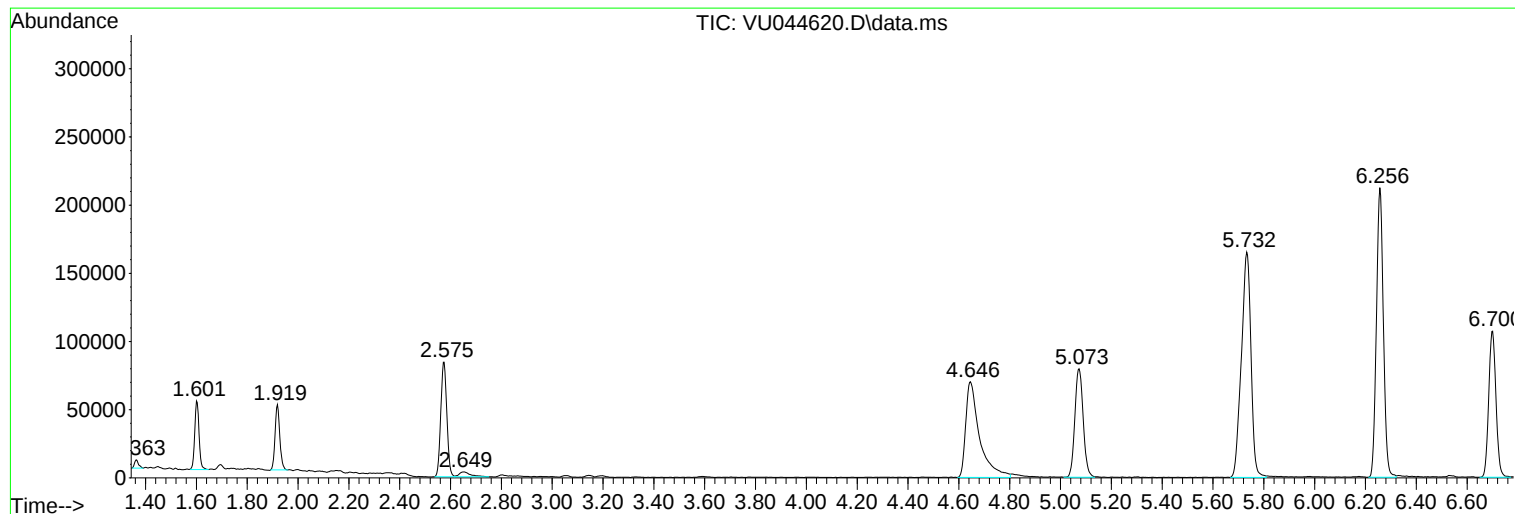

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091021\
Data File : VU044620.D
Acq On : 10 Sep 2021 13:49
Operator : SY/MD
Sample : M3712-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JCEP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091021\
Data File : VU044620.D
Acq On : 10 Sep 2021 13:49
Operator : SY/MD
Sample : M3712-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JCEP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
