


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091021\
 Data File : VU044617.D
 Acq On : 10 Sep 2021 08:46
 Operator : SY/MD
 Sample : BFB016
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB016

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Sep 11 00:26:11 2021

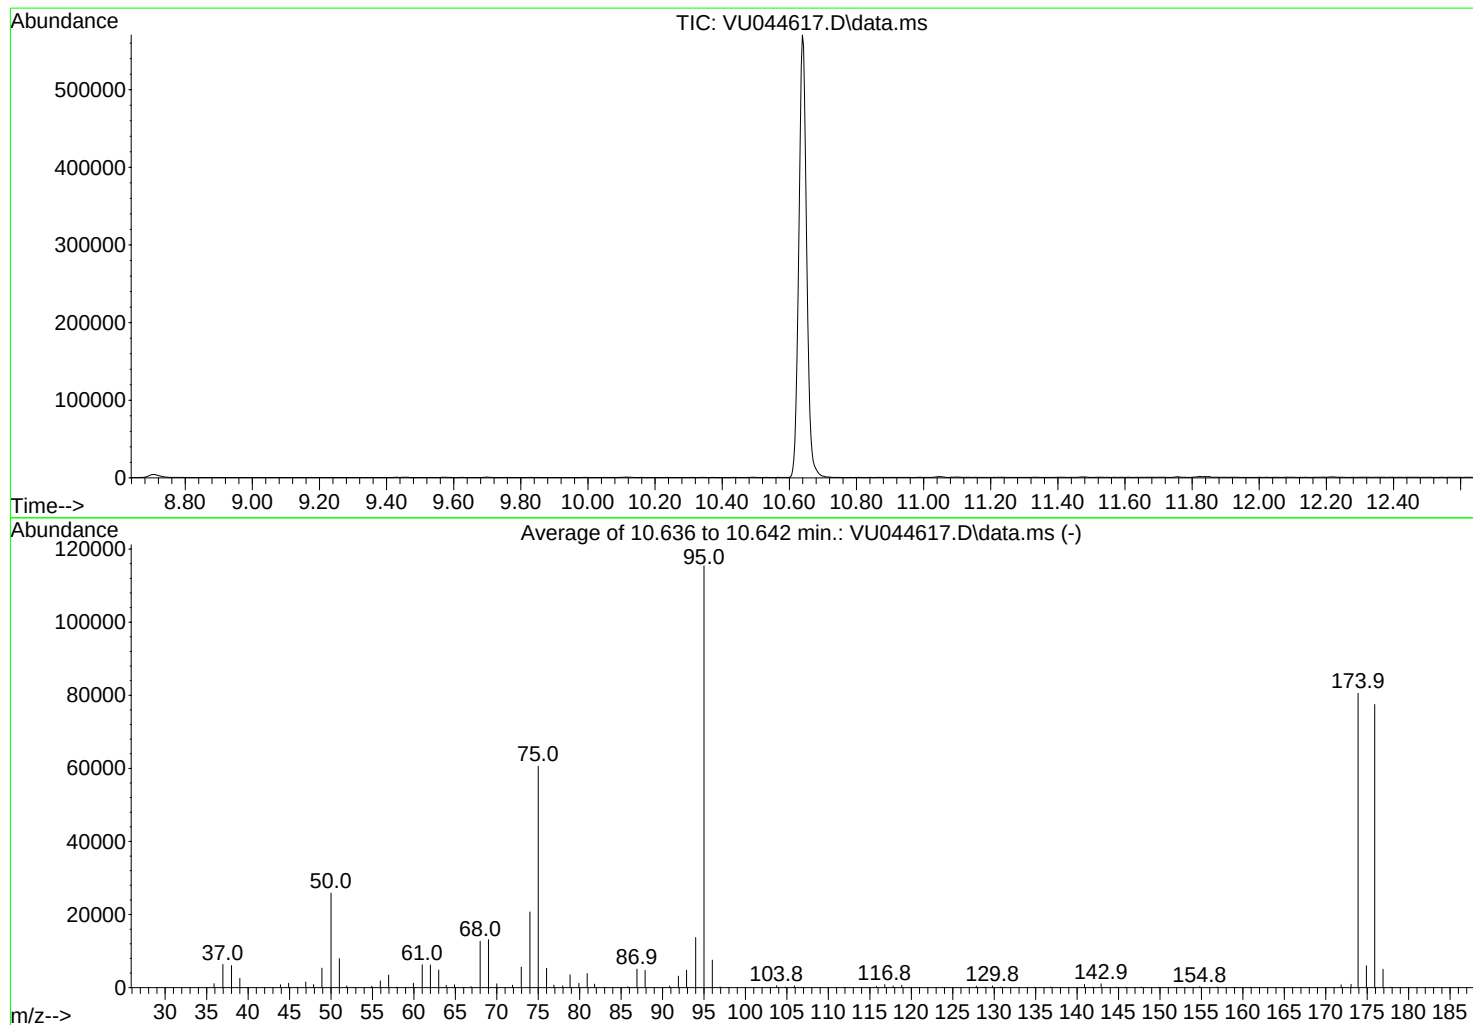

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	25861	PASS
75	95	30	80	52.5	60592	PASS
95	95	100	100	100.0	115416	PASS
96	95	5	9	6.5	7528	PASS
173	174	0.00	2	1.1	920	PASS
174	95	50	120	69.8	80576	PASS
175	174	5	9	7.4	5996	PASS
176	174	95	101	96.2	77480	PASS
177	176	5	9	6.5	5053	PASS

m/z	Abundance
39.80	237.0
43.90	332.0

Instrument :
MSVOA_U
ClientSampleId :
BFB016

m/z	Abundance
35.90	1086.0
36.90	6213.0
38.00	5969.0
39.00	2441.0
39.90	298.0
43.90	1179.0
44.90	1175.0
45.90	152.0
47.00	1614.0
47.90	828.0
48.90	5220.0
50.00	25376.0
51.00	7922.0
51.90	456.0
52.80	130.0
54.90	398.0
56.00	1813.0
57.00	3387.0
57.90	138.0
59.90	1229.0
61.00	6187.0
62.00	6276.0
63.00	4596.0
63.90	567.0
64.90	791.0
65.90	129.0
66.90	283.0
68.00	12539.0
69.00	12660.0
70.00	1067.0
71.90	623.0
73.00	5414.0
74.00	20096.0
75.00	58440.0
76.00	5166.0
76.90	706.0
77.90	478.0
78.90	3325.0
79.90	1179.0
80.90	3727.0
81.80	940.0
85.80	210.0
86.90	4953.0
87.90	4634.0
90.80	515.0
91.90	2907.0
92.90	4737.0
94.00	13091.0
95.00	110648.0
96.00	7269.0
96.90	227.0
103.70	496.0
104.80	159.0
105.90	431.0
111.90	103.0
114.80	114.0
115.80	383.0
116.80	765.0
117.80	390.0
118.90	593.0
123.80	102.0
127.80	419.0
128.90	179.0
129.80	424.0
130.80	159.0
134.90	115.0
136.80	156.0
140.90	850.0
141.90	109.0
142.90	1052.0
144.80	190.0
145.80	127.0
147.80	171.0
149.80	127.0
154.80	291.0
156.90	163.0
158.90	102.0
160.90	100.0
171.80	734.0
173.10	876.0
173.90	76064.0
174.90	5662.0
175.90	72560.0
176.90	4694.0
177.90	120.0

Instrument :
MSVOA_U
ClientSampleId :
BFB016

m/z	Abundance
35.90	1139.0
36.90	6501.0
38.00	6247.0
39.00	2641.0
39.90	277.0
43.90	1167.0
44.90	1184.0
45.90	169.0
46.90	1571.0
47.90	877.0
48.90	5523.0
50.00	26688.0
51.00	8186.0
51.90	496.0
52.90	118.0
54.90	410.0
56.00	1909.0
57.00	3592.0
57.90	140.0
60.00	1278.0
61.00	6438.0
62.00	6407.0
63.00	4943.0
63.90	659.0
64.90	793.0
65.90	135.0
66.90	311.0
68.00	13028.0
69.00	13632.0
70.00	1060.0
71.90	695.0
72.90	5860.0
74.00	21336.0
75.00	62424.0
76.00	5501.0
76.90	750.0
78.00	474.0
78.90	3602.0
79.90	1235.0
80.90	3968.0
81.80	992.0
82.90	105.0
85.80	260.0
86.90	5251.0
87.90	4892.0
90.90	478.0
91.90	3204.0
92.90	4924.0
94.00	14133.0
95.00	119184.0
96.00	7770.0
96.90	233.0
103.80	533.0
104.80	166.0
105.90	478.0
106.80	122.0
111.90	111.0
114.80	116.0
115.80	404.0
116.80	843.0
117.80	429.0
118.80	675.0
123.80	105.0
127.80	445.0
128.90	161.0
129.80	491.0
130.80	182.0
134.80	136.0
136.80	198.0
140.90	901.0
141.80	105.0
142.90	1114.0
144.80	172.0
145.90	133.0
147.80	196.0
149.80	117.0
154.80	313.0
156.90	185.0
158.90	108.0
160.90	130.0
171.80	785.0
173.00	937.0
173.90	83272.0
174.90	6155.0
175.90	80024.0
176.90	5285.0
177.90	127.0

Instrument :
MSVOA_U
ClientSampleId :
BFB016

m/z	Abundance
35.90	1087.0
37.00	6335.0
38.00	5954.0
39.00	2526.0
39.90	262.0
43.90	1075.0
44.90	1164.0
45.90	145.0
46.90	1424.0
47.90	848.0
48.90	5349.0
50.00	25520.0
51.00	7703.0
51.90	449.0
54.90	367.0
55.90	1822.0
56.90	3462.0
57.90	162.0
60.00	1176.0
61.00	6211.0
62.00	5999.0
63.00	4880.0
63.90	649.0
64.90	722.0
65.90	110.0
66.90	337.0
68.00	12467.0
69.00	13066.0
70.00	980.0
71.90	685.0
72.90	5692.0
74.00	20704.0
75.00	60912.0
76.00	5274.0
76.90	695.0
77.90	458.0
78.80	3586.0
79.90	1122.0
80.90	3883.0
81.80	942.0
82.90	106.0
85.80	262.0
86.90	5071.0
87.90	4664.0
90.80	369.0
91.90	3328.0
92.90	4698.0
94.00	13835.0
95.00	116416.0
96.00	7545.0
97.00	210.0
103.80	538.0
104.80	186.0
105.90	488.0
106.80	113.0
111.80	108.0
114.90	103.0
115.80	427.0
116.80	867.0
117.80	441.0
118.80	664.0
127.90	402.0
128.90	149.0
129.80	489.0
130.80	177.0
134.80	163.0
136.80	227.0
140.90	871.0
142.90	1022.0
144.70	168.0
145.80	143.0
147.80	201.0
149.80	104.0
154.80	301.0
156.90	165.0
158.80	117.0
160.90	126.0
171.90	810.0
173.00	947.0
173.90	82392.0
174.90	6172.0
175.90	79856.0
176.90	5181.0
177.80	132.0

Instrument :
MSVOA_U
ClientSampleId :
BFB016