

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091024\
 Data File : VU060673.D
 Acq On : 10 Sep 2024 17:53
 Operator : MD/SY
 Sample : P3918-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Quant Time: Sep 11 02:49:59 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Sep 11 02:46:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	105139	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	112799	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.808	152	46501	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	24618	5.301	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	106.000%
7) Chloroethane-d5	1.911	69	25482	3.622	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	72.400%
11) 1,1-Dichloroethene-d2	2.560	65	11555	4.222	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.400%
20) 2-Butanone-d5	4.637	46	63021	39.465	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	78.920%
24) Chloroform-d	5.055	84	66419	5.017	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.400%
26) 1,2-Dichloroethane-d4	5.695	65	35825	5.186	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.800%
32) Benzene-d6	5.721	84	120850	4.899	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.000%
36) 1,2-Dichloropropane-d6	6.682	67	41620	5.230	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.600%
41) Toluene-d8	7.891	98	102702	4.438	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.800%
43) trans-1,3-Dichloroprop...	8.178	79	12905	4.532	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.600%
46) 2-Hexanone-d5	8.631	63	49446	36.264	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	72.520%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	30527	4.311	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.200%
66) 1,2-Dichlorobenzene-d4	12.187	152	36465	5.318	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.400%
Target Compounds						
					Qvalue	
16) Methylene chloride	3.046	84	3632	0.434	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091024\
Data File : VU060673.D
Acq On : 10 Sep 2024 17:53
Operator : MD/SY
Sample : P3918-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001


Quant Time: Sep 11 02:49:59 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Sep 11 02:46:13 2024
Response via : Initial Calibration

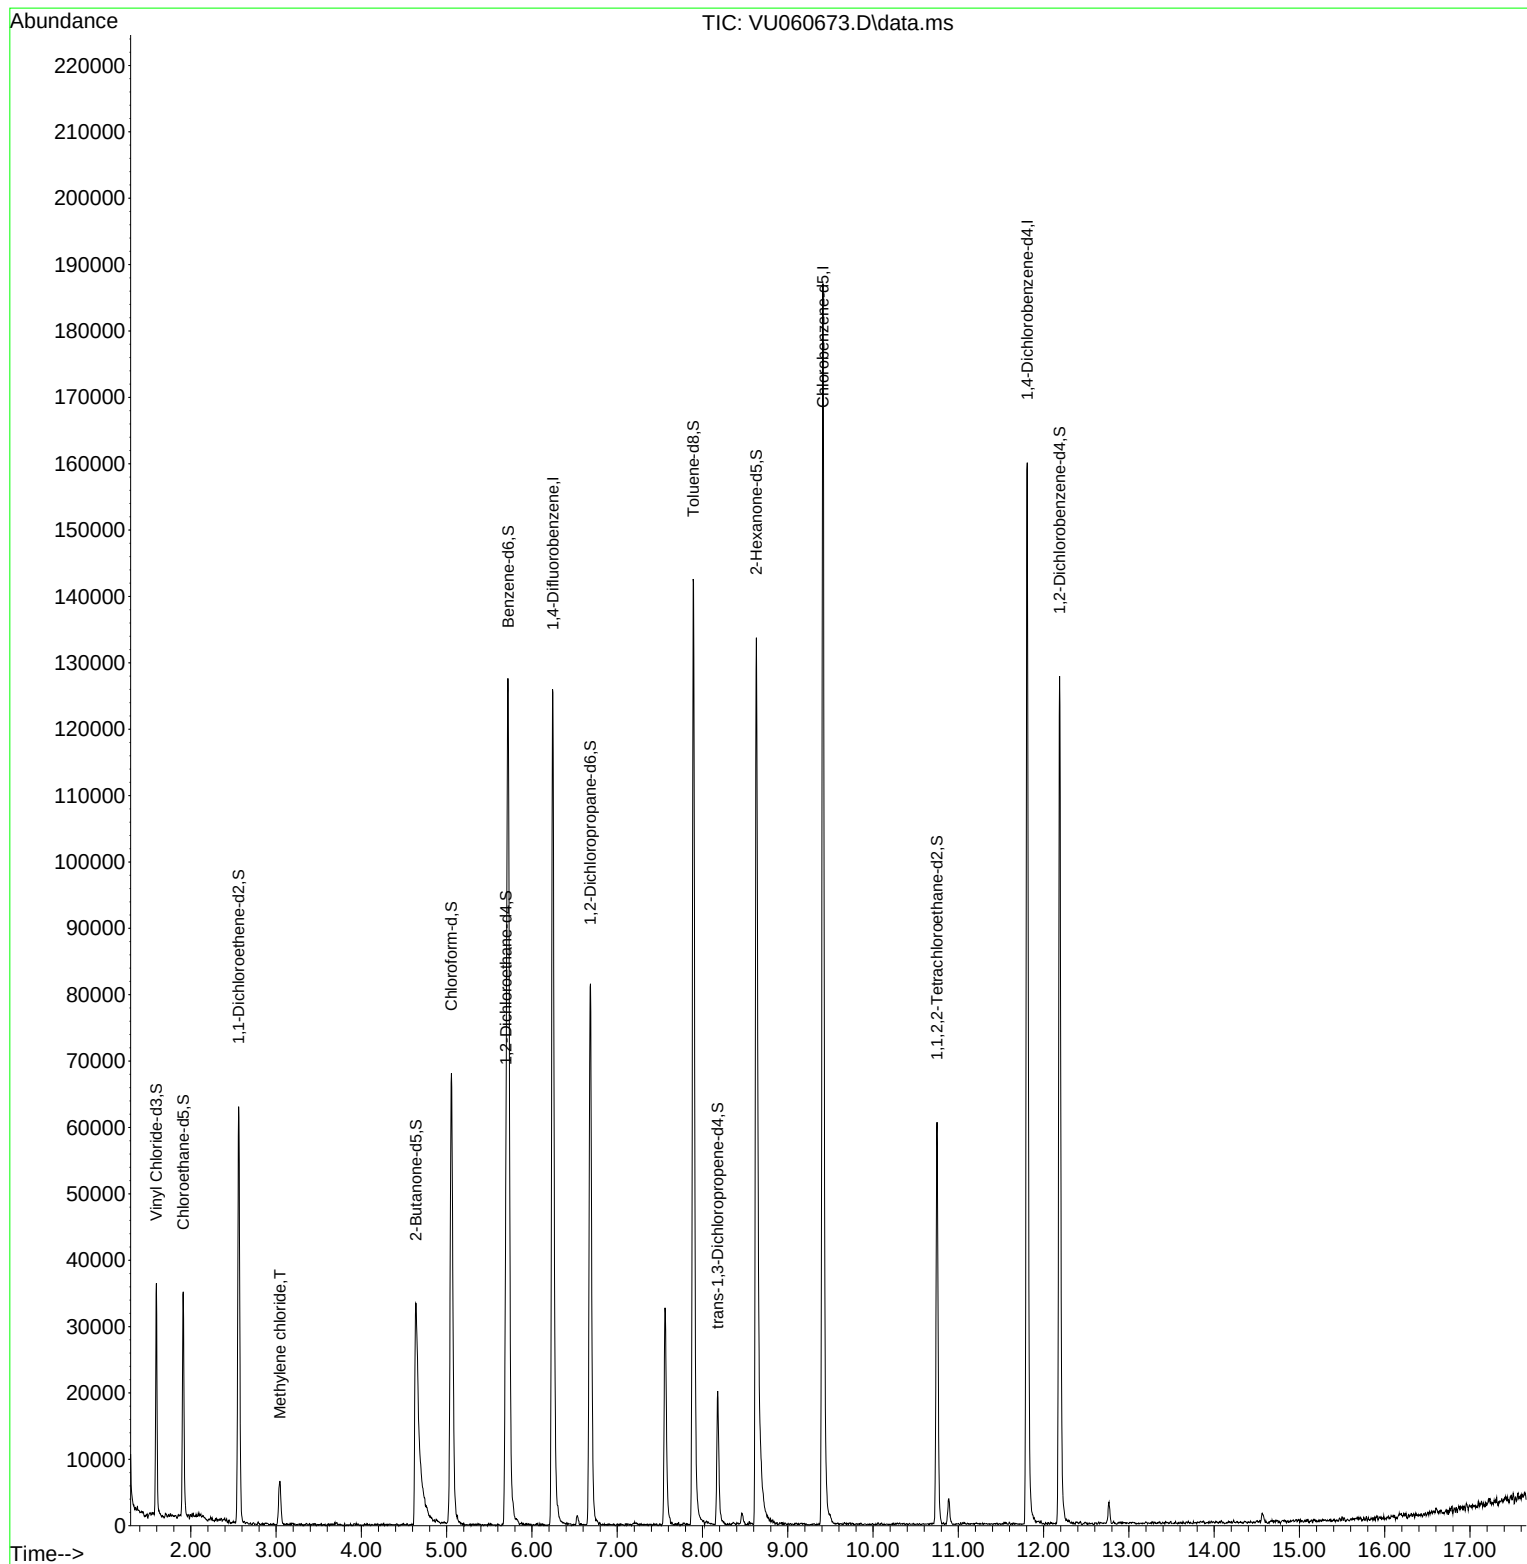

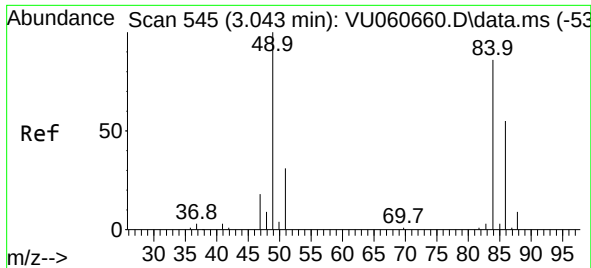

#16
Methylene chloride
Concen: 0.434 ug/L
RT: 3.046 min Scan# 54
Delta R.T. 0.003 min
Lab File: VU060673.D
Acq: 10 Sep 2024 17:53

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

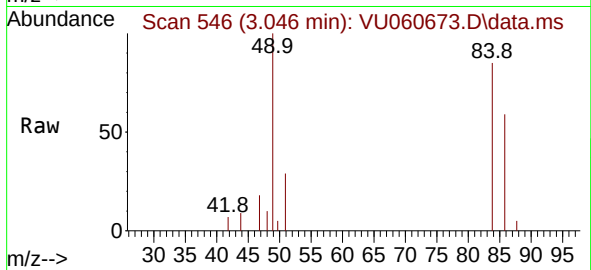

Tgt Ion: 84 Resp: 3632

Ion	Ratio	Lower	Upper
84	100		
86	69.2	47.5	88.3
49	124.1	94.4	175.2

