

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091024\
 Data File : VU060671.D
 Acq On : 10 Sep 2024 17:04
 Operator : MD/SY
 Sample : VIBLK132
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK132

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU060671.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	81	95	107	rVB	32044	37153	11.42%	1.392%
2	1.911	184	193	208	rBV	32157	43879	13.49%	1.644%
3	2.560	384	395	410	rBV	60390	97001	29.83%	3.634%
4	3.039	531	544	560	rBV2	9511	18514	5.69%	0.694%
5	4.634	1030	1040	1070	rBV2	33799	108357	33.32%	4.059%
6	5.055	1156	1171	1195	rBV2	66262	148129	45.55%	5.549%
7	5.718	1359	1377	1403	rBV2	123837	325220	100.00%	12.184%
8	6.242	1526	1540	1567	rBV	113324	225557	69.36%	8.450%
9	6.685	1665	1678	1696	rBV	76863	156444	48.10%	5.861%
10	7.560	1937	1950	1972	rBV	31798	58436	17.97%	2.189%
11	7.891	2042	2053	2072	rBV	137615	249431	76.70%	9.345%
12	8.177	2132	2142	2159	rBV2	18598	33974	10.45%	1.273%
13	8.467	2221	2232	2242	rBV3	2144	3515	1.08%	0.132%
14	8.631	2272	2283	2317	rBV	132754	282384	86.83%	10.579%
15	9.412	2514	2526	2551	rBV	172236	303321	93.27%	11.363%
16	10.750	2931	2942	2959	rBV	58372	97484	29.97%	3.652%
17	10.888	2974	2985	2997	rVB2	5326	8234	2.53%	0.308%
18	11.807	3258	3271	3294	rBV	148044	253841	78.05%	9.510%
19	12.187	3377	3389	3411	rBV	121514	214260	65.88%	8.027%
20	12.762	3559	3568	3570	rBV5	3579	4132	1.27%	0.155%




Sum of corrected areas: 2669266

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091024\
Data File : VU060671.D
Acq On : 10 Sep 2024 17:04
Operator : MD/SY
Sample : VIBLK132
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK132

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

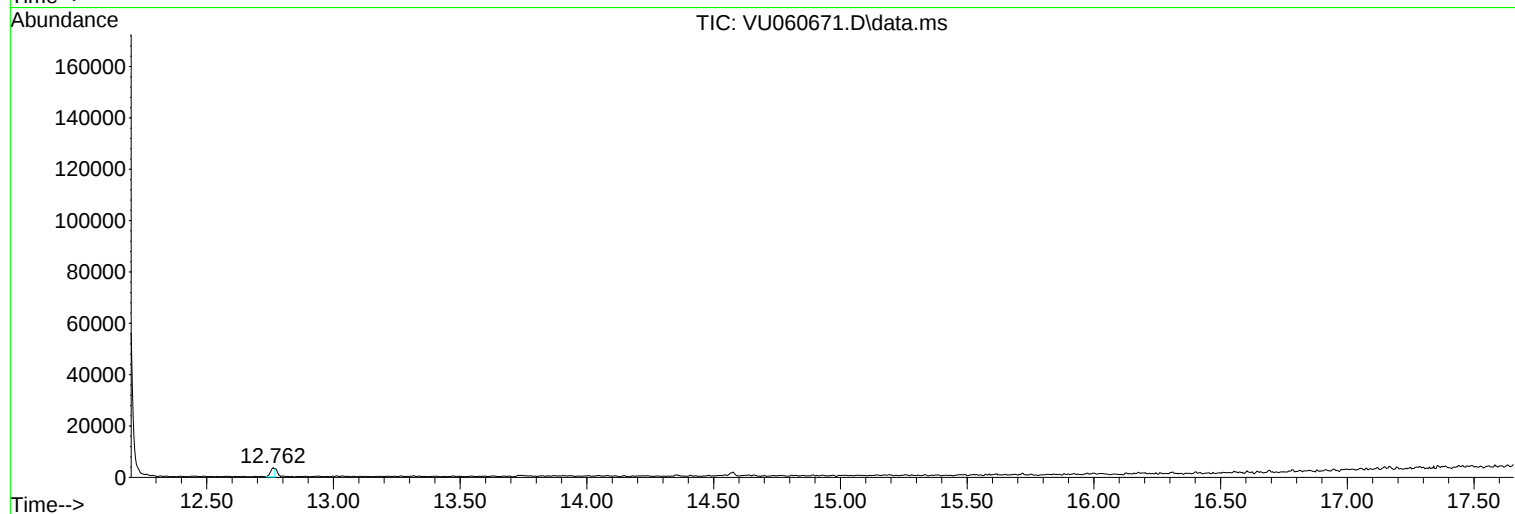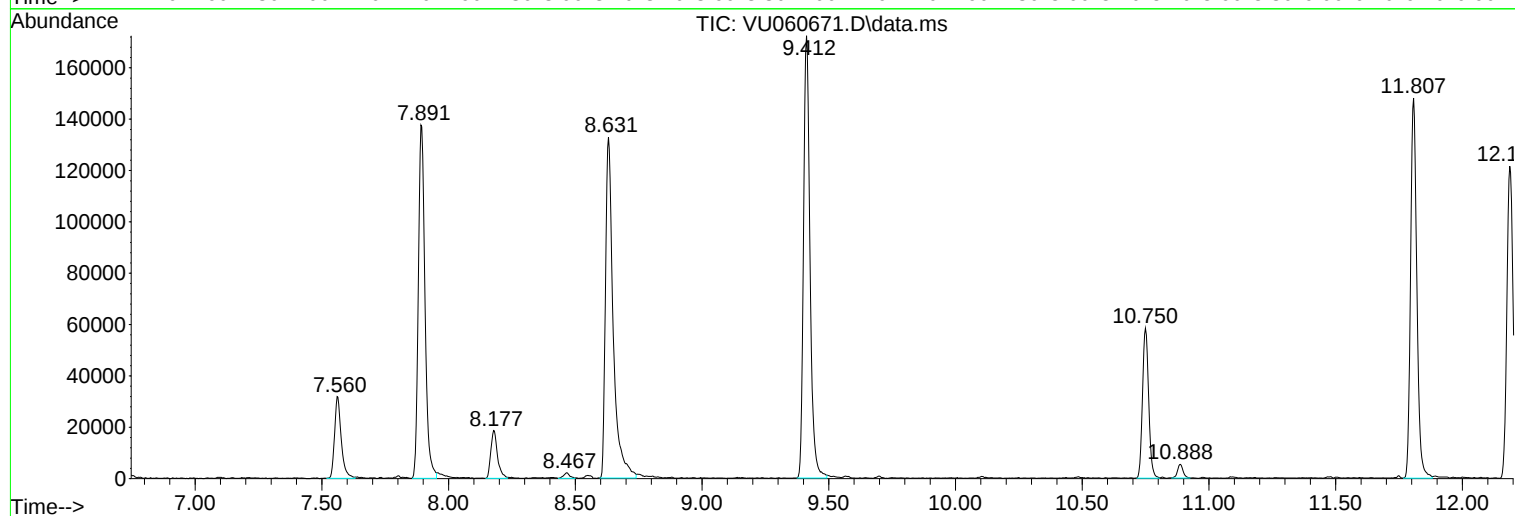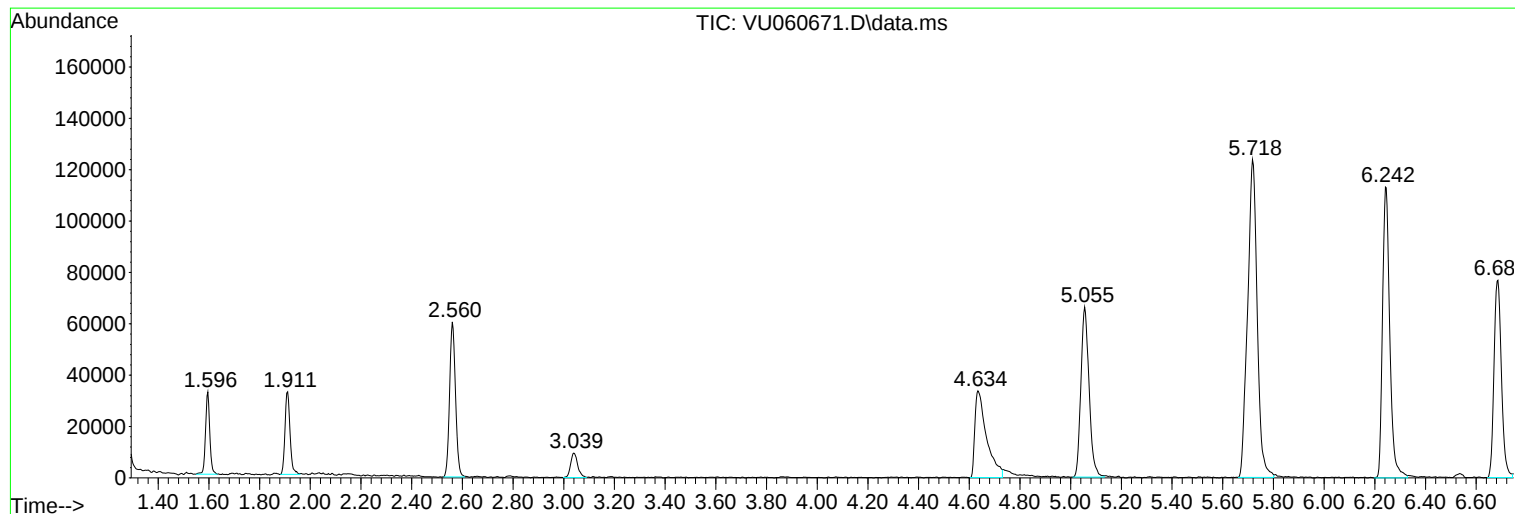

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091024\
Data File : VU060671.D
Acq On : 10 Sep 2024 17:04
Operator : MD/SY
Sample : VIBLK132
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK132

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091024\
Data File : VU060671.D
Acq On : 10 Sep 2024 17:04
Operator : MD/SY
Sample : VIBLK132
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK132

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc