


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091024\
Data File : VU060659.D
Acq On : 10 Sep 2024 09:52
Operator : MD/SY
Sample : BFB195
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB195

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Sep 11 02:46:13 2024

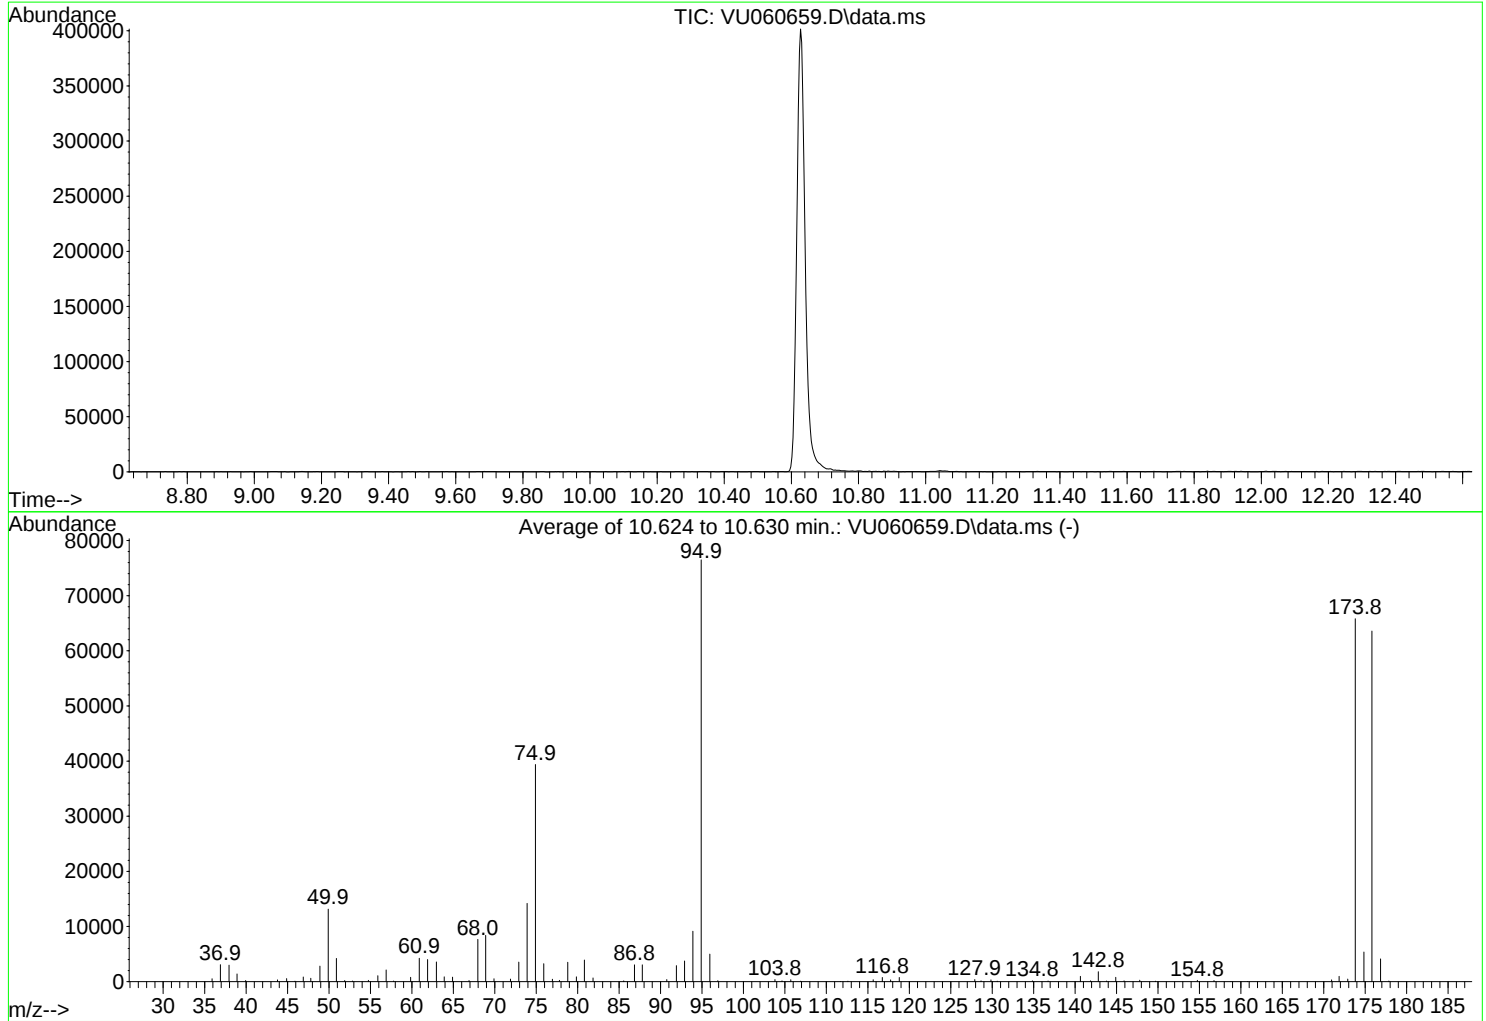

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.2	13154	PASS
75	95	30	80	51.5	39373	PASS
95	95	100	100	100.0	76499	PASS
96	95	5	9	6.5	4997	PASS
173	174	0.00	2	0.7	467	PASS
174	95	50	120	86.0	65824	PASS
175	174	5	9	8.2	5380	PASS
176	174	95	101	96.6	63584	PASS
177	176	5	9	6.5	4113	PASS

m/z	Abundance
43.70	199.0

Instrument :
MSVOA_U
ClientSampleId :
BFB195

m/z	Abundance
35.90	547.0
36.90	3241.0
38.00	2884.0
38.90	1183.0
40.00	196.0
43.90	607.0
44.90	546.0
46.90	950.0
47.80	600.0
48.90	2659.0
49.90	13003.0
50.90	4208.0
51.90	175.0
52.80	127.0
54.80	234.0
55.90	989.0
56.90	2064.0
57.80	163.0
59.90	775.0
60.90	4327.0
61.90	3953.0
63.00	3453.0
63.90	848.0
64.90	776.0
66.80	167.0
68.00	7095.0
68.90	8376.0
69.90	555.0
71.90	426.0
72.90	3496.0
73.90	13953.0
74.90	38560.0
75.90	3230.0
76.90	373.0
77.70	206.0
78.80	3450.0
79.80	819.0
80.80	4000.0
81.90	596.0
85.50	120.0
86.90	3260.0
87.80	3181.0
90.80	394.0
91.90	2836.0
92.90	3591.0
93.90	8890.0
94.90	74808.0
96.00	4921.0
96.90	249.0
103.80	353.0
104.60	142.0
105.70	357.0
111.70	104.0
112.60	131.0
115.60	347.0
116.70	805.0
117.70	304.0
118.80	701.0
127.90	365.0
128.60	146.0
129.80	426.0
130.60	165.0
134.90	119.0
136.80	130.0
140.70	961.0
141.90	142.0
142.80	1721.0
143.80	122.0
144.90	813.0
145.90	134.0
147.80	293.0
154.80	217.0
156.70	213.0
160.80	106.0
171.00	360.0
171.80	881.0
172.90	1401.0
173.80	63056.0
174.80	5234.0
175.80	60304.0
176.90	3840.0
177.90	106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB195

m/z	Abundance
35.90	540.0
36.90	3137.0
38.00	3111.0
38.90	1467.0
39.90	197.0
43.90	506.0
44.90	586.0
45.90	103.0
46.90	824.0
47.80	652.0
48.90	2887.0
49.90	13564.0
50.90	4331.0
51.90	207.0
52.90	129.0
54.70	247.0
55.90	1087.0
56.90	2133.0
57.80	161.0
59.80	800.0
60.90	4356.0
61.90	4156.0
62.90	3650.0
63.90	899.0
64.90	799.0
66.90	202.0
67.90	7956.0
68.90	8726.0
69.90	533.0
71.90	482.0
72.90	3676.0
73.90	14633.0
74.90	40360.0
75.90	3312.0
76.90	449.0
77.80	217.0
78.80	3578.0
79.90	891.0
80.80	4060.0
81.90	688.0
85.60	144.0
86.80	3089.0
87.80	3167.0
90.80	386.0
91.90	3073.0
92.90	3833.0
93.90	9431.0
94.90	78960.0
95.90	5201.0
96.90	187.0
103.80	375.0
104.70	165.0
105.70	347.0
106.90	117.0
112.60	111.0
115.60	357.0
116.80	753.0
117.70	333.0
118.80	796.0
127.90	395.0
128.70	179.0
129.90	321.0
130.60	138.0
134.90	141.0
136.80	131.0
140.70	1000.0
141.90	145.0
142.80	1864.0
143.80	138.0
144.90	820.0
145.90	136.0
147.80	277.0
149.70	108.0
154.70	240.0
156.70	213.0
170.90	333.0
171.80	955.0
173.80	67776.0
174.90	5490.0
175.80	65304.0
176.90	4218.0
177.80	126.0

Instrument :
MSVOA_U
ClientSampleId :
BFB195

m/z	Abundance
35.90	515.0
36.90	2839.0
37.90	2962.0
38.90	1572.0
39.90	198.0
43.90	480.0
44.90	556.0
45.90	126.0
46.90	731.0
47.80	579.0
48.90	2891.0
49.90	12894.0
50.90	4069.0
51.90	230.0
52.90	111.0
54.70	214.0
55.90	1115.0
56.90	2143.0
59.80	741.0
60.90	4037.0
61.90	3961.0
62.90	3633.0
63.90	909.0
64.90	828.0
67.00	222.0
67.90	7909.0
68.90	8086.0
69.90	495.0
71.90	458.0
72.90	3467.0
73.90	13997.0
74.90	39200.0
75.90	3215.0
77.00	500.0
77.90	257.0
78.80	3472.0
79.90	928.0
80.80	3667.0
81.80	726.0
85.60	145.0
86.80	2827.0
87.80	2785.0
90.70	349.0
91.90	2826.0
92.90	3776.0
93.90	9082.0
94.90	75728.0
95.90	4869.0
97.00	120.0
103.80	404.0
104.70	162.0
105.70	343.0
106.90	126.0
115.70	335.0
116.80	721.0
117.80	352.0
118.80	780.0
127.90	387.0
128.70	165.0
129.80	257.0
134.80	170.0
136.70	128.0
140.60	925.0
141.70	140.0
142.80	1788.0
143.80	131.0
144.90	711.0
145.90	149.0
147.80	188.0
149.70	132.0
154.70	222.0
156.80	189.0
158.80	124.0
170.90	294.0
171.90	1026.0
173.80	66640.0
174.90	5417.0
175.80	65144.0
176.80	4281.0
177.80	145.0

Instrument :
MSVOA_U
ClientSampleId :
BFB195