


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091118\
Data File : VU026670.D
Acq On : 11 Sep 2018 07:25
Operator : MD/SY
Sample : BFB53
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB53

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091018WMA.M
Title : VOC Analysis
Last Update : Wed Sep 12 00:46:21 2018

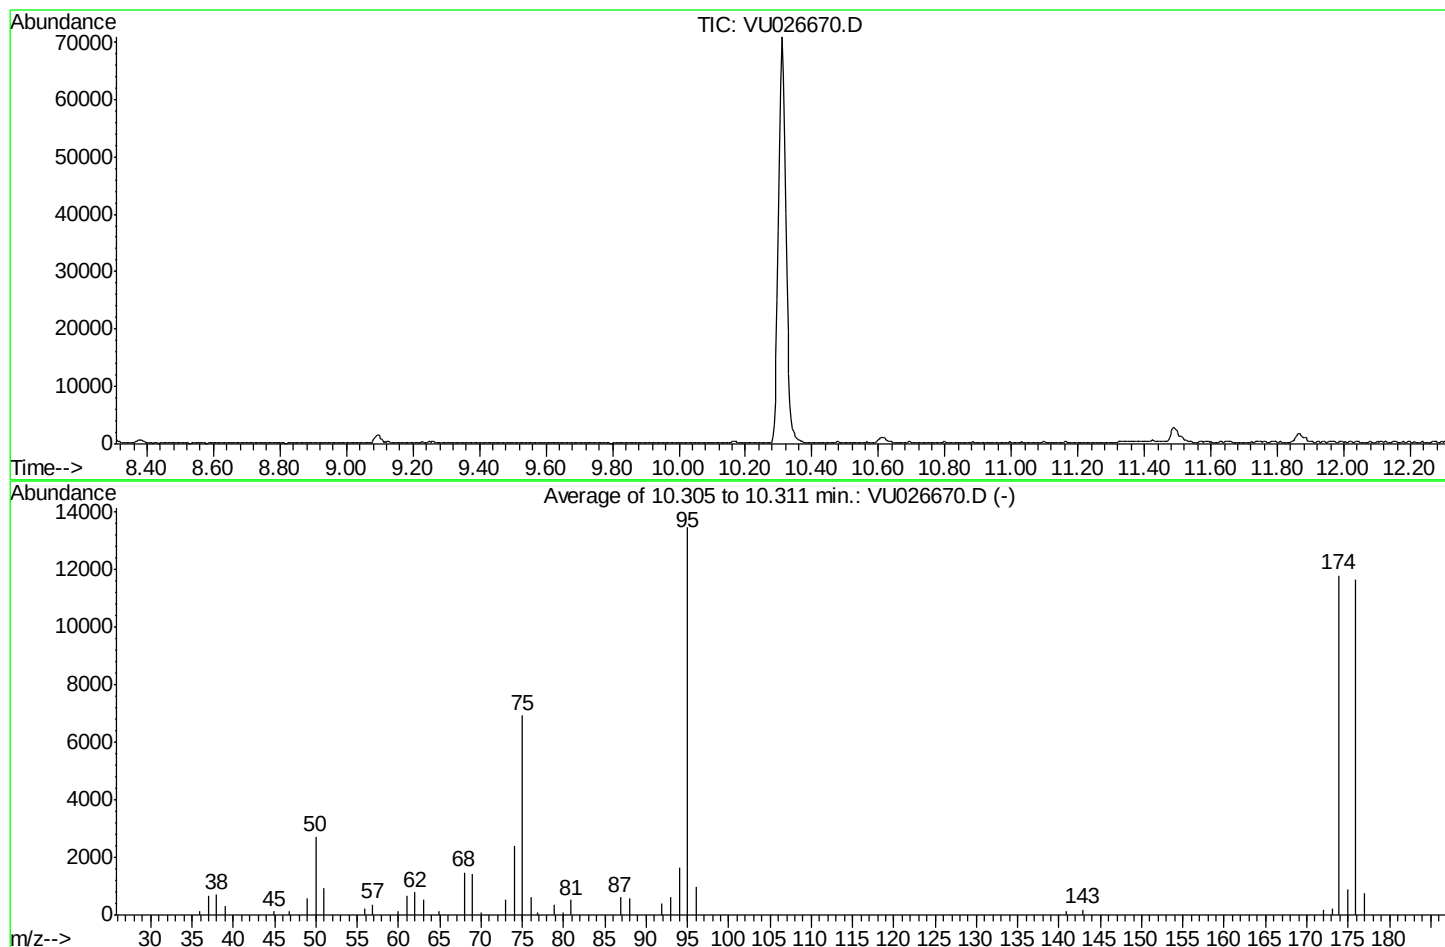

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2830

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	2722	PASS
75	95	30	80	51.5	6927	PASS
95	95	100	100	100.0	13452	PASS
96	95	5	9	7.3	983	PASS
173	174	0.00	2	1.8	215	PASS
174	95	50	120	87.7	11792	PASS
175	174	5	9	7.5	879	PASS
176	174	95	101	98.7	11643	PASS
177	176	5	9	6.4	748	PASS

m/z	Abundance
43.90	252.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

m/z	Abundance
35.90	121.0
37.00	592.0
37.90	618.0
39.00	339.0
43.90	235.0
45.00	127.0
46.80	145.0
49.00	574.0
50.00	2559.0
51.00	887.0
55.90	200.0
56.90	359.0
59.90	137.0
61.00	623.0
62.00	762.0
63.00	520.0
64.90	136.0
68.00	1388.0
69.00	1311.0
70.00	103.0
73.00	508.0
74.00	2208.0
75.00	6545.0
76.00	539.0
76.90	128.0
78.90	332.0
79.90	112.0
80.90	459.0
86.90	476.0
88.00	525.0
91.90	352.0
93.00	528.0
94.00	1540.0
95.00	12610.0
96.00	908.0
140.80	114.0
142.90	194.0
171.90	171.0
173.00	175.0
173.90	10803.0
174.90	784.0
175.90	10372.0
176.90	674.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

m/z	Abundance
35.90	155.0
37.00	675.0
38.00	726.0
39.00	325.0
43.90	224.0
45.00	129.0
46.80	125.0
49.00	574.0
50.00	2857.0
51.00	941.0
56.00	215.0
56.90	391.0
59.90	155.0
61.00	675.0
62.00	828.0
63.00	544.0
64.90	131.0
68.00	1523.0
69.00	1446.0
70.00	111.0
73.00	562.0
74.00	2480.0
75.00	7161.0
76.00	626.0
76.90	115.0
78.90	380.0
79.90	115.0
80.90	545.0
86.90	615.0
88.00	573.0
91.90	396.0
93.00	633.0
94.00	1684.0
95.00	13974.0
96.00	1035.0
140.80	145.0
142.90	213.0
171.90	191.0
173.00	230.0
173.90	12122.0
174.90	901.0
175.90	12083.0
176.90	762.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

m/z	Abundance
35.90	165.0
37.00	713.0
38.00	765.0
39.00	305.0
43.90	231.0
44.90	107.0
46.80	109.0
49.00	563.0
50.00	2750.0
51.00	917.0
56.00	221.0
56.90	375.0
59.90	165.0
61.00	699.0
62.00	783.0
63.00	534.0
64.90	153.0
68.00	1500.0
69.00	1493.0
70.00	110.0
72.90	579.0
74.00	2460.0
75.00	7076.0
76.00	642.0
78.90	411.0
79.90	106.0
80.90	581.0
86.90	725.0
88.00	610.0
91.90	390.0
93.00	657.0
94.00	1657.0
95.00	13772.0
96.00	1008.0
140.80	172.0
142.90	195.0
172.00	222.0
173.10	240.0
173.90	12451.0
174.90	953.0
175.90	12474.0
176.90	808.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53