


Iodomethane

Response Ratio

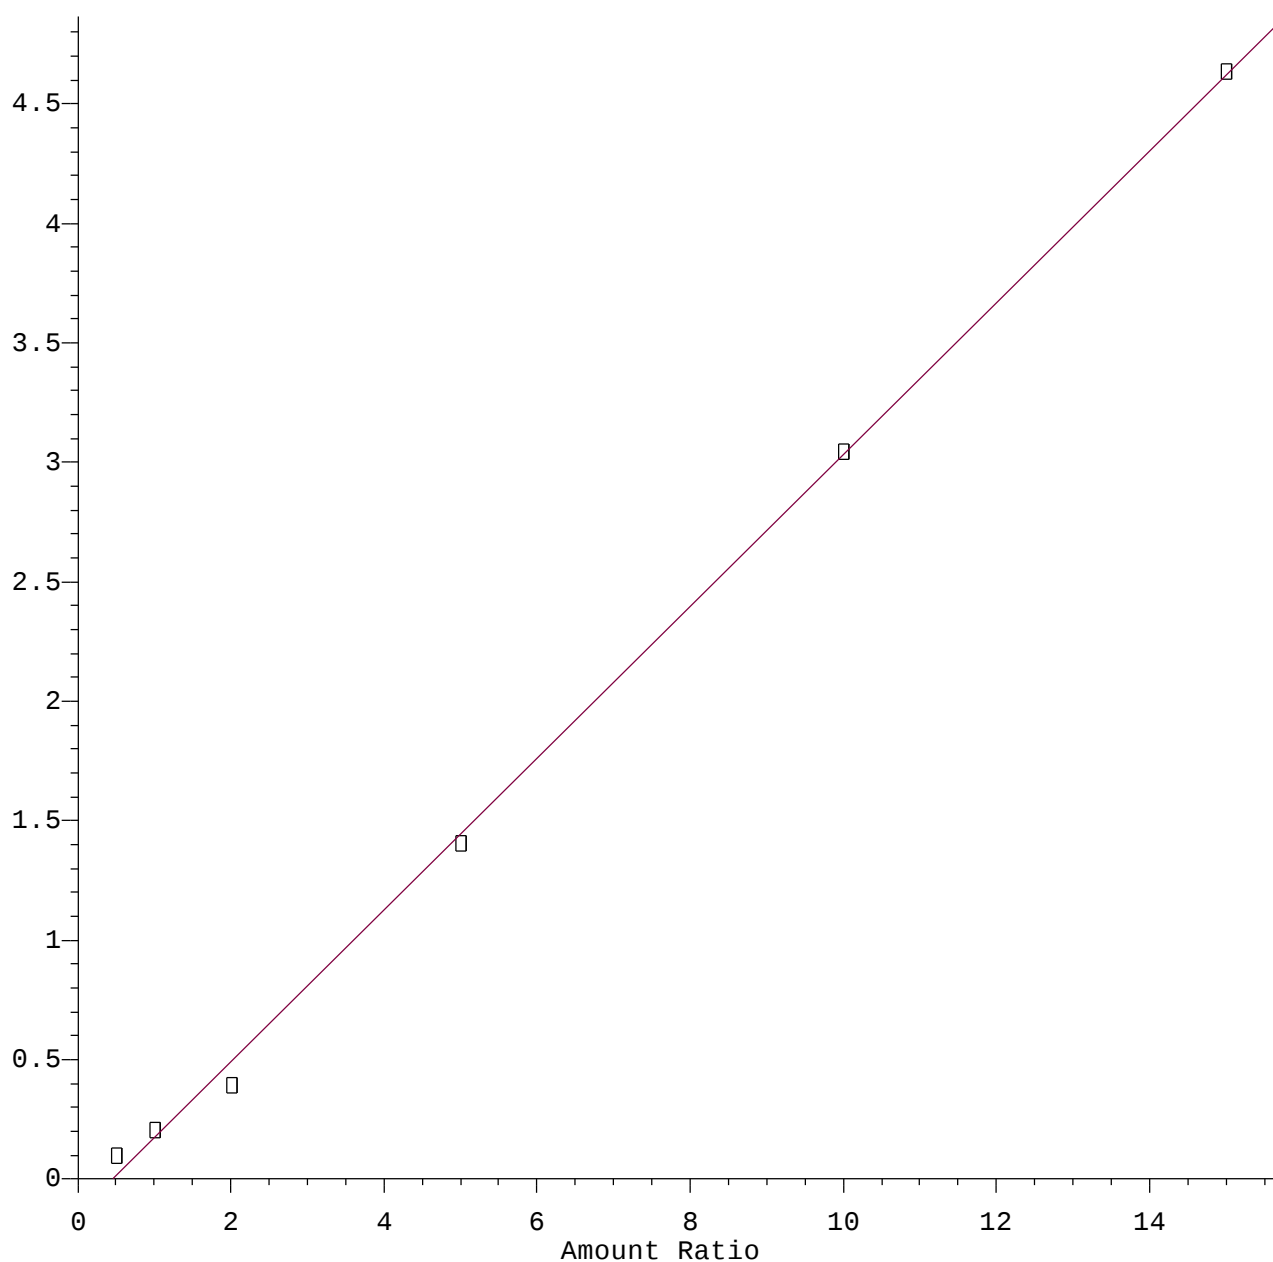


Resp Ratio = $3.18 \times 10^{-1} \times \text{Amt} - 1.44 \times 10^{-1}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U091119DW.M
Calibration Table Last Updated: Thu Sep 12 02:53:57 2019

tert-Butyl Alcohol

Response Ratio

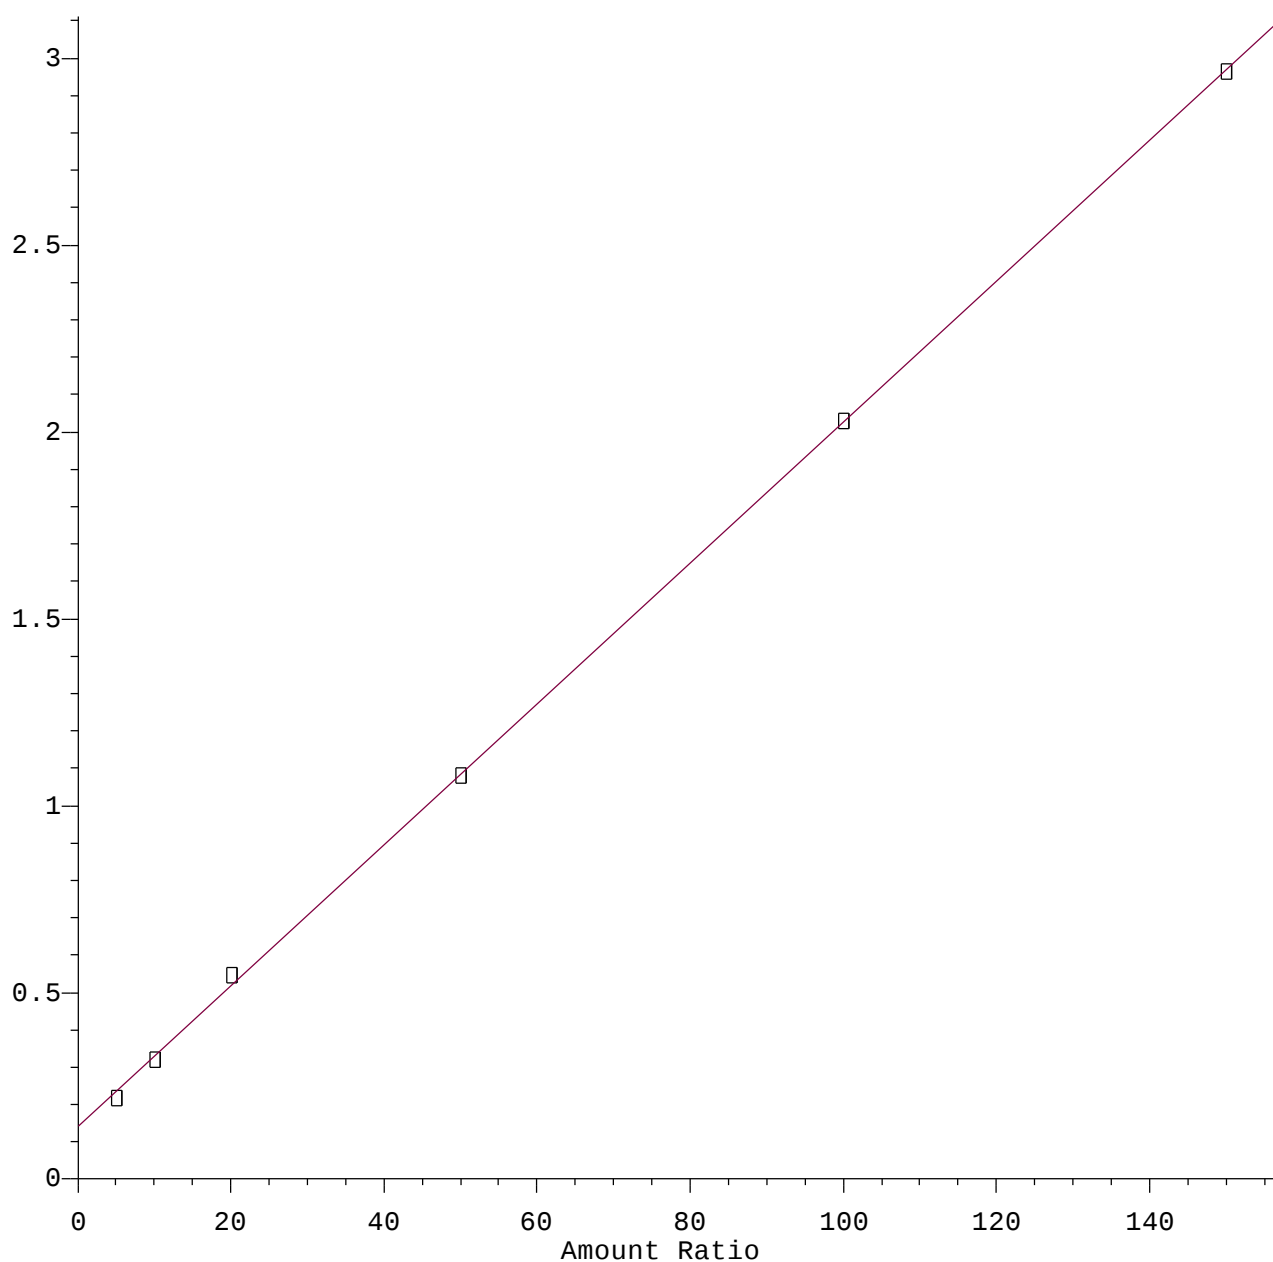


Resp Ratio = 1.89e-002 * Amt + 1.40e-001
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U091119DW.M
Calibration Table Last Updated: Thu Sep 12 02:53:57 2019

Naphthalene

Response Ratio

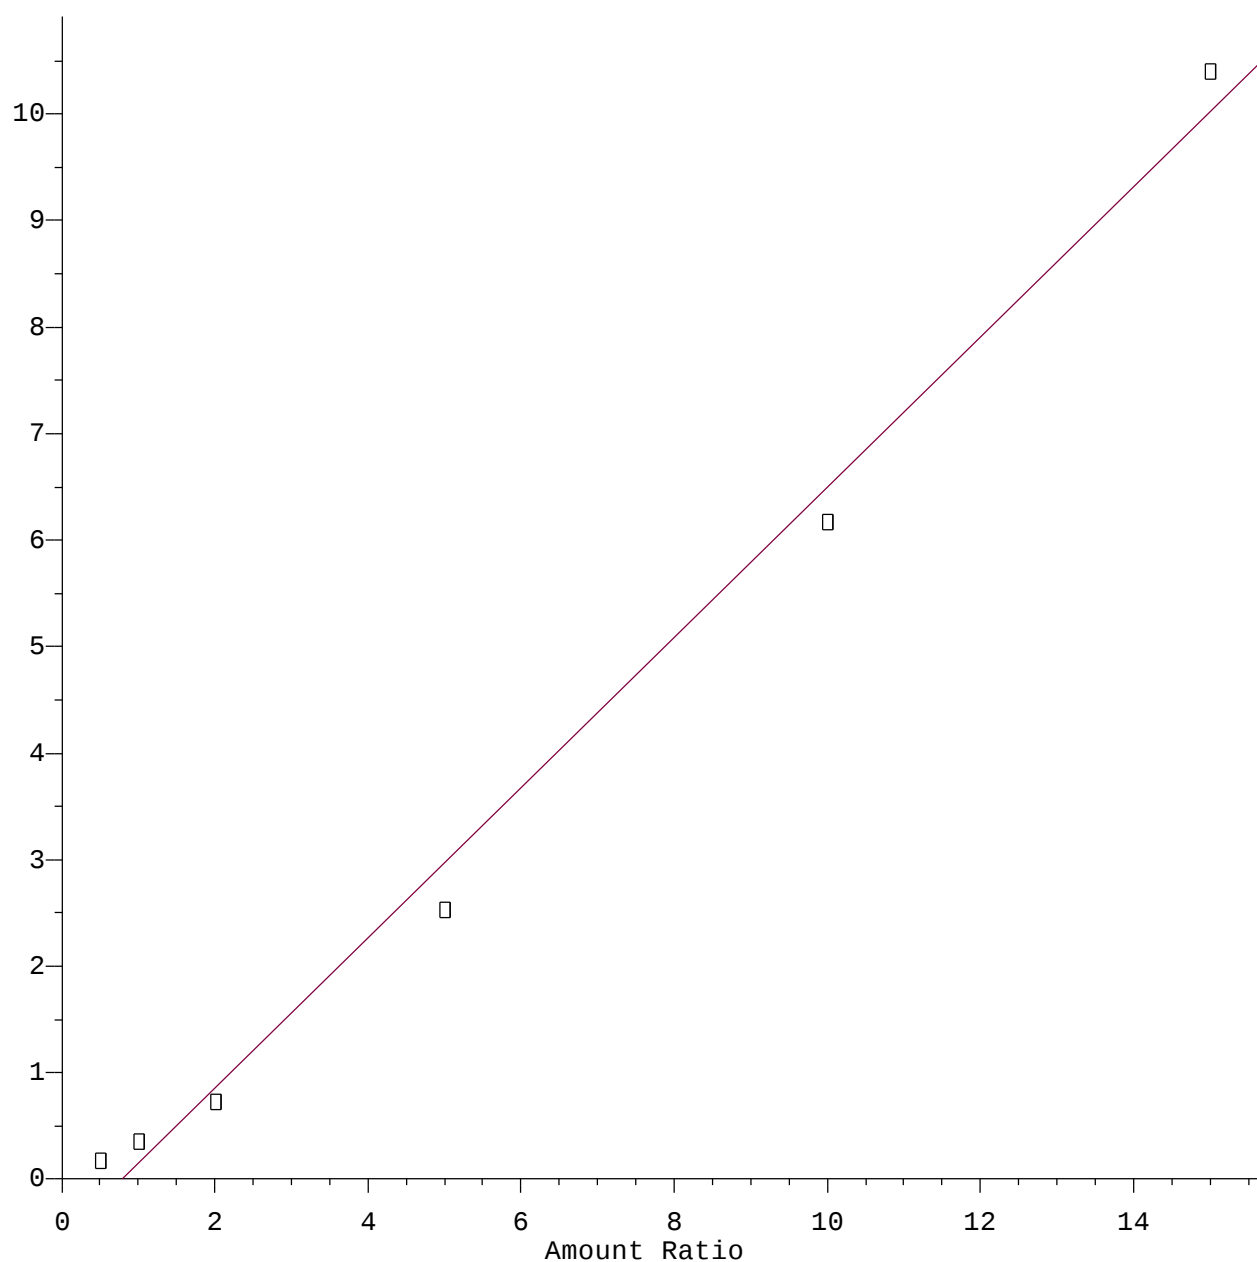

Resp Ratio = $7.05 \times 10^{-1} \times \text{Amt} - 5.46 \times 10^{-1}$
Coef of Det (r^2) = 0.992 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U091119DW.M
Calibration Table Last Updated: Thu Sep 12 02:53:57 2019