

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091119\
Data File : VU034473.D
Acq On : 11 Sep 2019 13:29
Operator : JC/SP
Sample : VU0911WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0911WBL01

Quant Time: Sep 12 04:01:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U091119DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Sep 12 02:53:57 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene	5.72	96	57434	1.00	ug/l	0.00

System Monitoring Compounds

57) 4-Bromofluorobenzene	10.29	95	18103	0.81	ug/l	0.00
Spiked Amount	1.000		Recovery	=	81.00%	
68) 1,2-Dichlorobenzene-d4	11.84	152	20455	0.85	ug/l	0.00
Spiked Amount	1.000		Recovery	=	85.00%	


Target Compounds	Ovalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU091119\
Data File : VU034473.D
Acq On : 11 Sep 2019 13:29
Operator : JC/SP
Sample : VU0911WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0911WBL01

Quant Time: Sep 12 04:01:37 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U091119DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Sep 12 02:53:57 2019
Response via : Initial Calibration




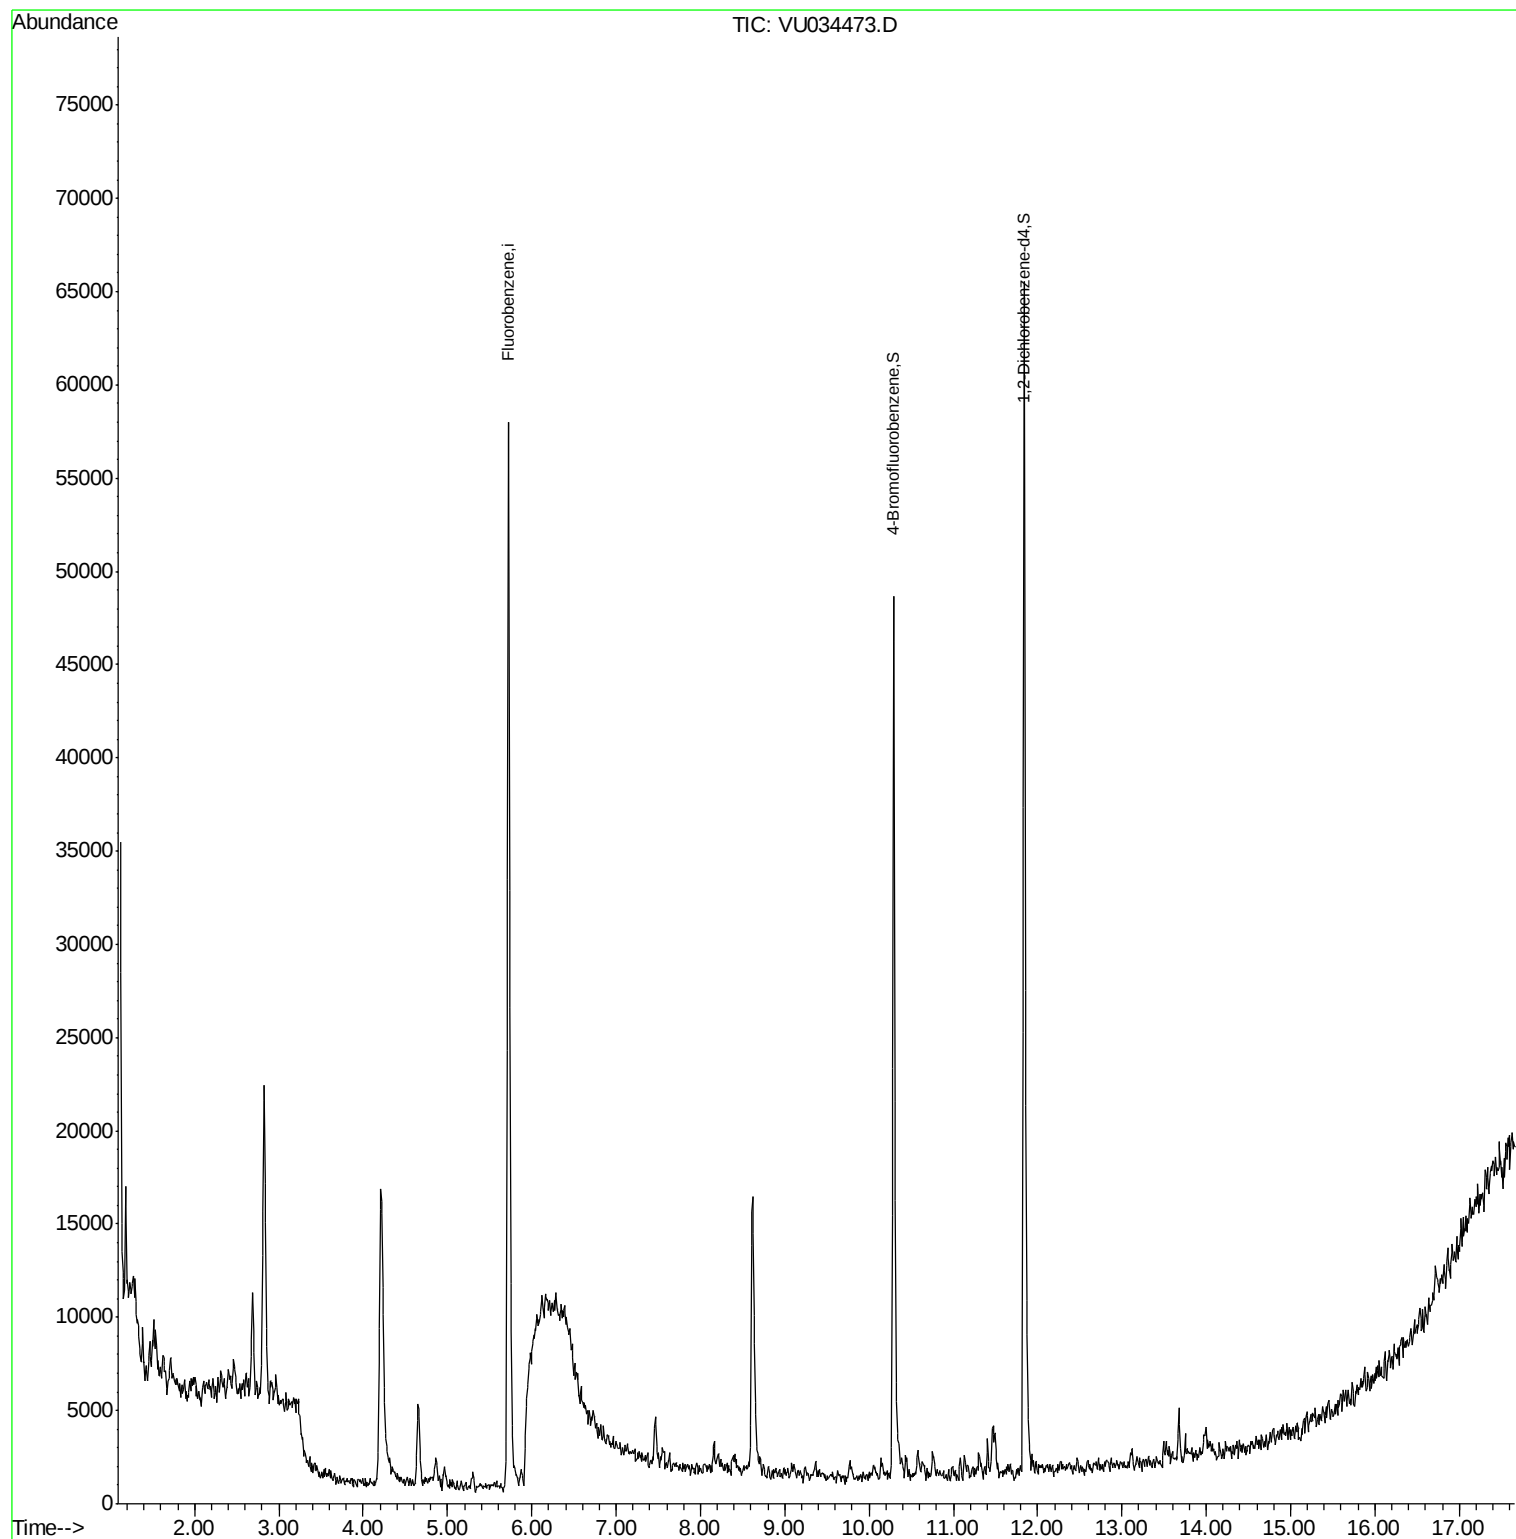


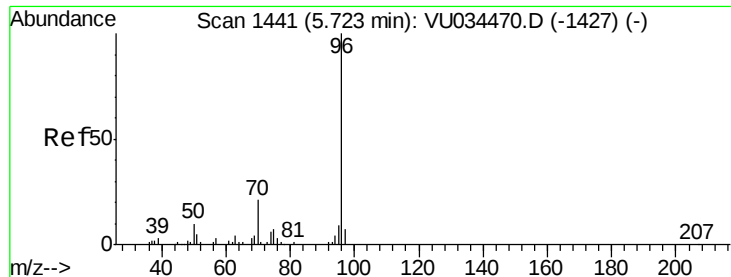

#1
 Fluorobenzene
 Concen: 1.000 ug/l
 RT: 5.72 min Scan# 1441
 Delta R.T. -0.00 min
 Lab File: VU034473.D
 Acq: 11 Sep 2019 13:29




Instrument :
 MSVOA_U
 ClientSampleId :
 VU0911WBL01


Tot Ion:	96	Resp:	57434
Ion	Ratio	Lower	Upper
96	100		
70	20.4	16.5	24.7
95	9.1	7.0	10.6
97	5.9	0.0	0.0#

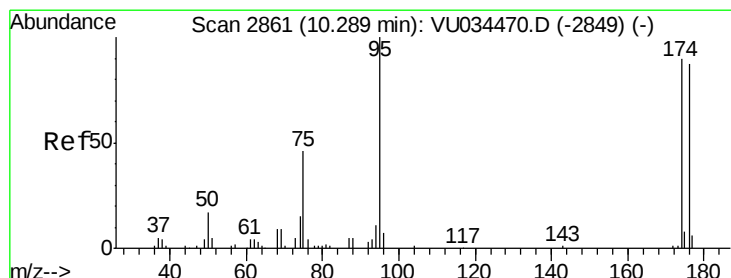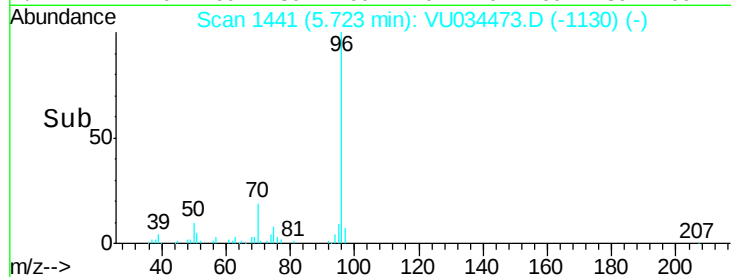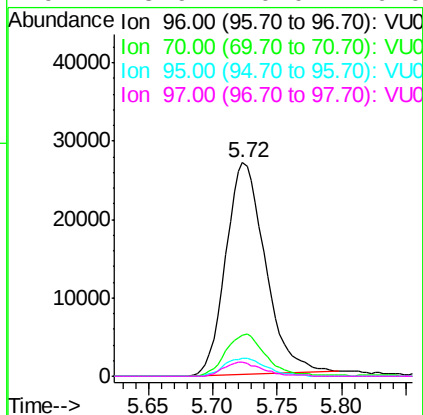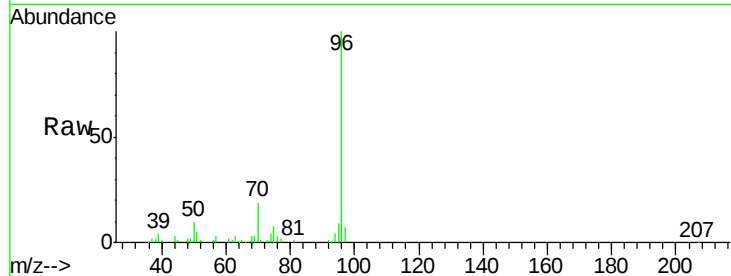

#57
 4-Bromofluorobenzene
 Concen: 0.814 ug/l
 RT: 10.29 min Scan# 2862
 Delta R.T. 0.00 min
 Lab File: VU034473.D
 Acq: 11 Sep 2019 13:29

Tgt Ion:	95	Resp:	18103
Ion	Ratio	Lower	Upper
95	100		
174	90.2	70.1	105.1
176	82.9	67.7	101.5

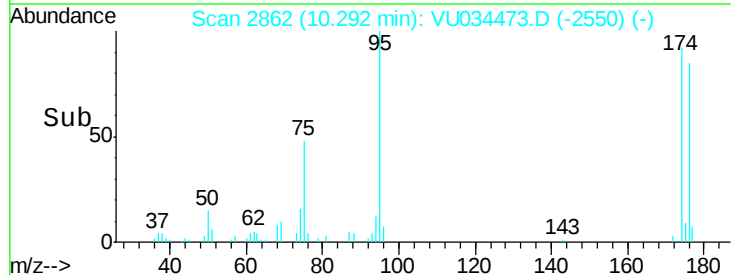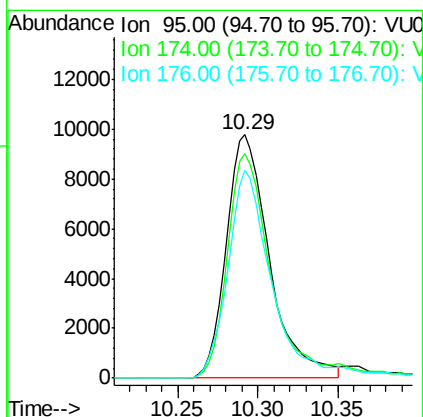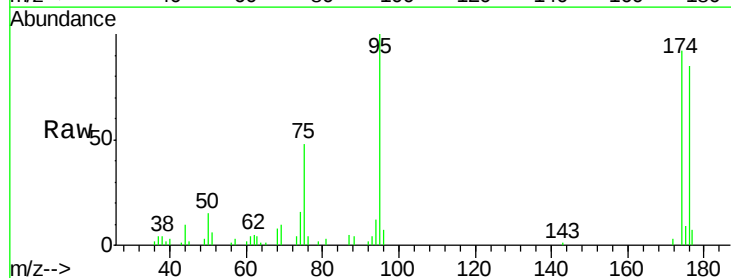

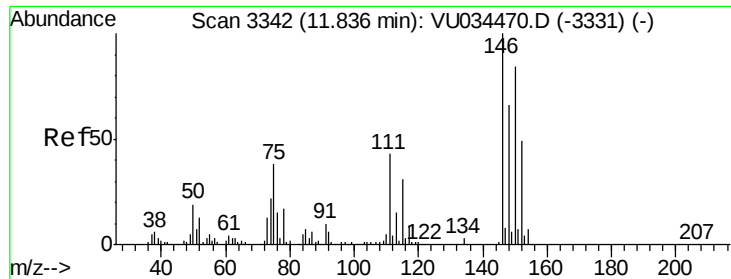

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.853 ug/l
 RT: 11.84 min Scan# 3344
 Delta R.T. 0.01 min
 Lab File: VU034473.D
 Acq: 11 Sep 2019 13:29

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0911WBL01

Tot Ion	Ratio	Lower	Upper
152	100		
115	60.0	0.0	126.6
150	152.9	0.0	633.6

