


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU091119\
Data File : VU034465.D
Acq On : 11 Sep 2019 08:47
Operator : JC/SP
Sample : BFB
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U091119DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Thu Sep 12 02:53:57 2019

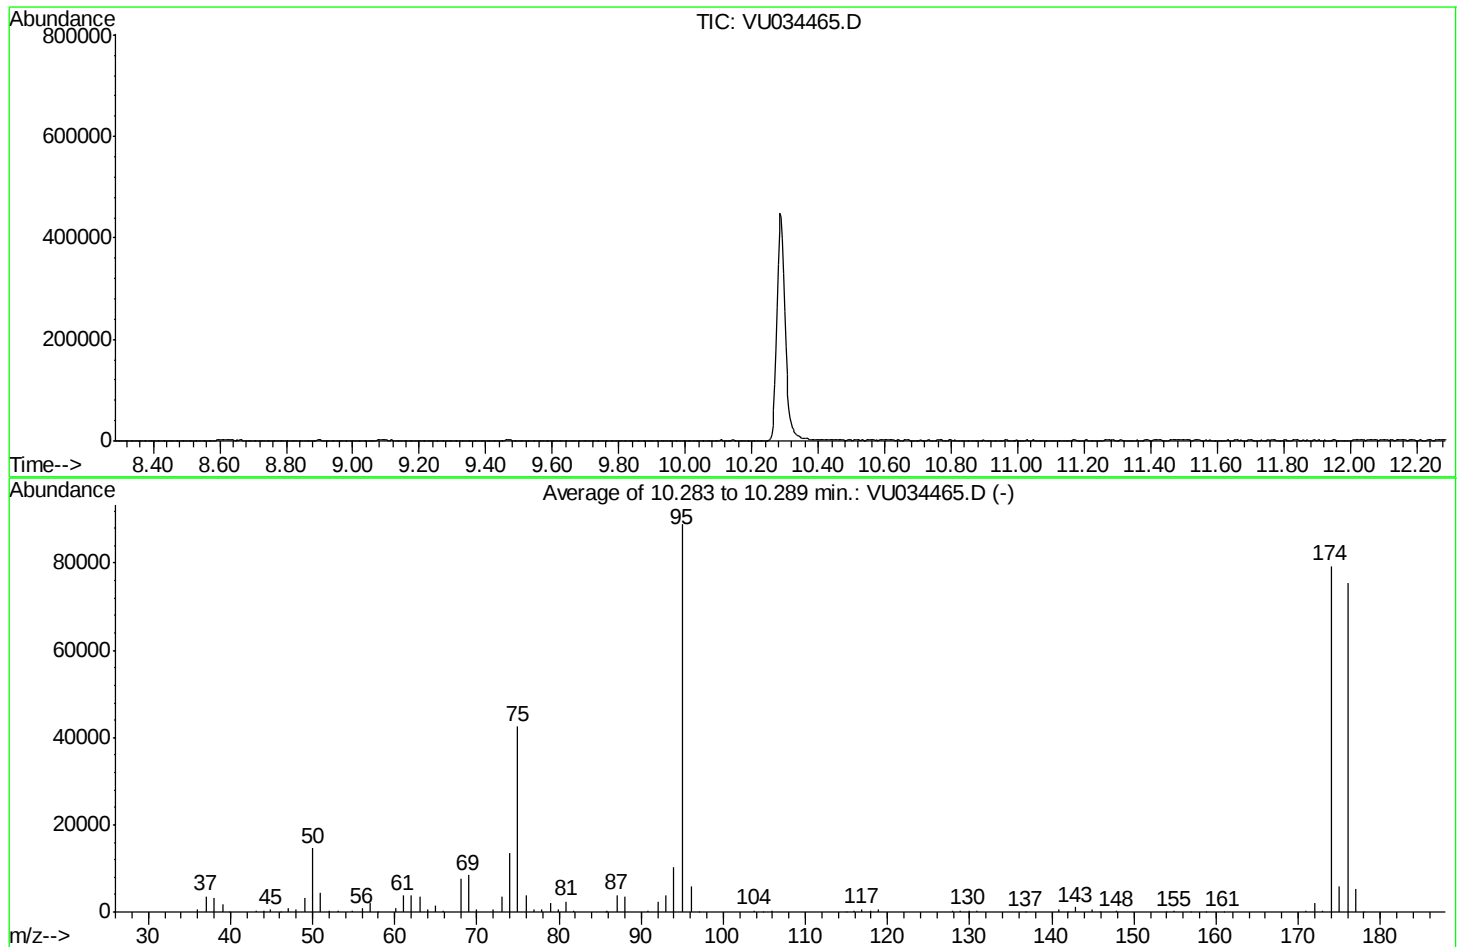

AutoFind: Scans 2859, 2860, 2861; Background Corrected with Scan 2847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	14580	PASS
75	95	30	60	47.9	42560	PASS
95	95	100	100	100.0	88896	PASS
96	95	5	9	6.6	5852	PASS
173	174	0.00	2	0.4	281	PASS
174	95	50	100	89.2	79304	PASS
175	174	5	9	7.4	5902	PASS
176	174	95	101	95.2	75528	PASS
177	176	5	9	7.0	5288	PASS