

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091120\
 Data File : VU040104.D
 Acq On : 11 Sep 2020 14:29
 Operator : SY/MD
 Sample : VU0911WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0911WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U091120DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.147	246	251	254	rBV3	1252	1071	1.53%	0.349%
2	2.163	254	256	264	rVB6	1678	1485	2.12%	0.484%
3	2.308	298	301	305	rBV4	1103	735	1.05%	0.240%
4	2.803	447	455	460	rBV2	1018	1511	2.15%	0.493%
5	3.060	526	535	546	rBV3	3665	6291	8.96%	2.051%
6	3.189	568	575	577	rBV2	1702	1717	2.45%	0.560%
7	4.658	1019	1032	1035	rBV2	8179	13414	19.11%	4.373%
8	5.305	1227	1233	1236	rBV2	703	869	1.24%	0.283%
9	6.125	1476	1488	1505	rBV	35144	66816	95.20%	21.784%
10	6.266	1526	1532	1536	rVB2	784	900	1.28%	0.293%
11	7.800	1995	2009	2022	rBV6	5529	11062	15.76%	3.606%
12	8.202	2125	2134	2136	rBV2	621	877	1.25%	0.286%
13	8.697	2278	2288	2305	rBV4	4587	9653	13.75%	3.147%
14	8.922	2349	2358	2372	rVB5	2033	4390	6.25%	1.431%
15	9.568	2553	2559	2563	rBV3	758	765	1.09%	0.249%
16	9.697	2591	2599	2601	rBV	713	736	1.05%	0.240%
17	10.108	2717	2727	2734	rBV5	1699	2663	3.79%	0.868%
18	10.481	2834	2843	2847	rBV4	1136	1372	1.95%	0.447%
19	10.632	2879	2890	2907	rBV	29787	46927	66.86%	15.299%
20	10.886	2959	2969	2976	rBV4	969	1527	2.18%	0.498%
21	11.083	3022	3030	3031	rBV2	1098	888	1.27%	0.290%
22	11.468	3140	3150	3156	rVB3	1943	2629	3.75%	0.857%
23	11.742	3227	3235	3244	rBV5	2288	3604	5.14%	1.175%
24	11.832	3254	3263	3271	rVB4	2869	3842	5.47%	1.253%
25	12.189	3363	3374	3387	rVB	43376	70185	100.00%	22.882%
26	12.764	3545	3553	3563	rVB2	1307	1994	2.84%	0.650%
27	12.983	3618	3621	3628	rVB4	711	910	1.30%	0.297%
28	13.211	3686	3692	3698	rVB5	3363	4453	6.34%	1.452%
29	13.443	3759	3764	3769	rVB2	738	856	1.22%	0.279%
30	13.828	3875	3884	3895	rBV6	6234	9890	14.09%	3.224%
31	14.079	3953	3962	3971	rVB2	8893	13185	18.79%	4.299%
32	14.317	4029	4036	4047	rVB4	8058	11598	16.52%	3.781%
33	14.529	4095	4102	4104	rBV2	547	725	1.03%	0.236%
34	15.504	4397	4405	4409	rBV3	716	851	1.21%	0.277%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091120\
Data File : VU040104.D
Acq On : 11 Sep 2020 14:29
Operator : SY/MD
Sample : VU0911WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0911WBL01

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U091120DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER

35	16.028	4562	4568	4571	rBV4	642	795	1.13%	0.259%
36	16.555	4729	4732	4740	rVB7	1335	1757	2.50%	0.573%
37	16.950	4849	4855	4858	rBV7	1456	1778	2.53%	0.580%
38	17.053	4882	4887	4894	rBV6	1435	2004	2.86%	0.653%


Sum of corrected areas: 306725

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU091120\
Data File : VU040104.D
Acq On : 11 Sep 2020 14:29
Operator : SY/MD
Sample : VU0911WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0911WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U091120DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

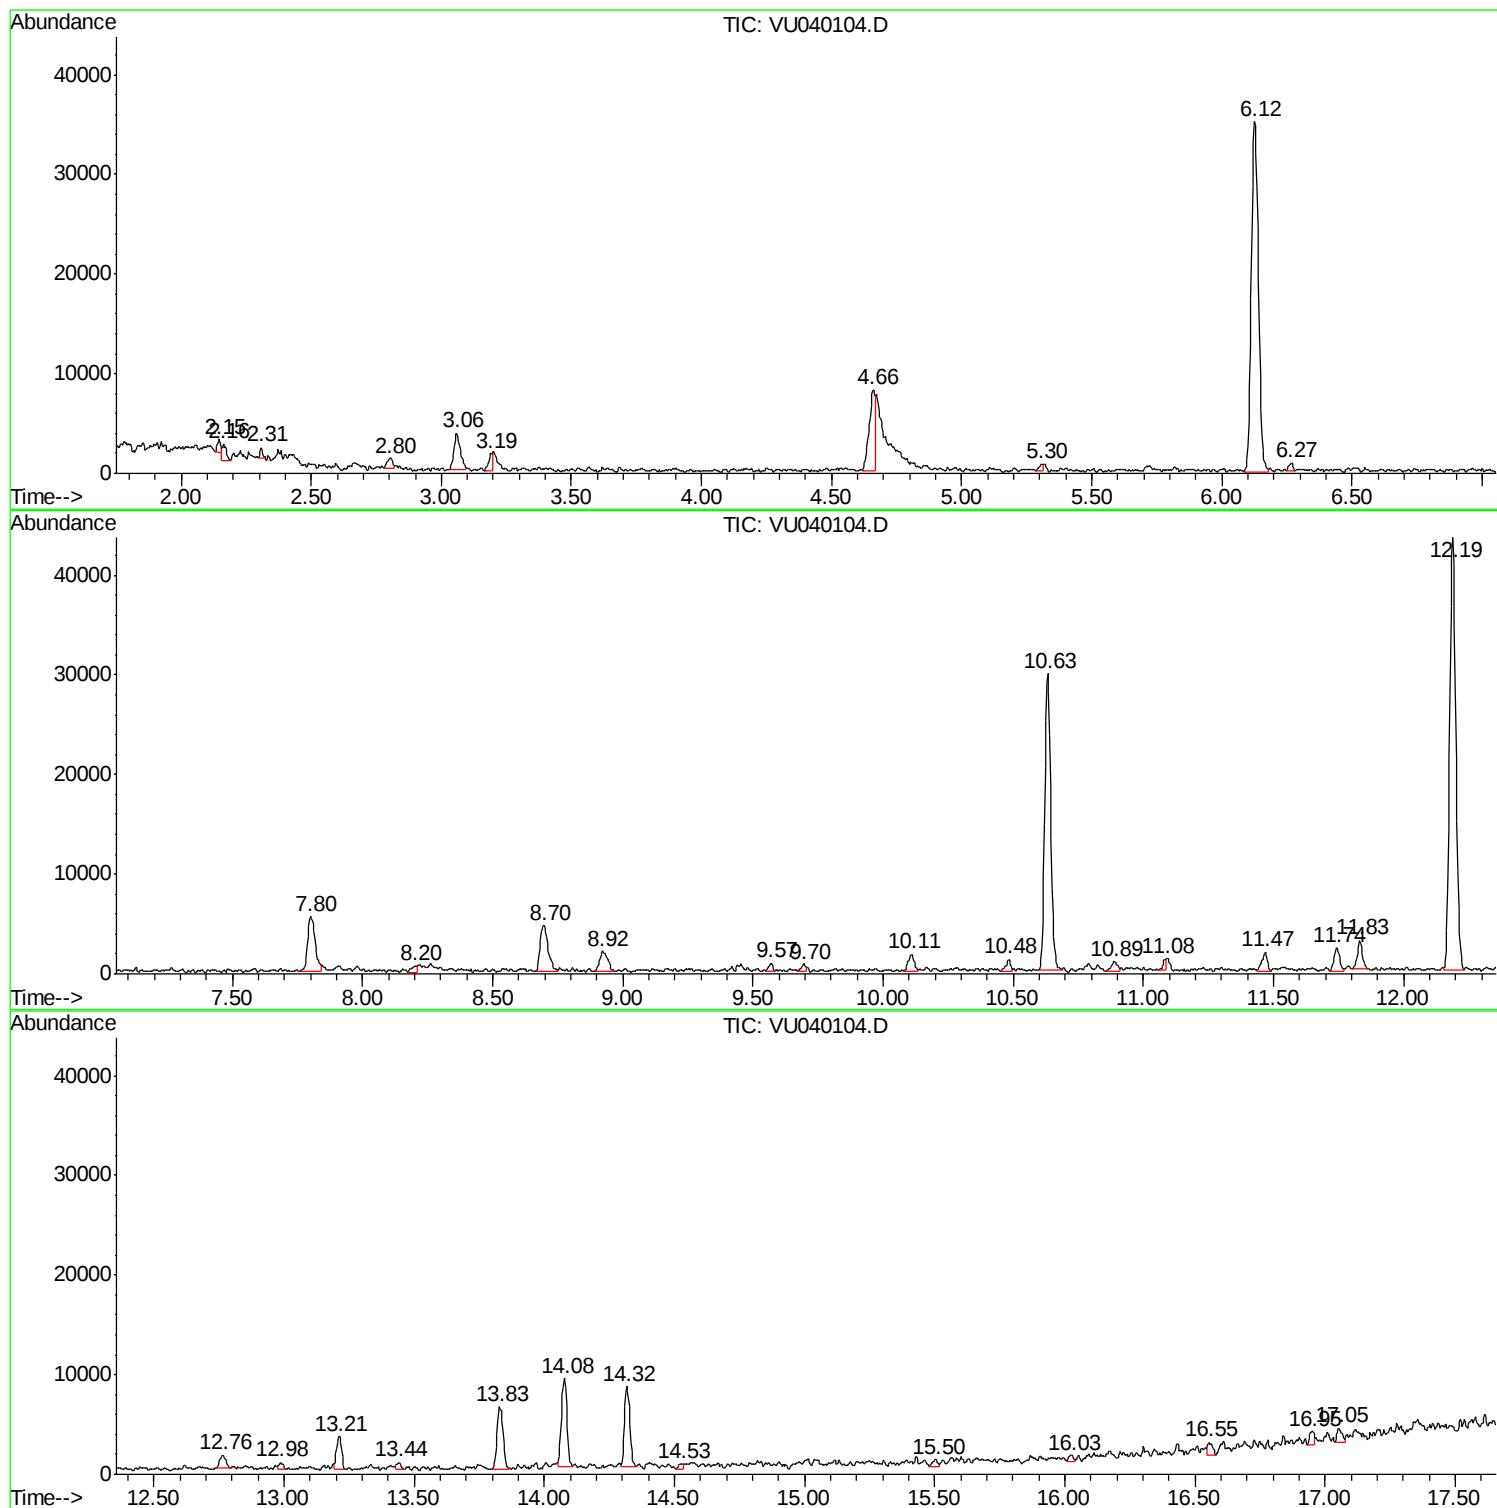

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU091120\
Data File : VU040104.D
Acq On : 11 Sep 2020 14:29
Operator : SY/MD
Sample : VU0911WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0911WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U091120DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU091120\
Data File : VU040104.D
Acq On : 11 Sep 2020 14:29
Operator : SY/MD
Sample : VU0911WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0911WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U091120DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc