


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU091120\
 Data File : VU040096.D
 Acq On : 11 Sep 2020 10:30
 Operator : SY/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U091120DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Fri Sep 11 13:27:06 2020

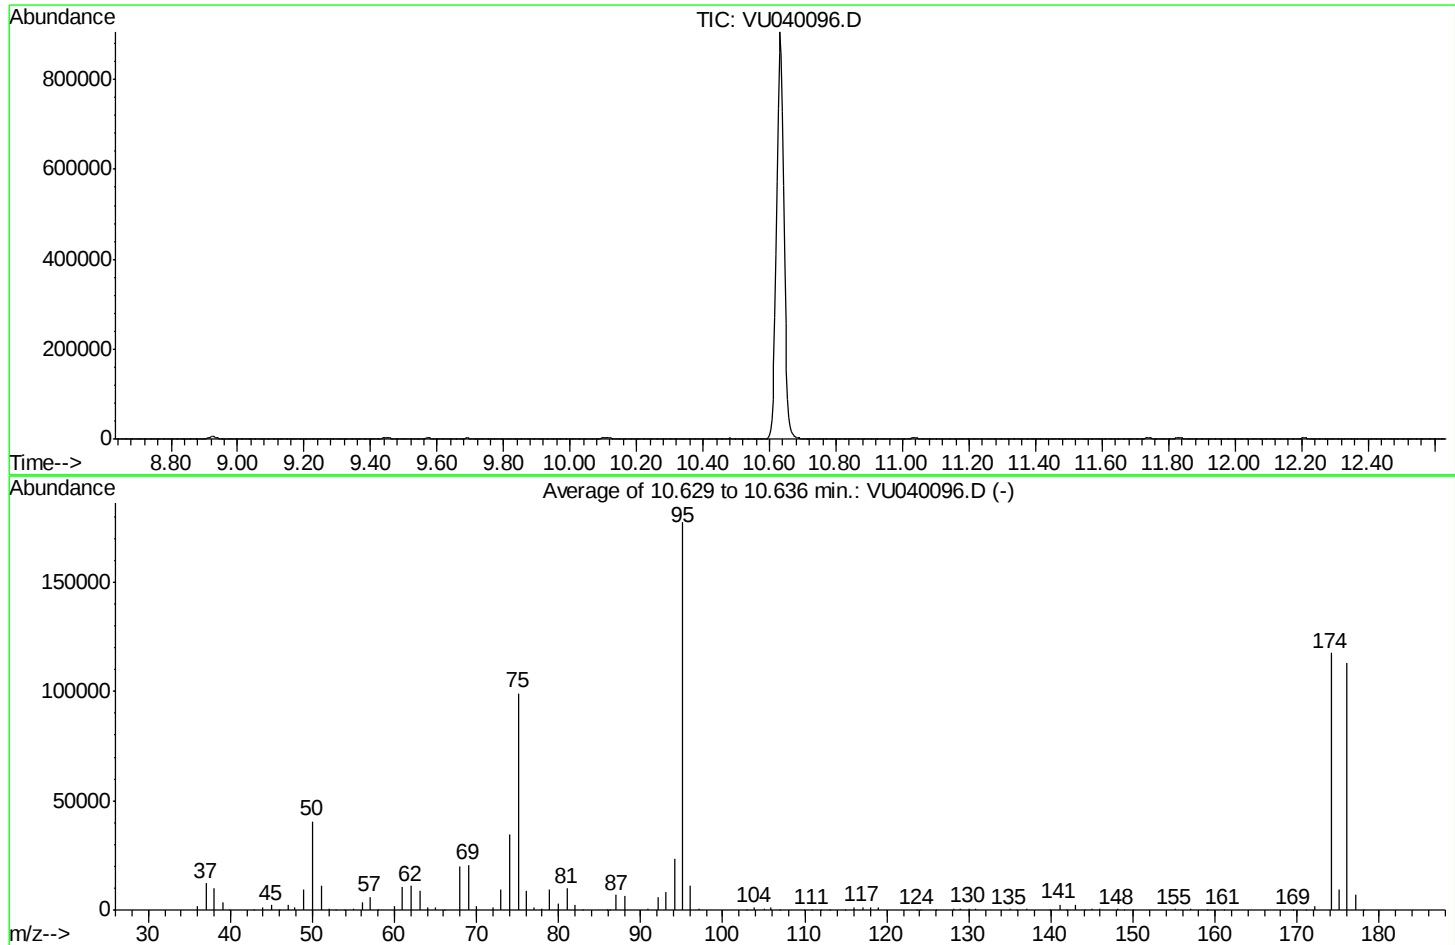

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	40640	PASS
75	95	30	60	55.9	99152	PASS
95	95	100	100	100.0	177365	PASS
96	95	5	9	6.2	11029	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	66.3	117546	PASS
175	174	5	9	7.8	9142	PASS
176	174	95	101	96.0	112869	PASS
177	176	5	9	6.3	7096	PASS