

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091123\
 Data File : VU055232.D
 Acq On : 11 Sep 2023 13:18
 Operator : MD/SY
 Sample : VU0911WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0911WBL01

Quant Time: Sep 12 08:59:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U091123DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Sep 12 08:56:31 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.113	96	58915	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.634	95	20098	0.879	ug/l	0.00
Spiked Amount 1.000			Recovery	=	88.000%	
68) 1,2-Dichlorobenzene-d4	12.193	152	18839	0.845	ug/l	0.00
Spiked Amount 1.000			Recovery	=	85.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091123\
Data File : VU055232.D
Acq On : 11 Sep 2023 13:18
Operator : MD/SY
Sample : VU0911WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0911WBL01

Quant Time: Sep 12 08:59:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U091123DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Sep 12 08:56:31 2023
Response via : Initial Calibration




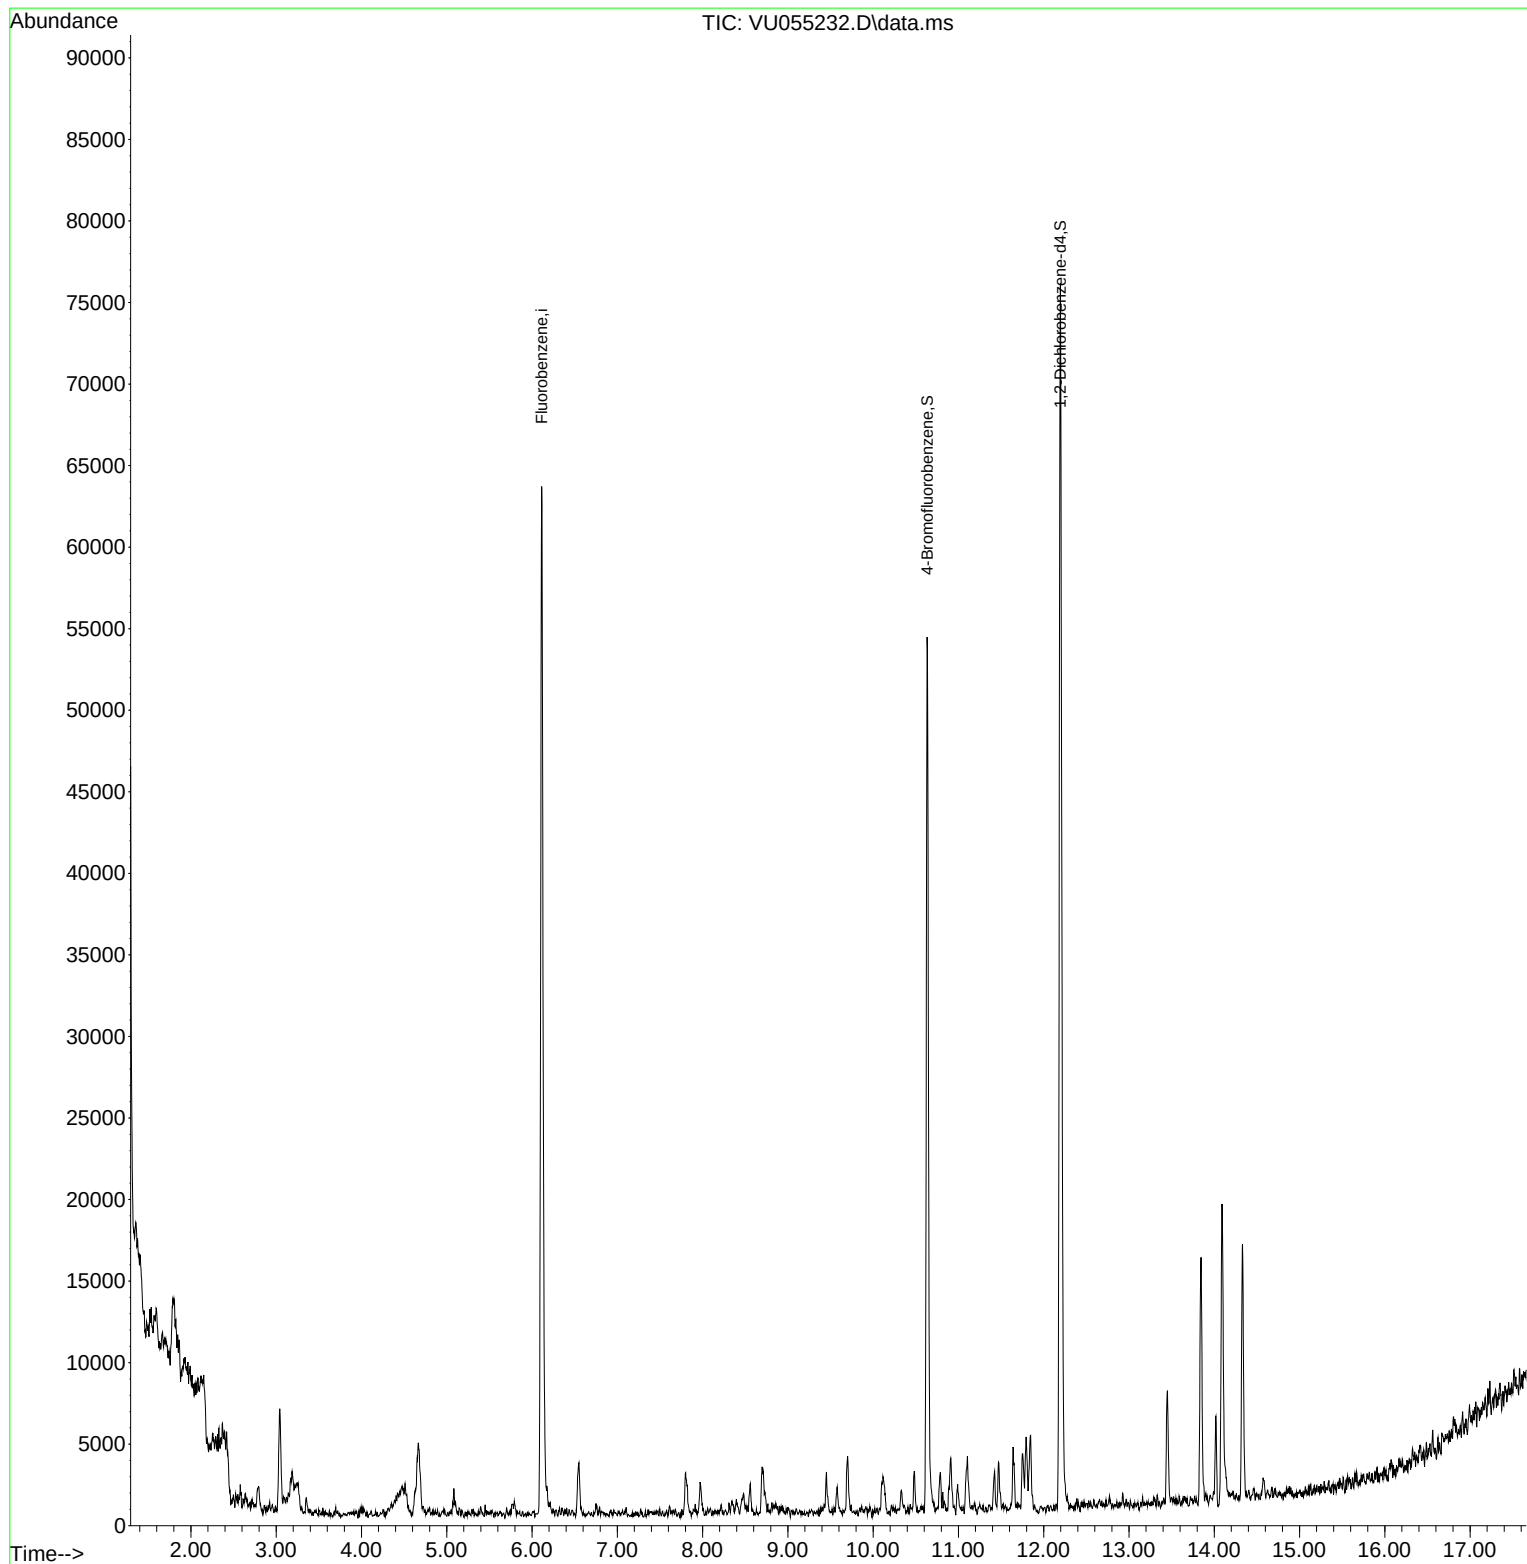


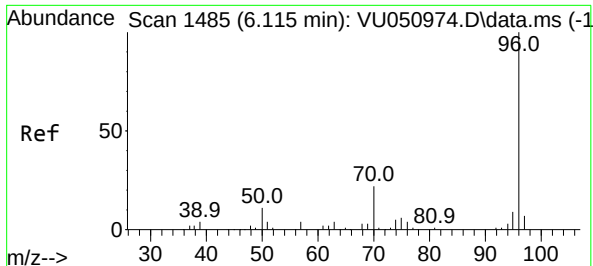

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.113 min Scan# 1
Delta R.T. -0.002 min
Lab File: VU055232.D
Acq: 11 Sep 2023 13:18




Instrument :
MSVOA_U
ClientSampleId :
VU0911WBL01


Tgt Ion:	96	Resp:	58915
Ion Ratio	Lower	Upper	
96	100		
70	19.7	16.5	24.7
95	9.1	7.4	11.0
97	6.7	0.0	0.0

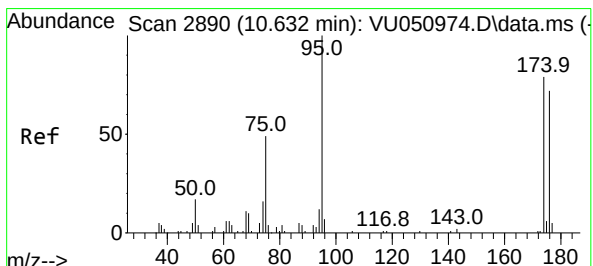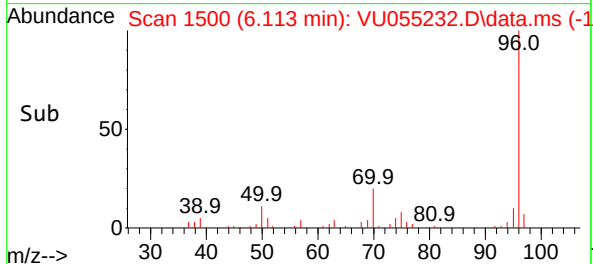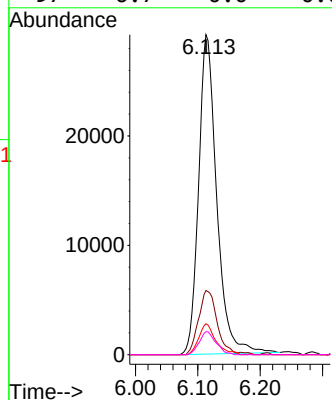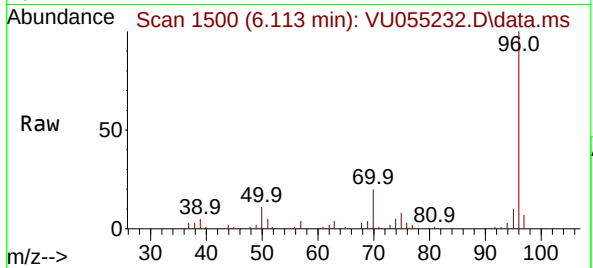

#57
4-Bromofluorobenzene
Concen: 0.879 ug/l
RT: 10.634 min Scan# 2906
Delta R.T. 0.002 min
Lab File: VU055232.D
Acq: 11 Sep 2023 13:18


Tgt Ion:	95	Resp:	20098
Ion Ratio	Lower	Upper	
95	100		
174	77.6	63.3	94.9
176	74.3	59.3	88.9

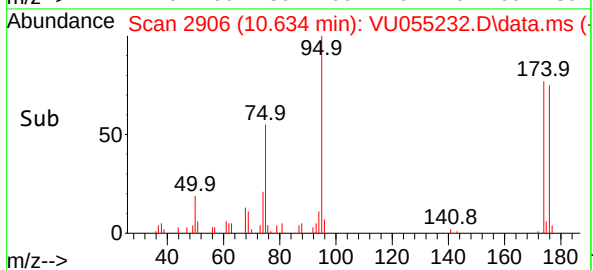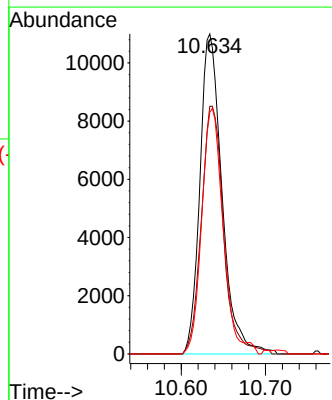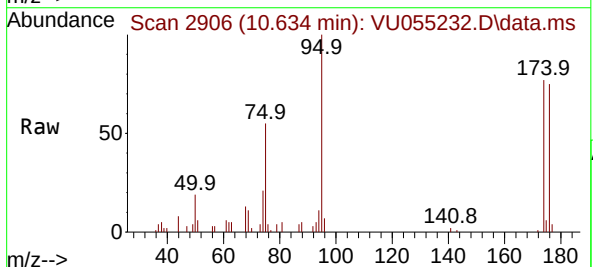

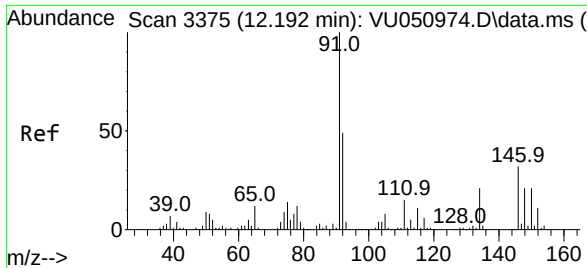

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.845 ug/l
 RT: 12.193 min Scan# 31
 Delta R.T. 0.001 min
 Lab File: VU055232.D
 Acq: 11 Sep 2023 13:18

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0911WBL01

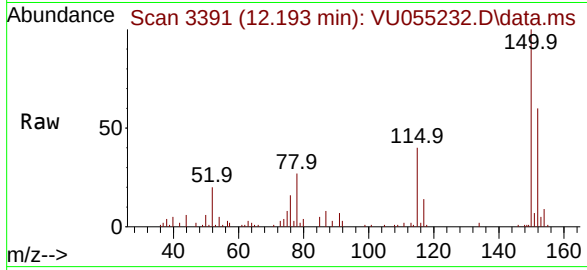

Tgt Ion:	152	Resp:	18839
Ion Ratio	Lower	Upper	
152	100		
115	67.3	0.0	308.8
150	165.2	0.0	635.0

