

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091123\
 Data File : VU055237.D
 Acq On : 11 Sep 2023 16:03
 Operator : MD/SY
 Sample : 04354-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PW-B6-L57-090723

Quant Time: Sep 21 05:15:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U091123DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Sep 21 05:13:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.116	96	49805	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.634	95	17376	0.899	ug/l	0.00
Spiked Amount	1.000		Recovery	=	90.000%	
68) 1,2-Dichlorobenzene-d4	12.196	152	16419	0.871	ug/l	0.00
Spiked Amount	1.000		Recovery	=	87.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091123\
Data File : VU055237.D
Acq On : 11 Sep 2023 16:03
Operator : MD/SY
Sample : 04354-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PW-B6-L57-090723

Quant Time: Sep 21 05:15:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U091123DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Sep 21 05:13:10 2023
Response via : Initial Calibration




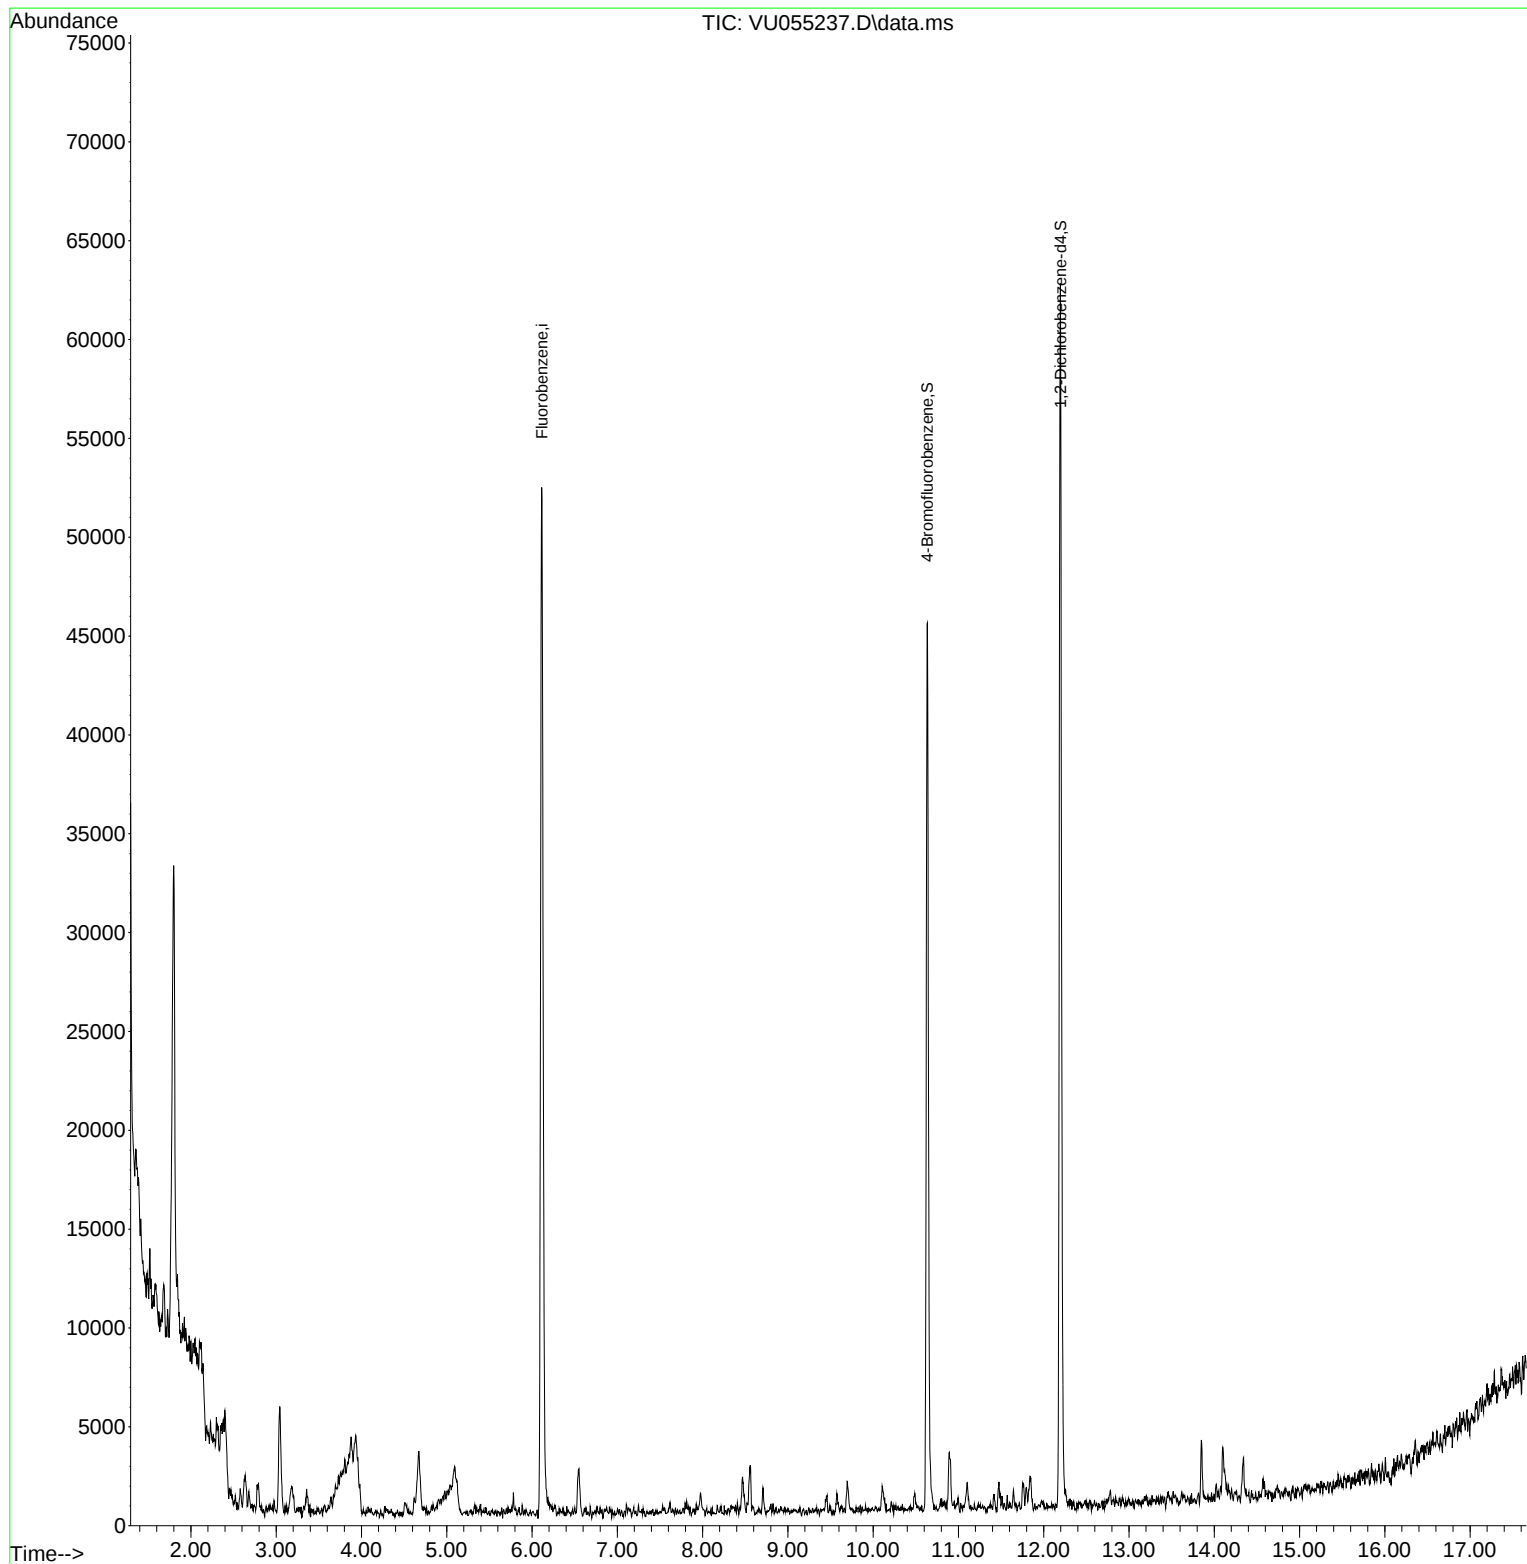


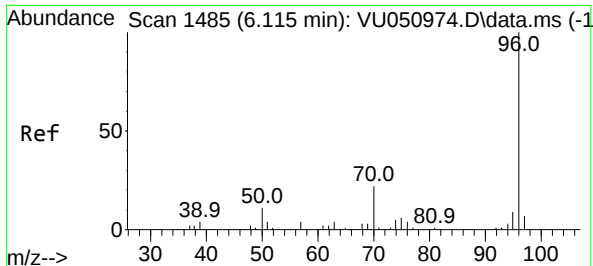

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.116 min Scan# 1
Delta R.T. 0.001 min
Lab File: VU055237.D
Acq: 11 Sep 2023 16:03




Instrument :
MSVOA_U
ClientSampleId :
PW-B6-L57-090723


Tgt Ion: 96	Resp: 49805
Ion Ratio	Lower Upper
96 100	
70 21.2	16.5 24.7
95 8.7	7.4 11.0
97 6.9	0.0 0.0

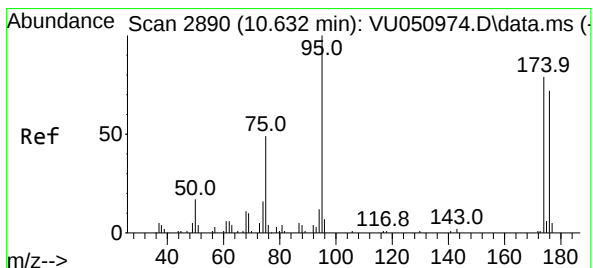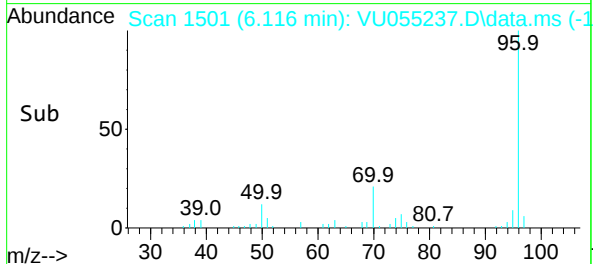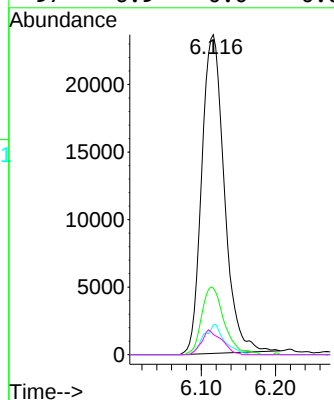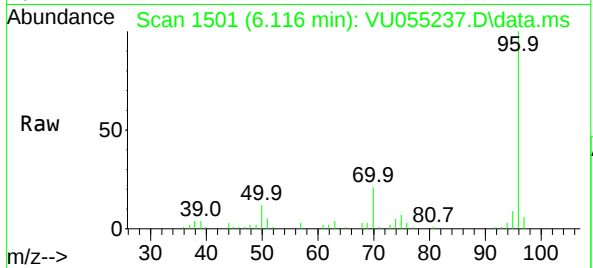

#57
4-Bromofluorobenzene
Concen: 0.899 ug/l
RT: 10.634 min Scan# 2906
Delta R.T. 0.002 min
Lab File: VU055237.D
Acq: 11 Sep 2023 16:03


Tgt Ion: 95	Resp: 17376
Ion Ratio	Lower Upper
95 100	
174 73.0	63.3 94.9
176 65.3	59.3 88.9

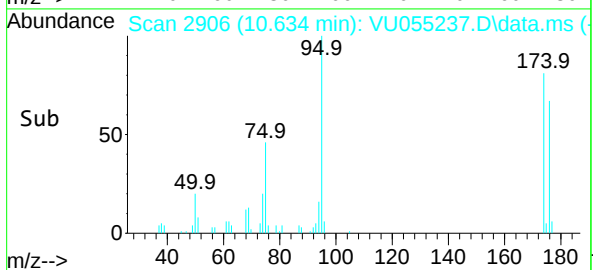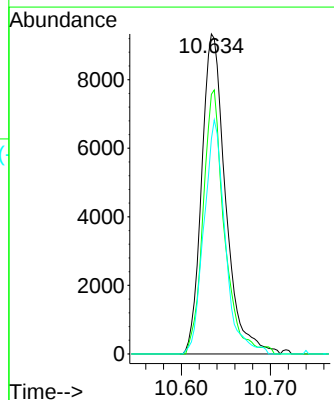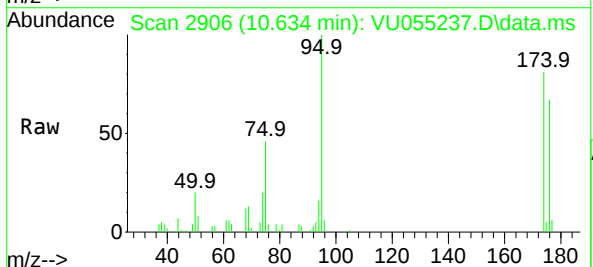

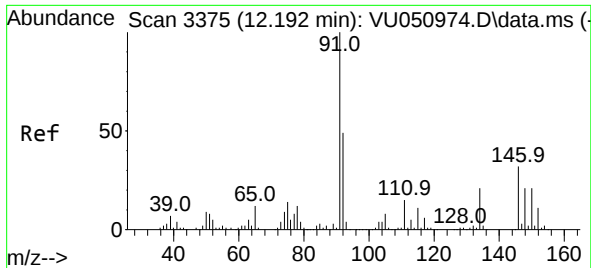

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.871 ug/l
 RT: 12.196 min Scan# 31
 Delta R.T. 0.004 min
 Lab File: VU055237.D
 Acq: 11 Sep 2023 16:03

Instrument :
 MSVOA_U
 ClientSampleId :
 PW-B6-L57-090723

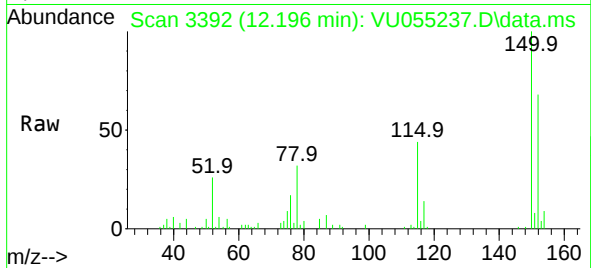

Tgt Ion:152	Resp:	16419
Ion	Ratio	Lower Upper
152	100	
115	69.0	0.0 308.8
150	155.7	0.0 635.0

