


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091123\
Data File : VU055224.D
Acq On : 11 Sep 2023 08:43
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U091123DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Tue Sep 12 08:56:31 2023

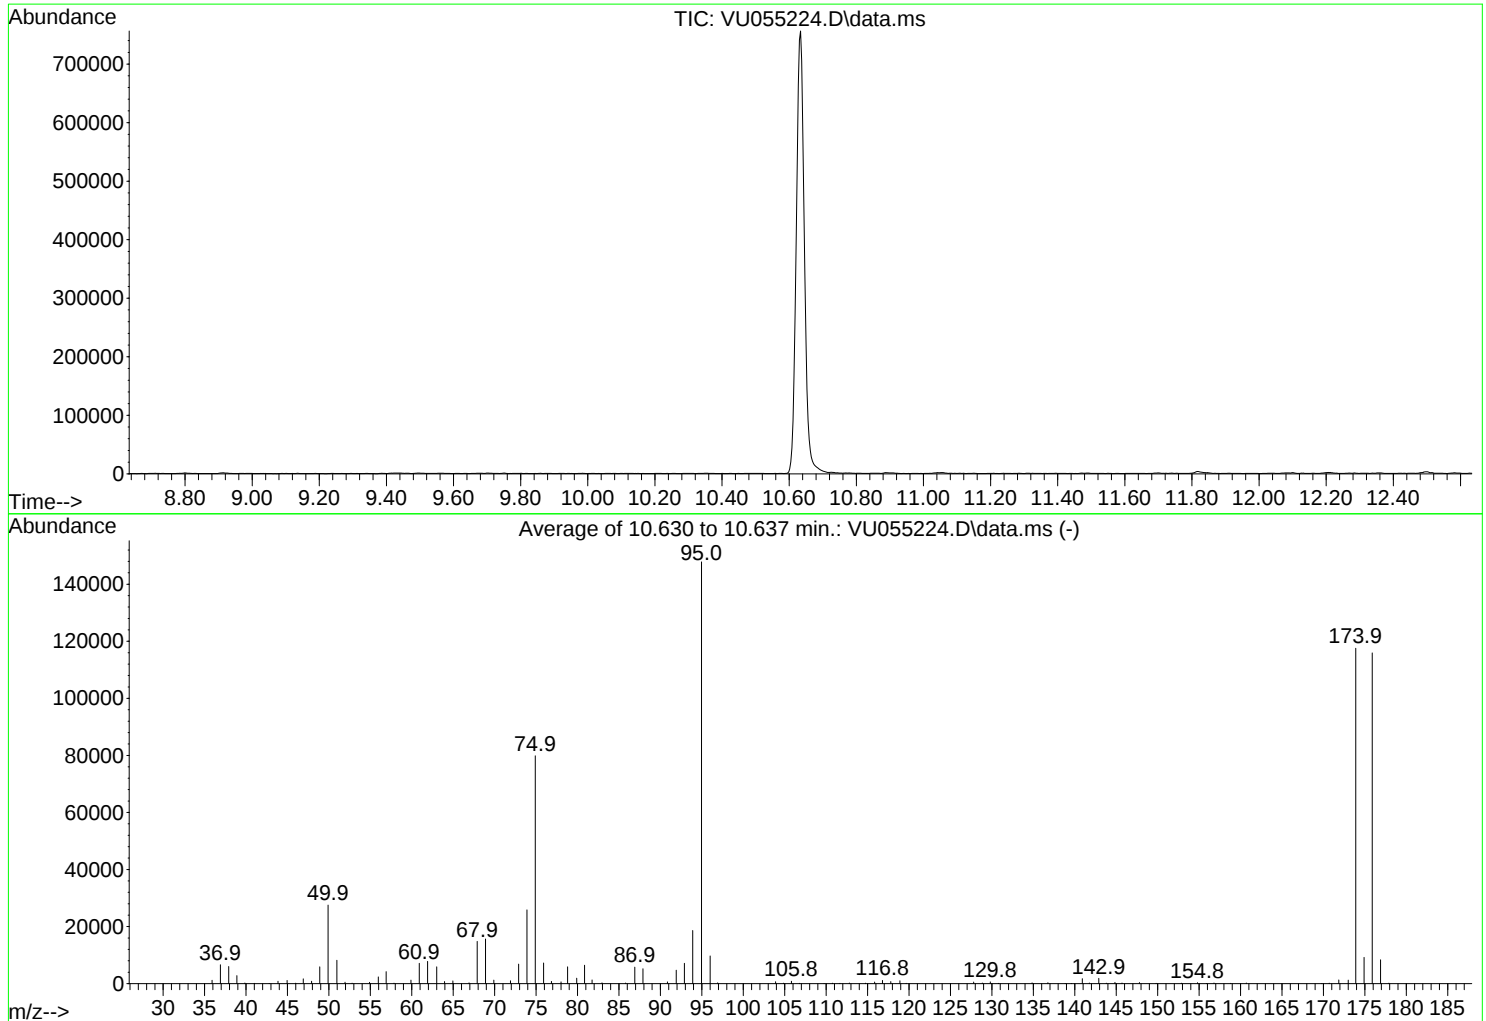

AutoFind: Scans 2905, 2906, 2907; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	27547	PASS
75	95	30	60	54.0	79864	PASS
95	95	100	100	100.0	147840	PASS
96	95	5	9	6.6	9693	PASS
173	174	0.00	2	1.0	1213	PASS
174	95	50	100	79.5	117552	PASS
175	174	5	9	7.9	9230	PASS
176	174	95	101	98.6	115899	PASS
177	176	5	9	7.2	8345	PASS