

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091124\
 Data File : VU060680.D
 Acq On : 11 Sep 2024 13:19
 Operator : MD/SY
 Sample : P3918-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Sep 12 02:21:55 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	4264	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.418	117	6645	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	1974	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	2944	0.424	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	84.000%
4) 1,2-Dichloroethane-d4	5.685	65	1974	0.537	ug/L	-0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	108.000%
7) 1,2-Dichloropropane-d6	6.687	67	1909	0.462	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	92.000%
8) Toluene-d8	7.887	98	4653	0.545	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	110.000%
10) 1,1,2,2-Tetrachloroeth...	10.745	84	1549	0.428	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	86.000%
Target Compounds						
6) Trichloroethene	6.544	95	3071	0.732	ug/L	96
12) 1,2,3-Trichloropropane	10.865	75	40	0.017	ug/L #	62
13) 1,2-Dibromo-3-chloropr...	12.750	75	26	0.058	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091124\
Data File : VU060680.D
Acq On : 11 Sep 2024 13:19
Operator : MD/SY
Sample : P3918-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Sep 12 02:21:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration

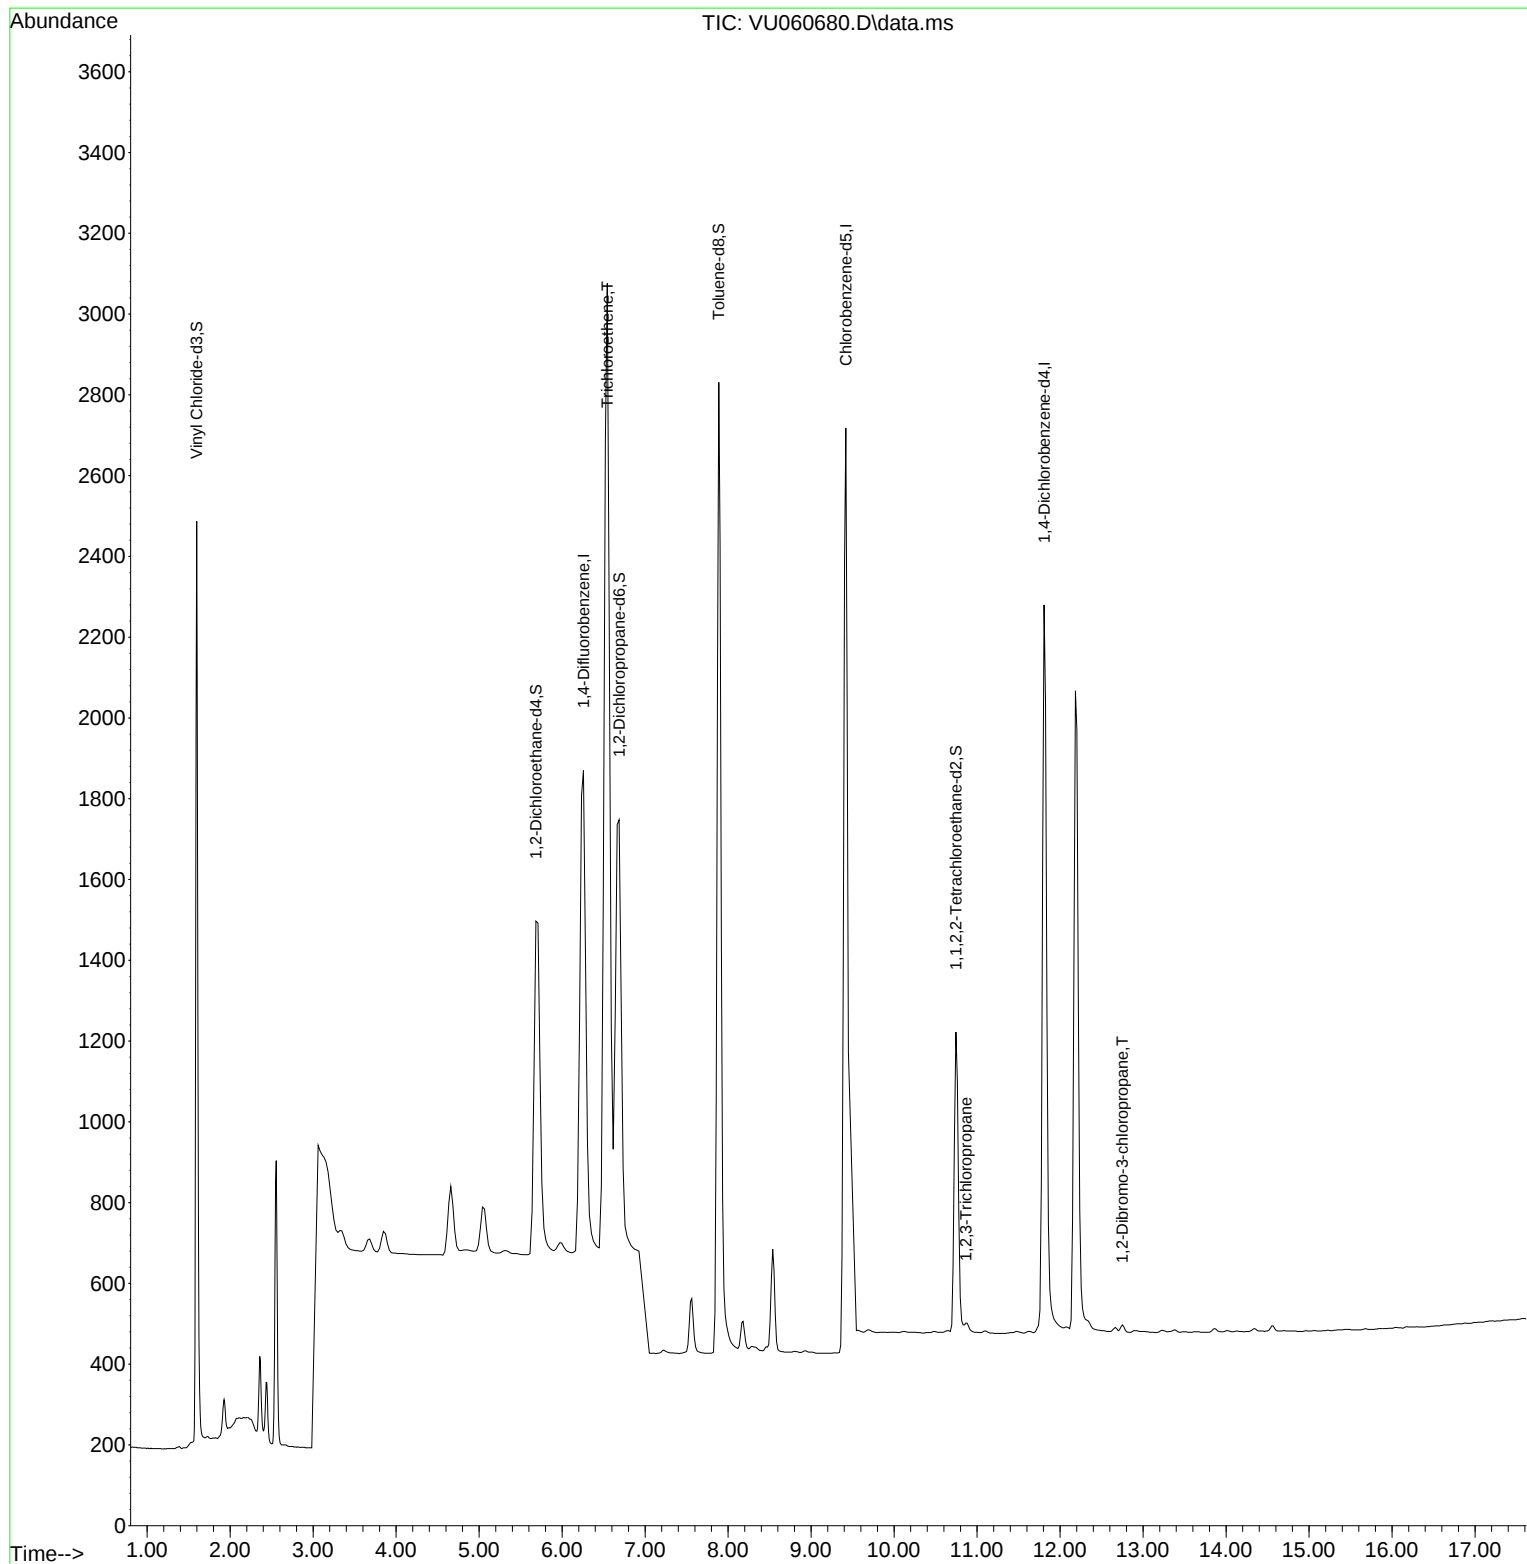

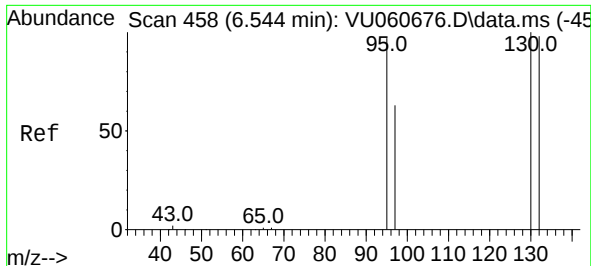




#6
 Trichloroethene
 Concen: 0.732 ug/L
 RT: 6.544 min Scan# 458
 Delta R.T. -0.000 min
 Lab File: VU060680.D
 Acq: 11 Sep 2024 13:19

Instrument :
 MSVOA_U
 ClientSampleId :

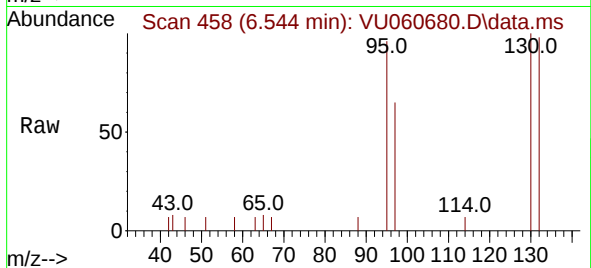

Tgt Ion: 95 Resp: 3071




Ion	Ratio	Lower	Upper
95	100		
97	67.7	48.5	90.1
132	102.3	75.5	140.1
130	103.9	76.3	141.7

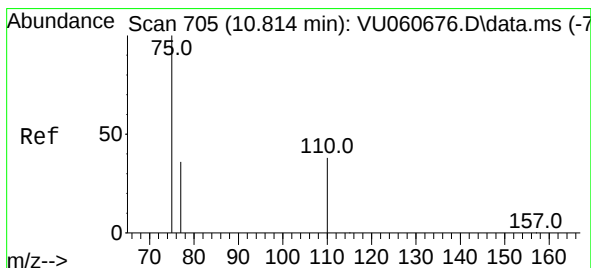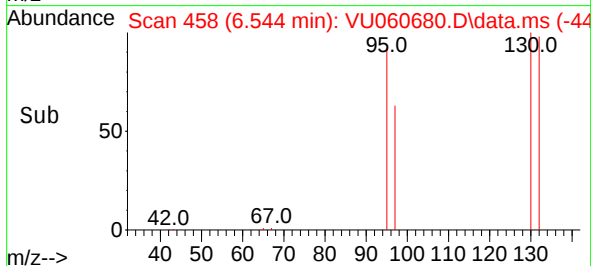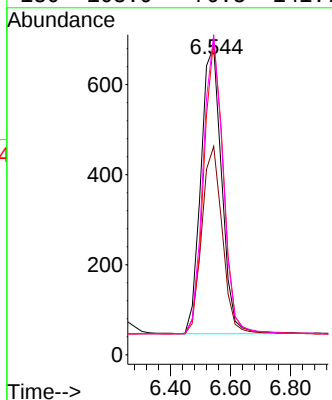


#12
 1,2,3-Trichloropropane
 Concen: 0.017 ug/L
 RT: 10.865 min Scan# 708
 Delta R.T. 0.051 min
 Lab File: VU060680.D
 Acq: 11 Sep 2024 13:19

Tgt Ion: 75 Resp: 40


Ion	Ratio	Lower	Upper
75	100		
110	25.0	32.4	48.6#
77	62.5	26.0	39.0#

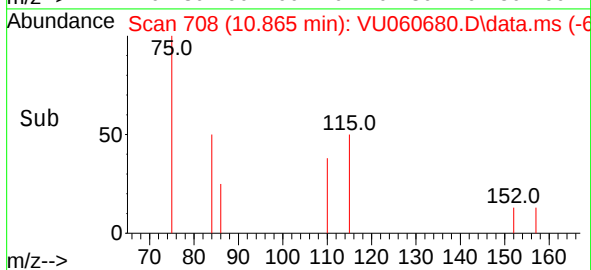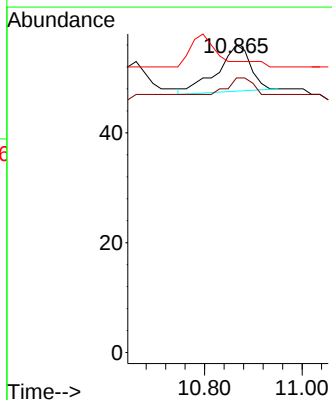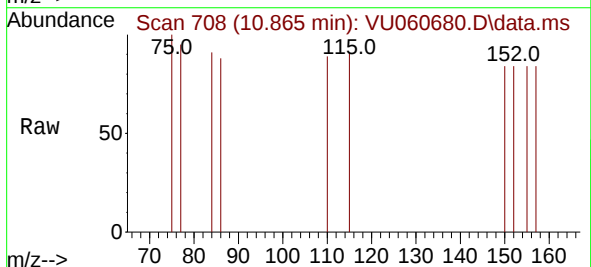

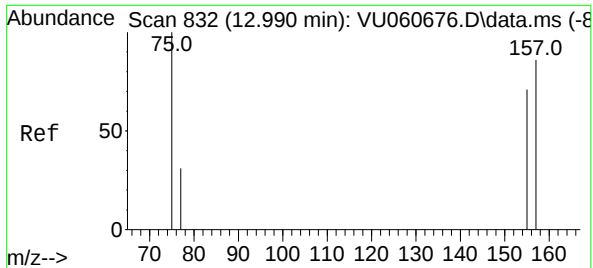

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.058 ug/L
 RT: 12.750 min Scan# 81
 Delta R.T. -0.240 min
 Lab File: VU060680.D
 Acq: 11 Sep 2024 13:19

Instrument :
 MSVOA_U
 ClientSampleId :

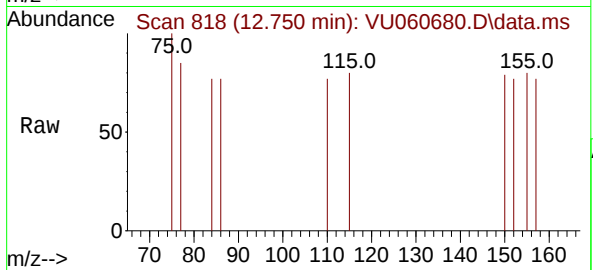

Tgt Ion: 75	Resp:	26
Ion	Ratio	Lower Upper
75	100	
157	77.0	74.3 111.5
155	80.3	66.2 99.2

