

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091124\
 Data File : VU060682.D
 Acq On : 11 Sep 2024 14:06
 Operator : MD/SY
 Sample : P3918-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Sep 12 02:22:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	4199	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.419	117	6415	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	1929	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	2833	0.415	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	82.000%		
4) 1,2-Dichloroethane-d4	5.685	65	1903	0.526	ug/L	-0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	106.000%		
7) 1,2-Dichloropropane-d6	6.687	67	1815	0.455	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	92.000%		
8) Toluene-d8	7.887	98	4452	0.540	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	108.000%		
10) 1,1,2,2-Tetrachloroeth...	10.745	84	1481	0.424	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	84.000%		
Target Compounds						
						Qvalue
6) Trichloroethene	6.544	95	1104	0.272	ug/L	95
13) 1,2-Dibromo-3-chloropr...	12.750	75	33	0.076	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091124\
Data File : VU060682.D
Acq On : 11 Sep 2024 14:06
Operator : MD/SY
Sample : P3918-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Sep 12 02:22:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration

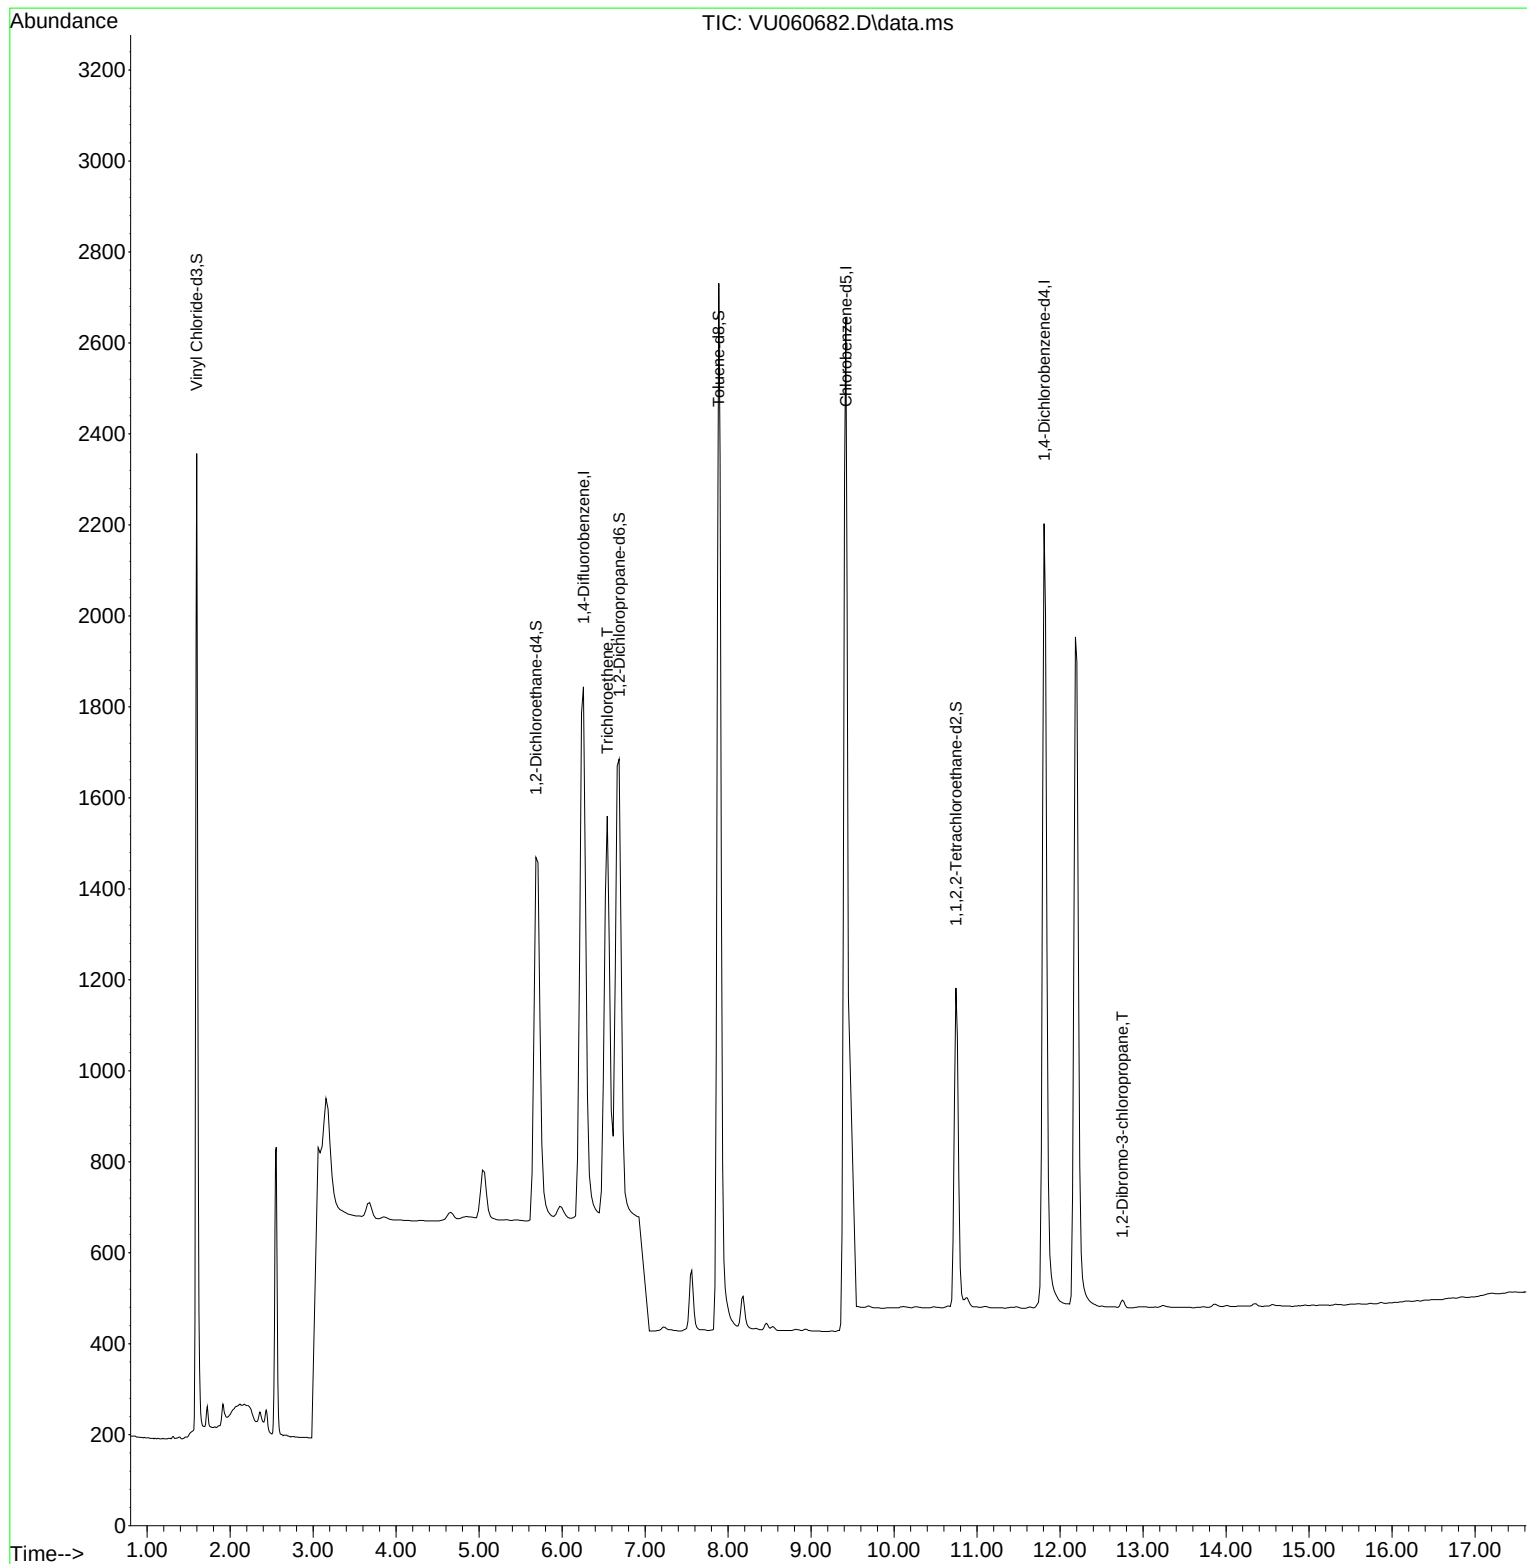

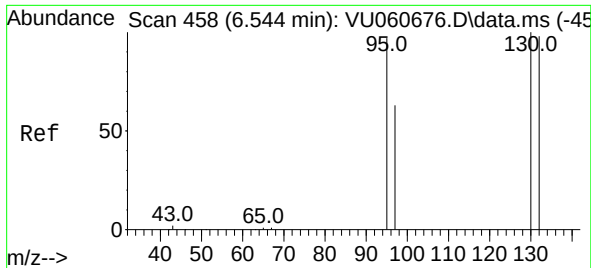




#6
 Trichloroethene
 Concen: 0.272 ug/L
 RT: 6.544 min Scan# 458
 Delta R.T. 0.000 min
 Lab File: VU060682.D
 Acq: 11 Sep 2024 14:06

Instrument :
 MSVOA_U
 ClientSampleId :

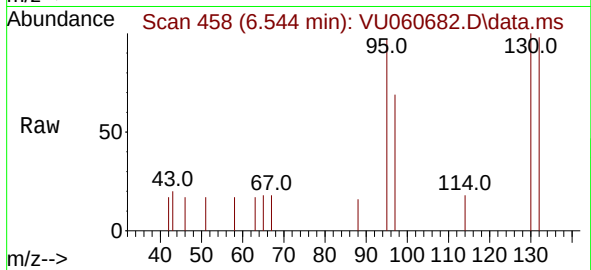

Tgt Ion: 95 Resp: 1104

Ion	Ratio	Lower	Upper
95	100		
97	71.7	48.5	90.1
132	101.4	75.5	140.1
130	103.6	76.3	141.7

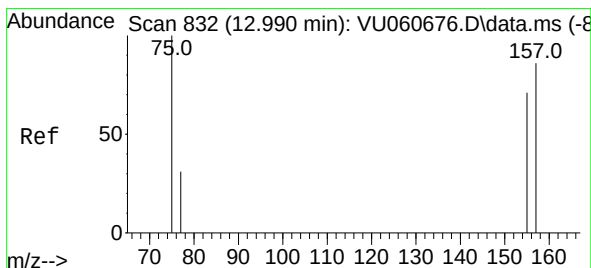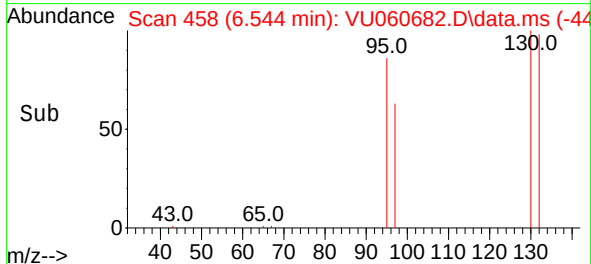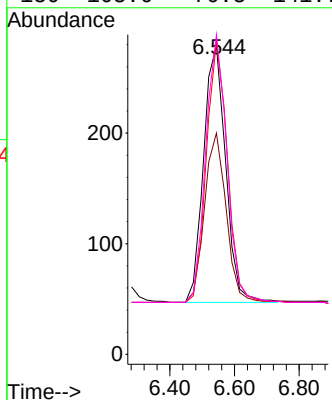

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.076 ug/L
 RT: 12.750 min Scan# 818
 Delta R.T. -0.240 min
 Lab File: VU060682.D
 Acq: 11 Sep 2024 14:06

Tgt Ion: 75 Resp: 33

Ion	Ratio	Lower	Upper
75	100		
157	78.3	74.3	111.5
155	81.7	66.2	99.2

