

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091124\
 Data File : VU060689.D
 Acq On : 11 Sep 2024 17:19
 Operator : MD/SY
 Sample : P3918-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Sep 12 02:23:18 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.257	114	4004	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.418	117	6203	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	1829	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	2634	0.404	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	80.000%
4) 1,2-Dichloroethane-d4	5.685	65	1890	0.548	ug/L	-0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	110.000%
7) 1,2-Dichloropropane-d6	6.687	67	1740	0.451	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	90.000%
8) Toluene-d8	7.887	98	4275	0.537	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	108.000%
10) 1,1,2,2-Tetrachloroeth...	10.745	84	1414	0.419	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	84.000%
Target Compounds						
					Qvalue	
6) Trichloroethene	6.520	95	22434	5.726	ug/L	81
13) 1,2-Dibromo-3-chloropr...	12.750	75	29	0.070	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091124\
Data File : VU060689.D
Acq On : 11 Sep 2024 17:19
Operator : MD/SY
Sample : P3918-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Sep 12 02:23:18 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration

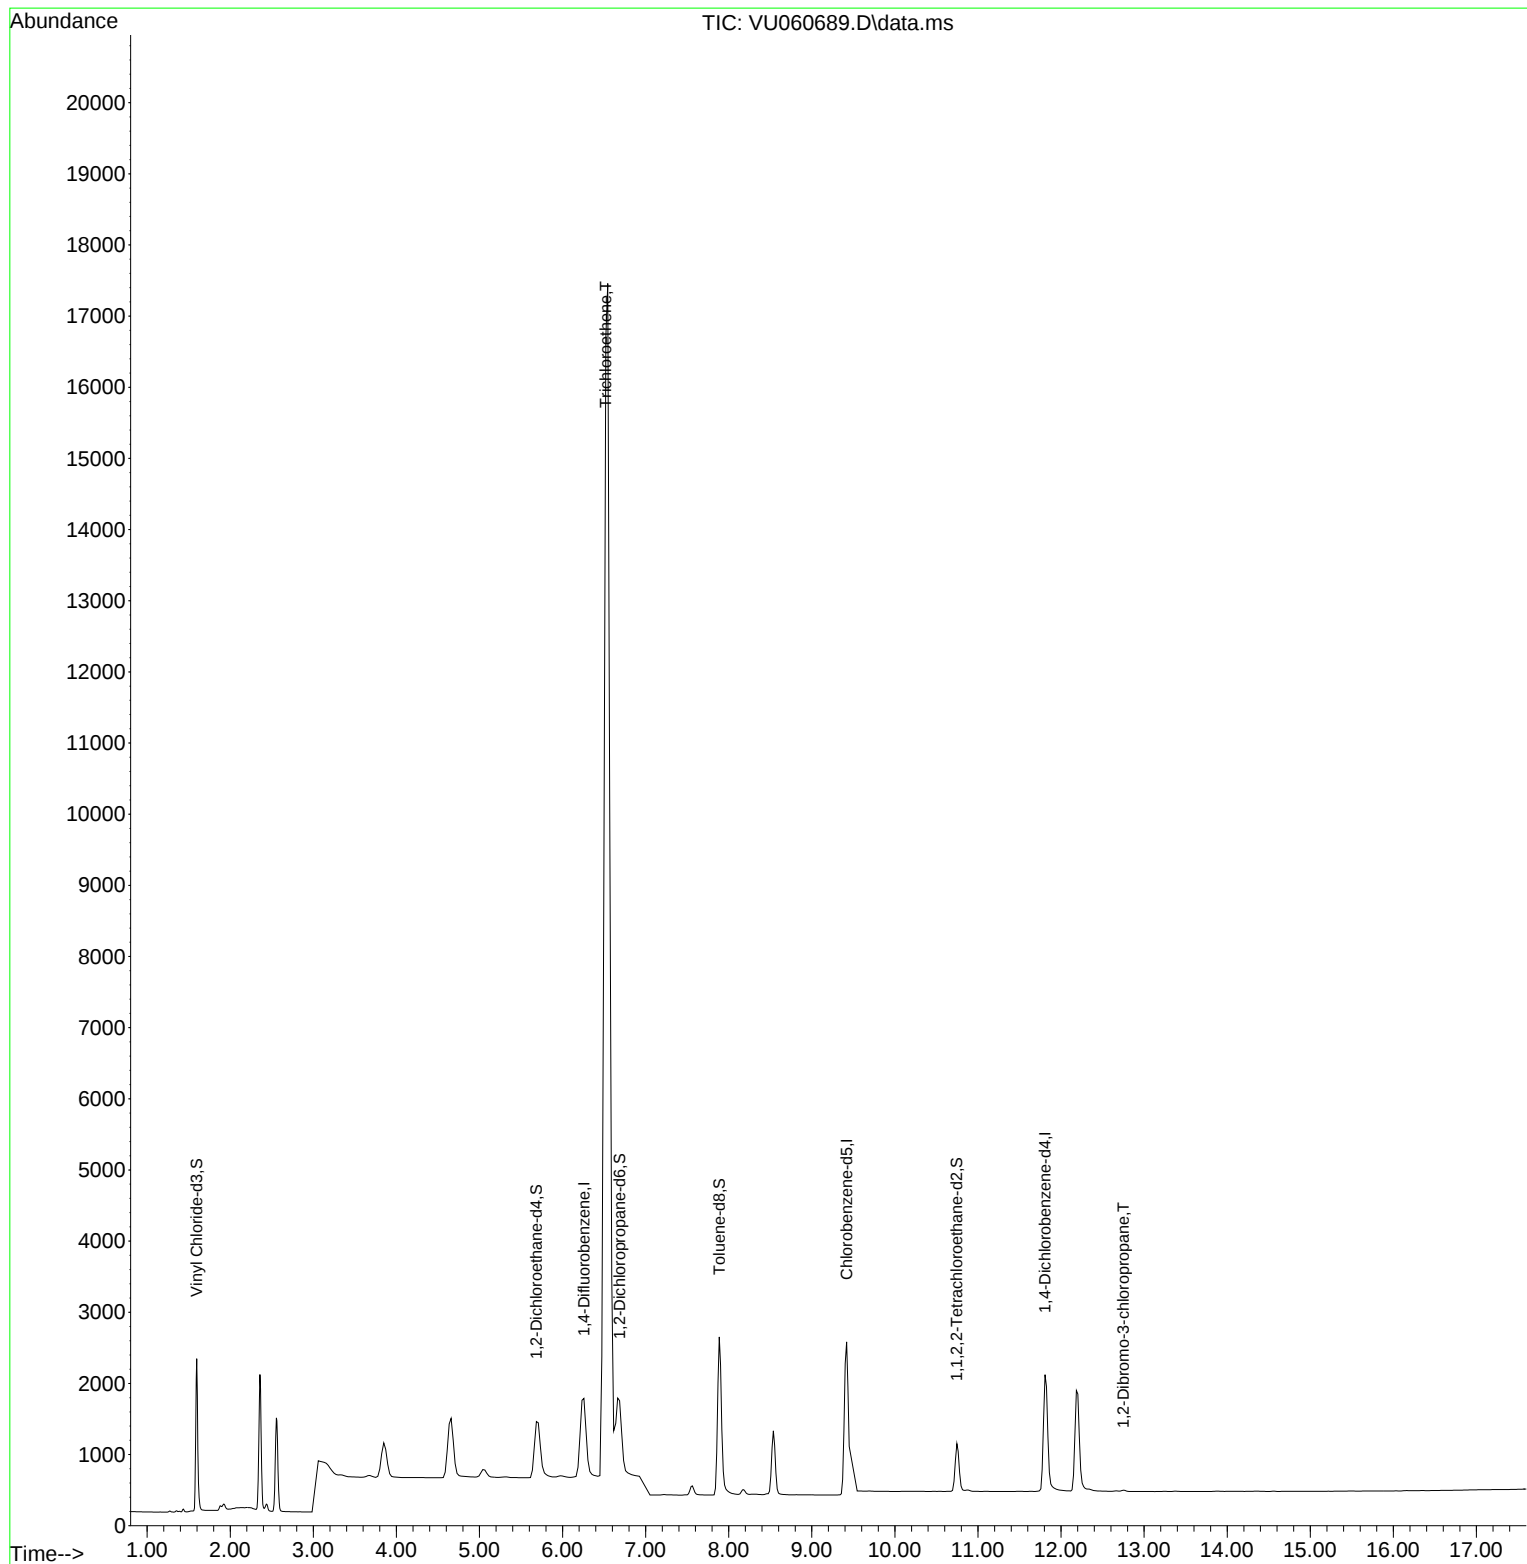

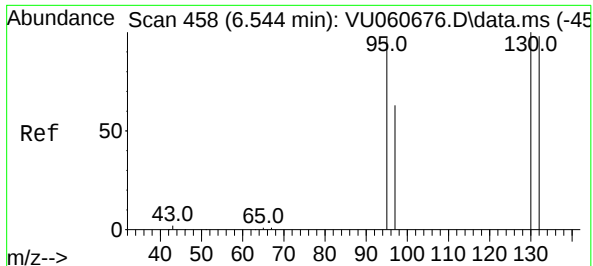




#6
 Trichloroethene
 Concen: 5.726 ug/L
 RT: 6.520 min Scan# 457
 Delta R.T. -0.024 min
 Lab File: VU060689.D
 Acq: 11 Sep 2024 17:19

Instrument :
 MSVOA_U
 ClientSampleId :

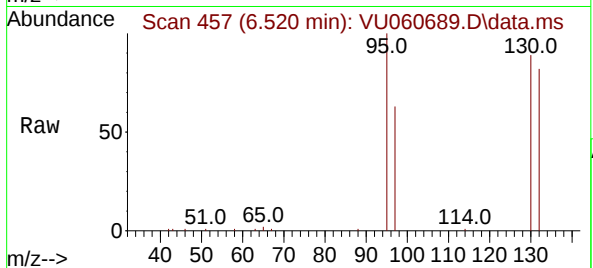

Tgt Ion: 95 Resp: 22434

Ion	Ratio	Lower	Upper
95	100		
97	62.5	48.5	90.1
132	81.5	75.5	140.1
130	88.9	76.3	141.7

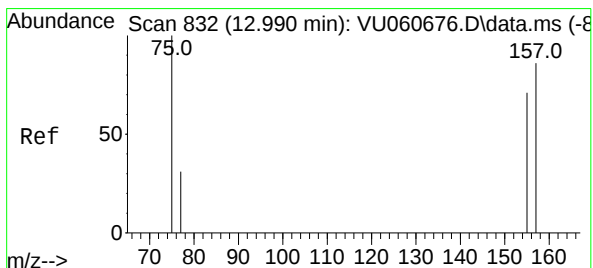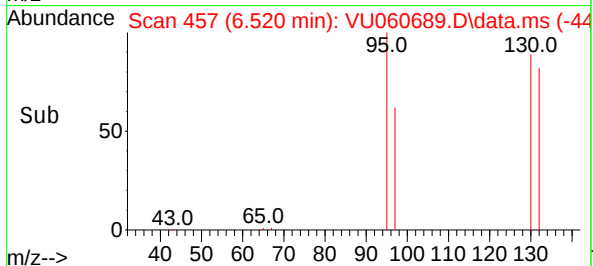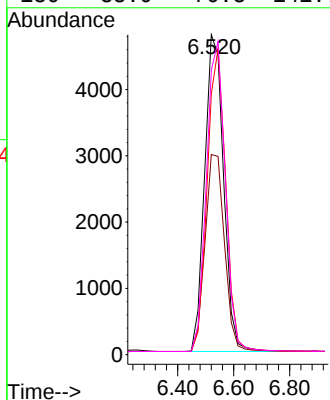

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.070 ug/L
 RT: 12.750 min Scan# 818
 Delta R.T. -0.240 min
 Lab File: VU060689.D
 Acq: 11 Sep 2024 17:19

Tgt Ion: 75 Resp: 29

Ion	Ratio	Lower	Upper
75	100		
157	77.0	74.3	111.5
155	80.3	66.2	99.2

