

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091124\
 Data File : VU060697.D
 Acq On : 11 Sep 2024 20:58
 Operator : MD/SY
 Sample : P3918-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Sep 12 02:51:53 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	3584	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.418	117	5527	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	1594	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	2403	0.412	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	82.000%		
4) 1,2-Dichloroethane-d4	5.685	65	1772	0.574	ug/L	-0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	114.000%		
7) 1,2-Dichloropropane-d6	6.687	67	1613	0.469	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	94.000%		
8) Toluene-d8	7.887	98	3887	0.548	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	110.000%		
10) 1,1,2,2-Tetrachloroeth...	10.745	84	1324	0.440	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	88.000%		
Target Compounds						
6) Trichloroethene	6.520	95	32300	9.253	ug/L	82
12) 1,2,3-Trichloropropane	10.865	75	41	0.022	ug/L #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091124\
Data File : VU060697.D
Acq On : 11 Sep 2024 20:58
Operator : MD/SY
Sample : P3918-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Sep 12 02:51:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration

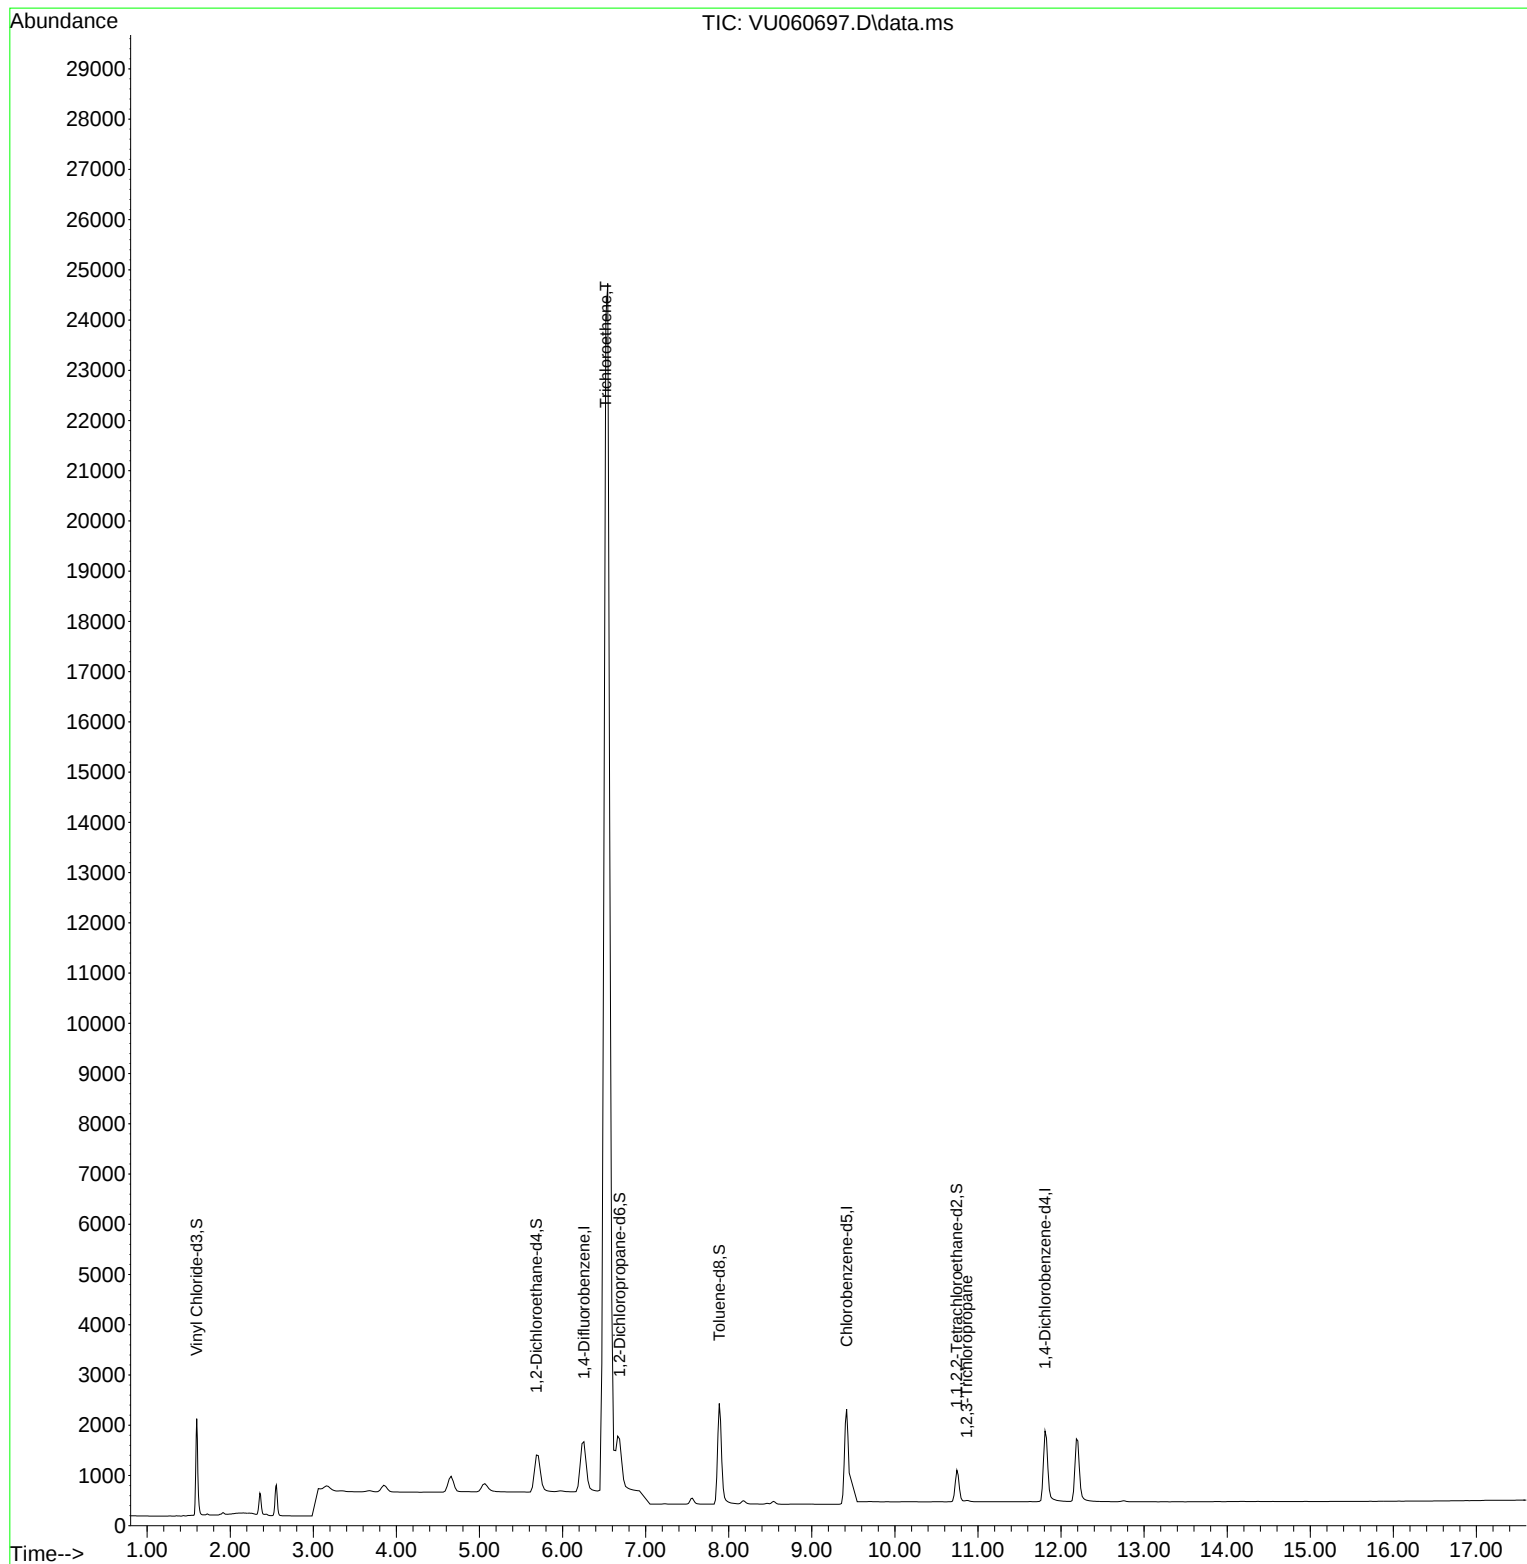

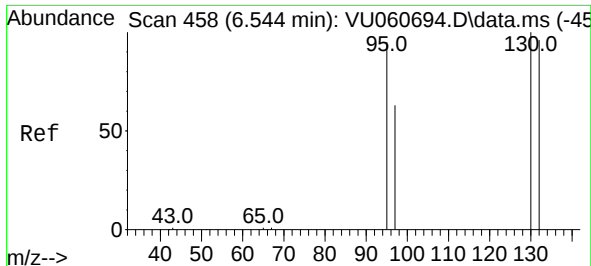




#6
Trichloroethene
Concen: 9.253 ug/L
RT: 6.520 min Scan# 457
Delta R.T. -0.024 min
Lab File: VU060697.D
Acq: 11 Sep 2024 20:58

Instrument :
MSVOA_U
ClientSampleId :

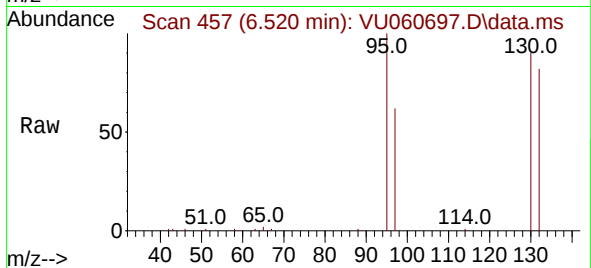

Tgt Ion: 95 Resp: 32300

Ion	Ratio	Lower	Upper
95	100		
97	62.3	48.5	90.1
132	82.1	75.5	140.1
130	89.7	76.3	141.7

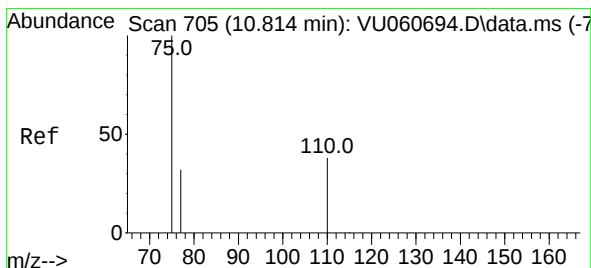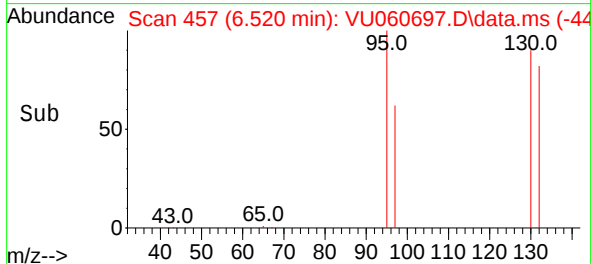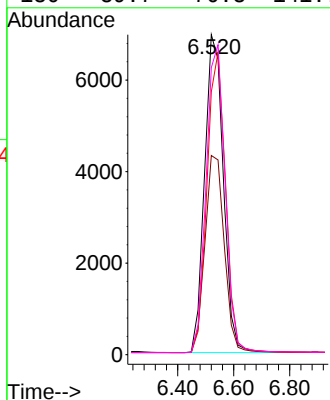

#12
1,2,3-Trichloropropane
Concen: 0.022 ug/L
RT: 10.865 min Scan# 708
Delta R.T. 0.051 min
Lab File: VU060697.D
Acq: 11 Sep 2024 20:58

Tgt Ion: 75 Resp: 41

Ion	Ratio	Lower	Upper
75	100		
110	65.9	32.4	48.6#
77	22.0	26.0	39.0#

