

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091124\
 Data File : VU060701.D
 Acq On : 11 Sep 2024 22:35
 Operator : MD/SY
 Sample : P3918-18
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Sep 12 02:52:29 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	3392	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.419	117	5289	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	1520	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	2292	0.415	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	84.000%		
4) 1,2-Dichloroethane-d4	5.685	65	1635	0.559	ug/L	-0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	112.000%		
7) 1,2-Dichloropropane-d6	6.687	67	1510	0.459	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	92.000%		
8) Toluene-d8	7.887	98	3526	0.519	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	104.000%		
10) 1,1,2,2-Tetrachloroeth...	10.745	84	1246	0.433	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	86.000%		
Target Compounds						
					Qvalue	
6) Trichloroethene	6.544	95	73	0.022	ug/L #	85
13) 1,2-Dibromo-3-chloropr...	12.750	75	26	0.076	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091124\
Data File : VU060701.D
Acq On : 11 Sep 2024 22:35
Operator : MD/SY
Sample : P3918-18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Sep 12 02:52:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration

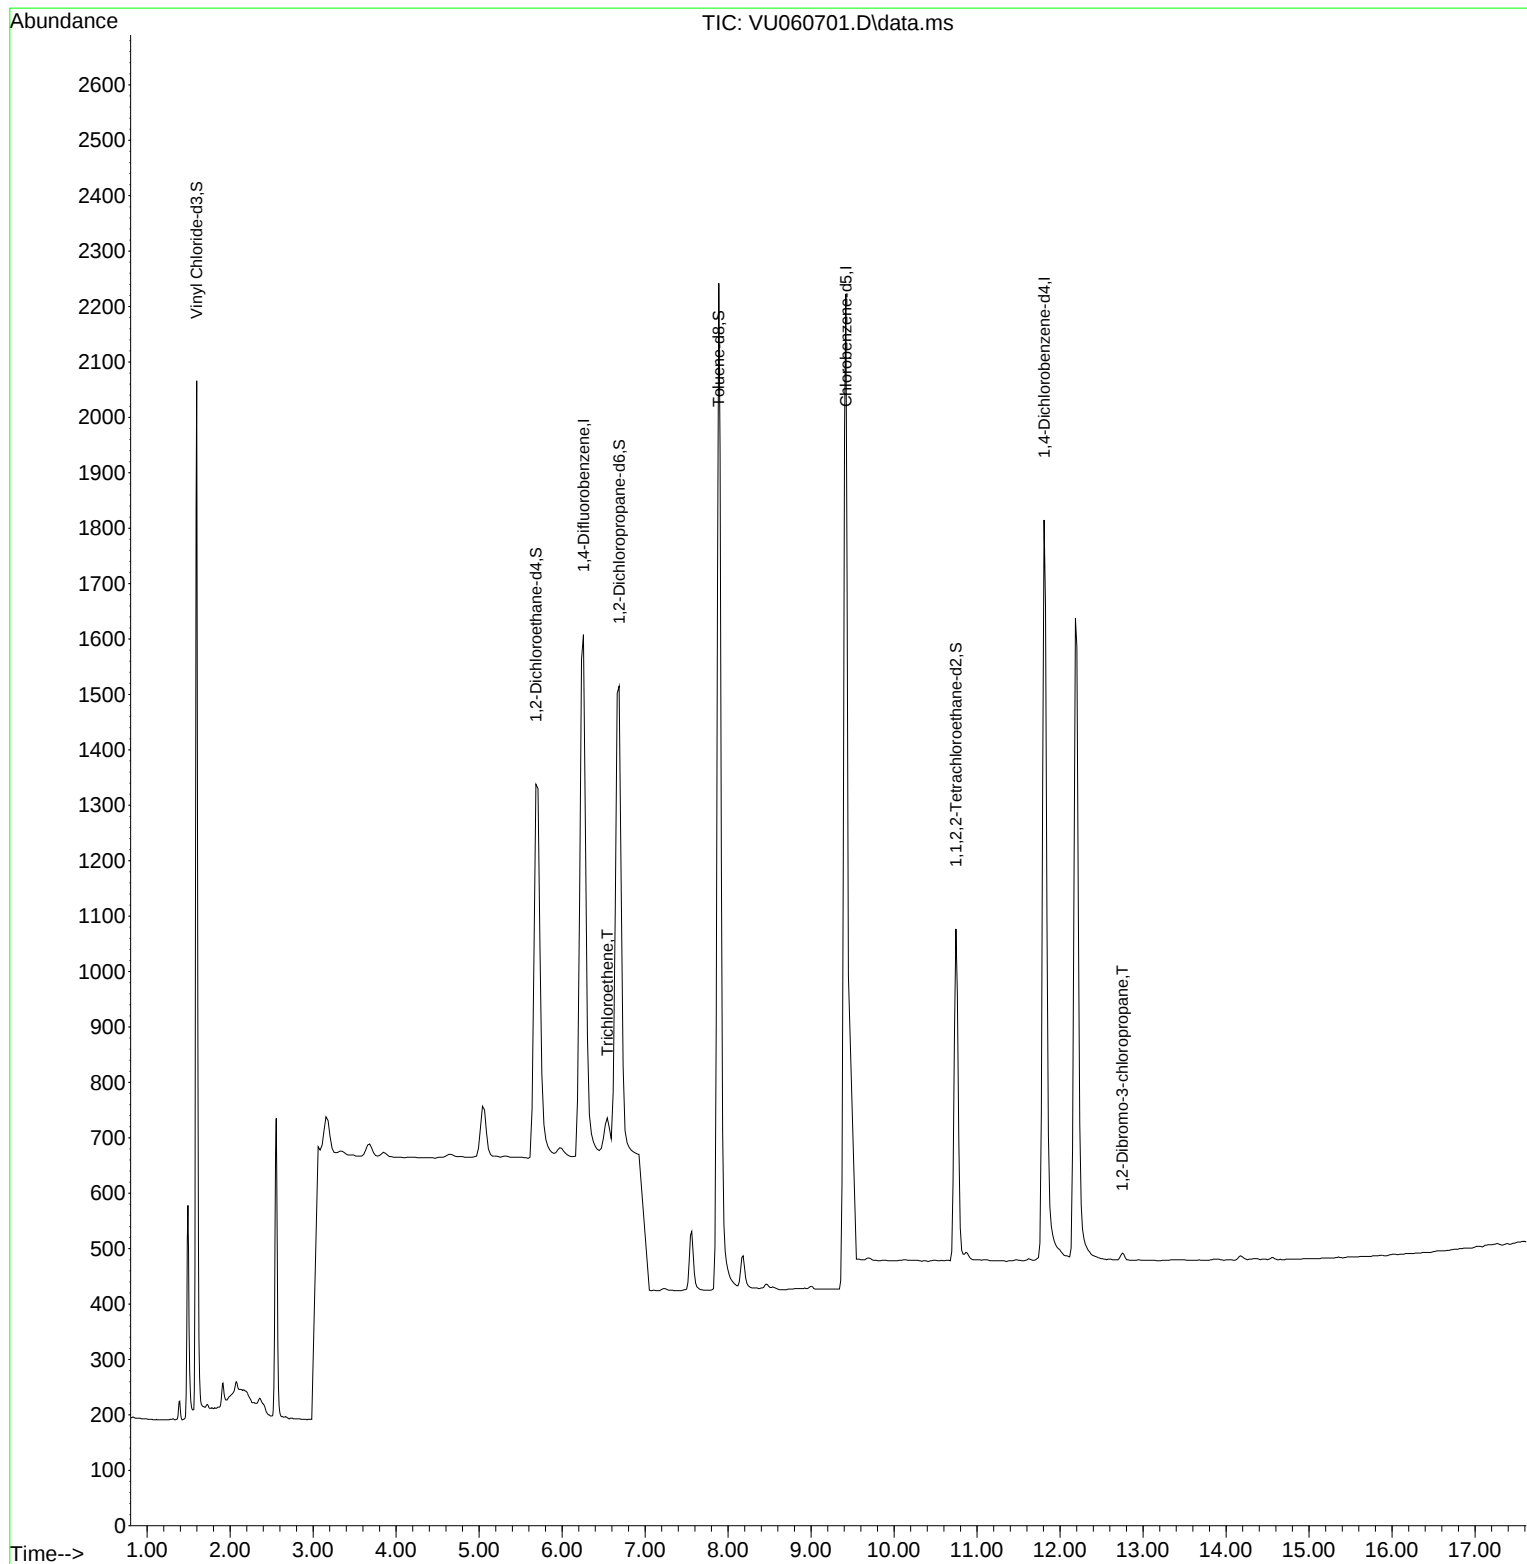

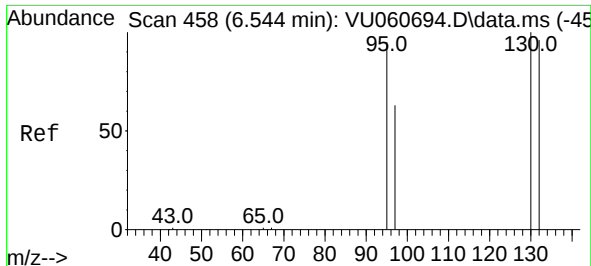




#6
 Trichloroethene
 Concen: 0.022 ug/L
 RT: 6.544 min Scan# 458
 Delta R.T. 0.000 min
 Lab File: VU060701.D
 Acq: 11 Sep 2024 22:35

Instrument :
 MSVOA_U
 ClientSampleId :

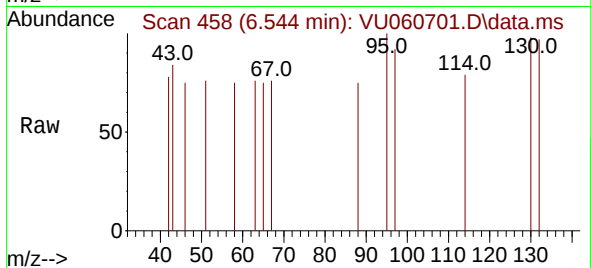


Tgt Ion: 95 Resp: 73

Ion	Ratio	Lower	Upper
95	100		
97	92.1	48.5	90.1#
132	96.8	75.5	140.1
130	98.4	76.3	141.7

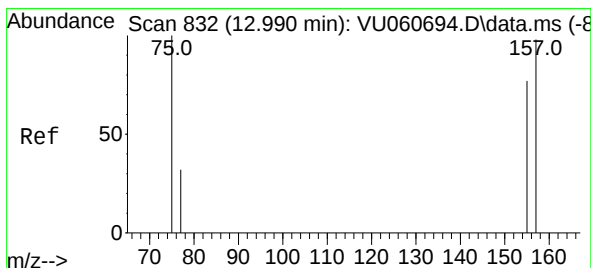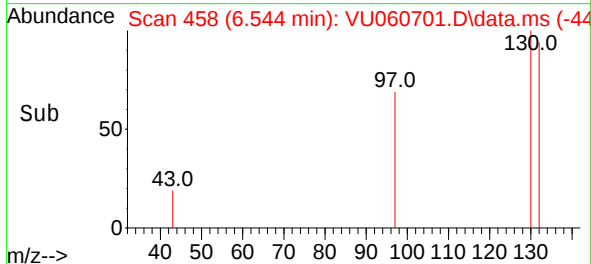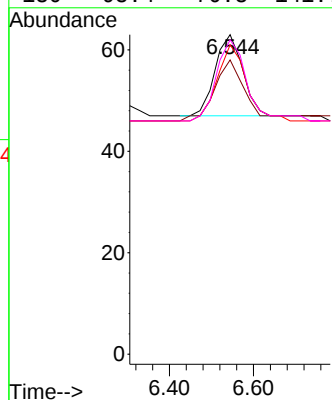

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.076 ug/L
 RT: 12.750 min Scan# 818
 Delta R.T. -0.240 min
 Lab File: VU060701.D
 Acq: 11 Sep 2024 22:35

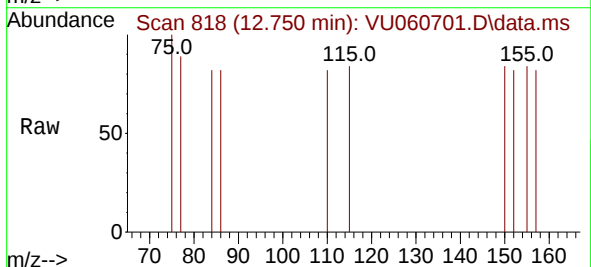

Tgt Ion: 75 Resp: 26

Ion	Ratio	Lower	Upper
75	100		
157	82.5	74.3	111.5
155	84.2	66.2	99.2

