

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091124\
 Data File : VU060707.D
 Acq On : 12 Sep 2024 09:18
 Operator : MD/SY
 Sample : VU0911WBL03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Sep 13 05:21:50 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	4489	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.419	117	6731	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	1867	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	2972	0.407	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	82.000%
4) 1,2-Dichloroethane-d4	5.685	65	1857	0.480	ug/L	-0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	96.000%
7) 1,2-Dichloropropane-d6	6.687	67	1976	0.472	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	94.000%
8) Toluene-d8	7.888	98	4598	0.532	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	106.000%
10) 1,1,2,2-Tetrachloroeth...	10.745	84	1587	0.433	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	86.000%
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.751	75	21	0.050	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091124\
Data File : VU060707.D
Acq On : 12 Sep 2024 09:18
Operator : MD/SY
Sample : VU0911WBL03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Sep 13 05:21:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration

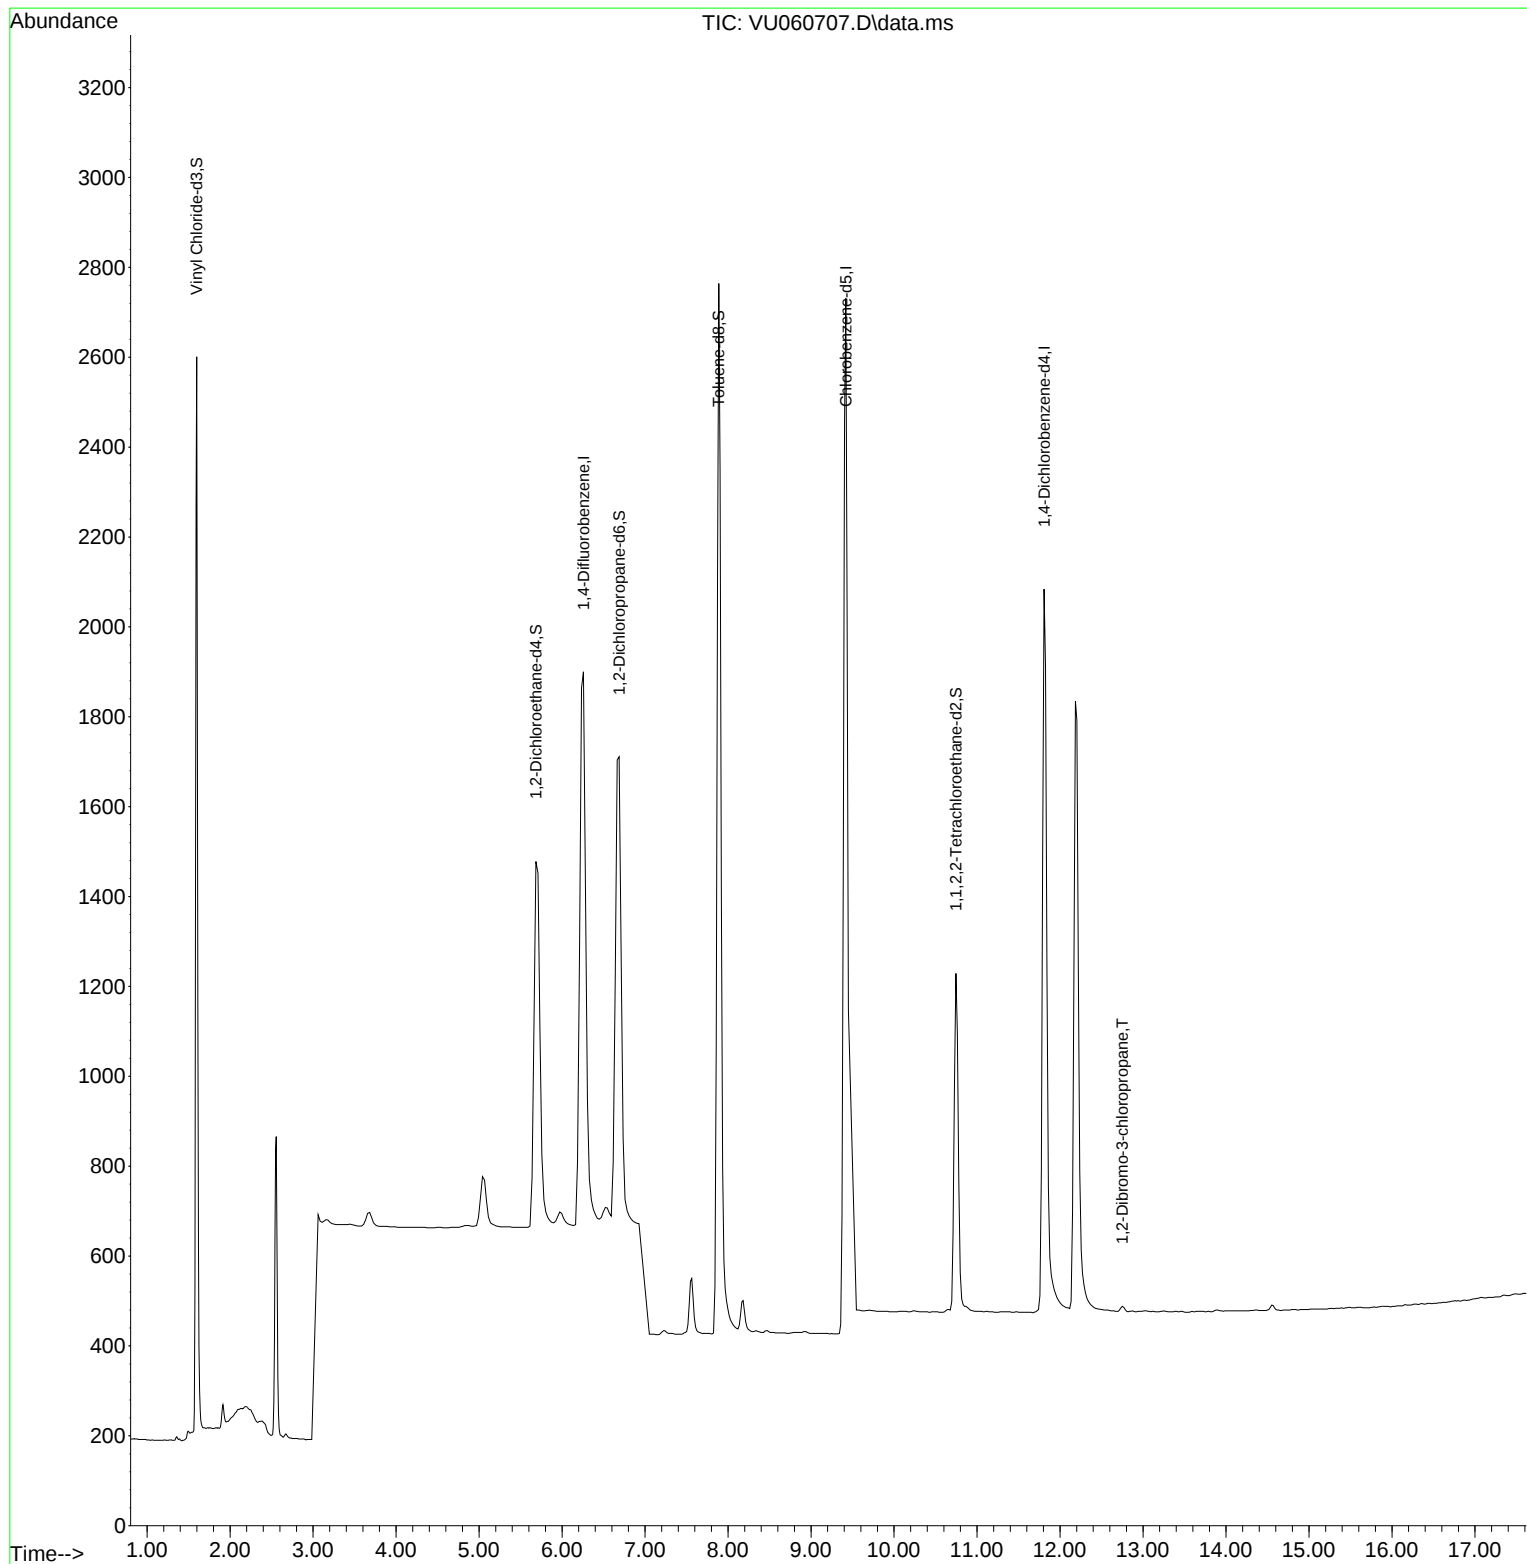

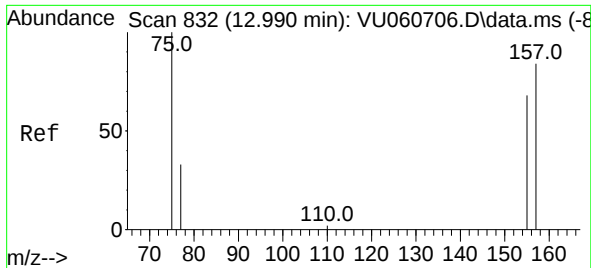

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.050 ug/L
 RT: 12.751 min Scan# 81
 Delta R.T. -0.240 min
 Lab File: VU060707.D
 Acq: 12 Sep 2024 09:18

Instrument :
 MSVOA_U
 ClientSampleId :

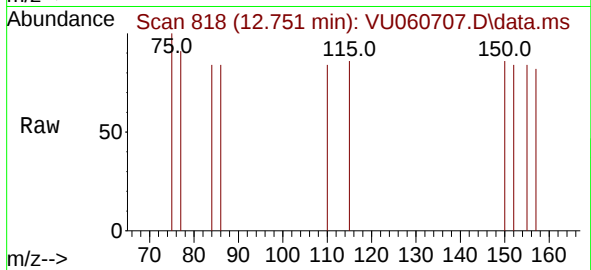

Tgt Ion: 75 Resp: 21
 Ion Ratio Lower Upper
 75 100
 157 82.1 74.3 111.5
 155 83.9 66.2 99.2

