

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091124\
 Data File : VU060684.D
 Acq On : 11 Sep 2024 15:17
 Operator : MD/SY
 Sample : P3918-05DL 5X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AP0DL

Quant Time: Sep 12 02:22:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	4168	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.418	117	6372	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	1879	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	3191	0.471	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	94.000%		
4) 1,2-Dichloroethane-d4	5.685	65	2255	0.628	ug/L	-0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	126.000%		
7) 1,2-Dichloropropane-d6	6.687	67	2145	0.542	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	108.000%		
8) Toluene-d8	7.887	98	5252	0.642	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	128.000%		
10) 1,1,2,2-Tetrachloroeth...	10.745	84	1669	0.481	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	96.000%		
Target Compounds					Qvalue	
6) Trichloroethene	6.544	95	3765	0.936	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091124\
Data File : VU060684.D
Acq On : 11 Sep 2024 15:17
Operator : MD/SY
Sample : P3918-05DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AP0DL


Quant Time: Sep 12 02:22:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration

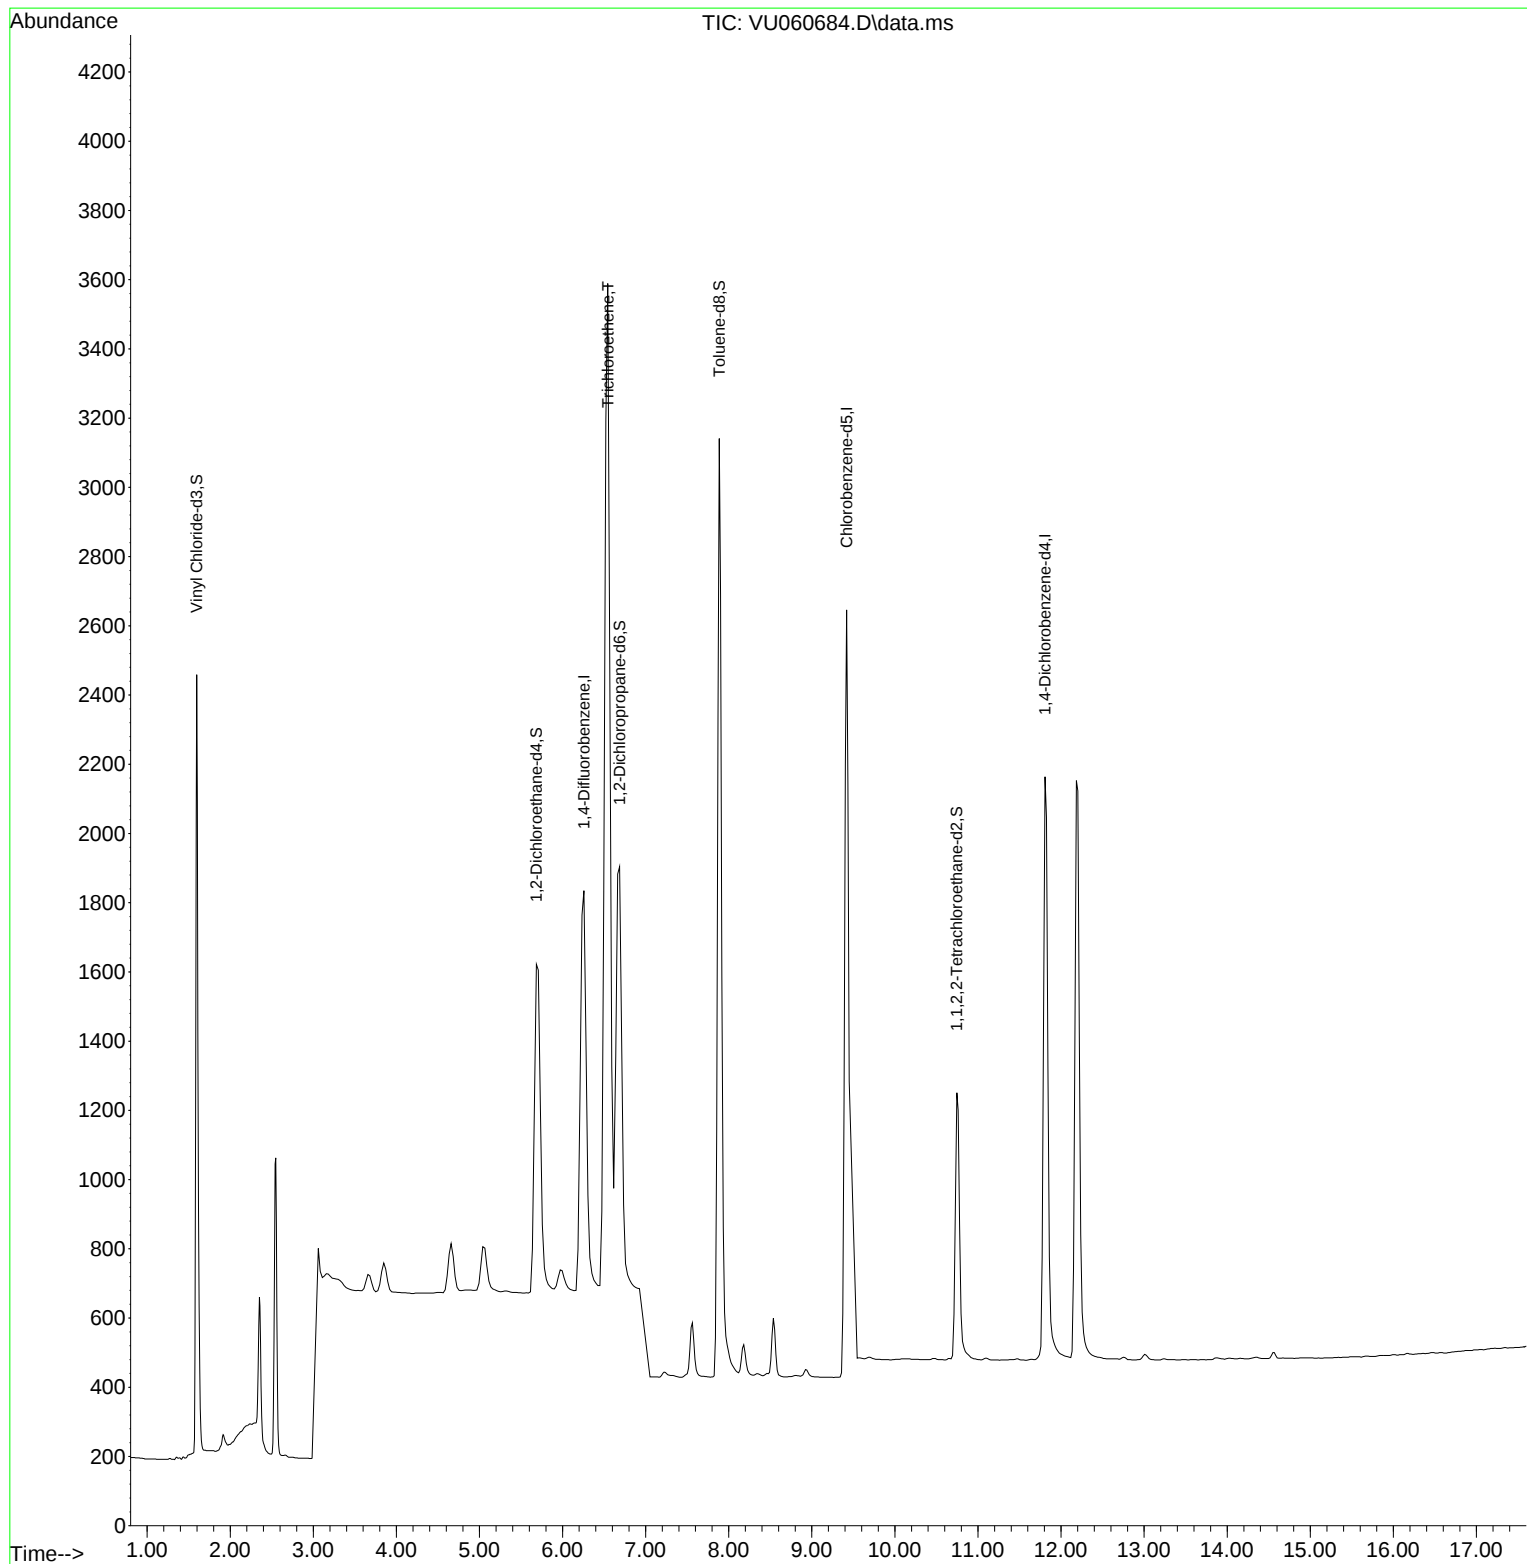

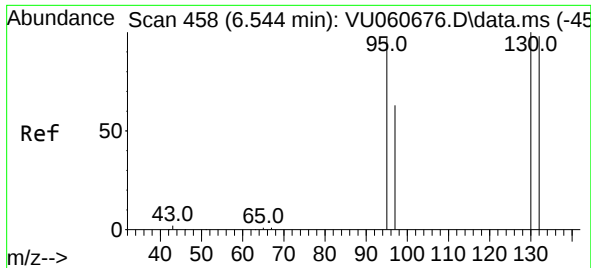

#6
 Trichloroethene
 Concen: 0.936 ug/L
 RT: 6.544 min Scan# 458
 Delta R.T. -0.000 min
 Lab File: VU060684.D
 Acq: 11 Sep 2024 15:17

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AP0DL

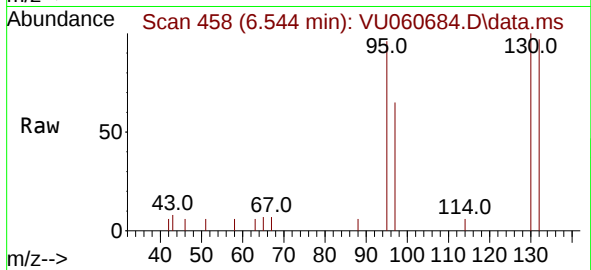

Tgt Ion: 95 Resp: 3765

Ion	Ratio	Lower	Upper
95	100		
97	67.4	48.5	90.1
132	101.1	75.5	140.1
130	103.8	76.3	141.7

