

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU091124\  
 Data File : VU060685.D  
 Acq On : 11 Sep 2024 15:41  
 Operator : MD/SY  
 Sample : P3918-04DL 4X  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 C0AN7DL

Quant Time: Sep 12 02:22:42 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUSIM081624.M  
 Quant Title : TRACE VOA SOM01.0  
 QLast Update : Sat Aug 17 05:03:57 2024  
 Response via : Initial Calibration


| Compound                      | R.T.           | QIon | Response   | Conc     | Units  | Dev(Min) |
|-------------------------------|----------------|------|------------|----------|--------|----------|
| -----                         |                |      |            |          |        |          |
| Internal Standards            |                |      |            |          |        |          |
| 1) 1,4-Difluorobenzene        | 6.258          | 114  | 4318       | 0.500    | ug/L   | 0.00     |
| 5) Chlorobenzene-d5           | 9.418          | 117  | 6615       | 0.500    | ug/L   | 0.00     |
| 11) 1,4-Dichlorobenzene-d4    | 11.808         | 152  | 1948       | 0.500    | ug/L   | 0.00     |
|                               |                |      |            |          |        |          |
| System Monitoring Compounds   |                |      |            |          |        |          |
| 2) Vinyl Chloride-d3          | 1.597          | 65   | 2712       | 0.386    | ug/L   | 0.00     |
| Spiked Amount 0.500           | Range 40 - 130 |      | Recovery = | 78.000%  |        |          |
| 4) 1,2-Dichloroethane-d4      | 5.685          | 65   | 1891       | 0.508    | ug/L   | -0.02    |
| Spiked Amount 0.500           | Range 70 - 130 |      | Recovery = | 102.000% |        |          |
| 7) 1,2-Dichloropropane-d6     | 6.687          | 67   | 1763       | 0.429    | ug/L   | 0.00     |
| Spiked Amount 0.500           | Range 60 - 140 |      | Recovery = | 86.000%  |        |          |
| 8) Toluene-d8                 | 7.887          | 98   | 4486       | 0.528    | ug/L   | 0.00     |
| Spiked Amount 0.500           | Range 70 - 130 |      | Recovery = | 106.000% |        |          |
| 10) 1,1,2,2-Tetrachloroeth... | 10.745         | 84   | 1380       | 0.383    | ug/L   | 0.00     |
| Spiked Amount 0.500           | Range 65 - 120 |      | Recovery = | 76.000%  |        |          |
|                               |                |      |            |          |        |          |
| Target Compounds              |                |      |            |          | Qvalue |          |
| 6) Trichloroethene            | 6.544          | 95   | 2651       | 0.635    | ug/L   | 95       |
| -----                         |                |      |            |          |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU091124\  
Data File : VU060685.D  
Acq On : 11 Sep 2024 15:41  
Operator : MD/SY  
Sample : P3918-04DL 4X  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
C0AN7DL


Quant Time: Sep 12 02:22:42 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUSIM081624.M  
Quant Title : TRACE VOA SOM01.0  
QLast Update : Sat Aug 17 05:03:57 2024  
Response via : Initial Calibration

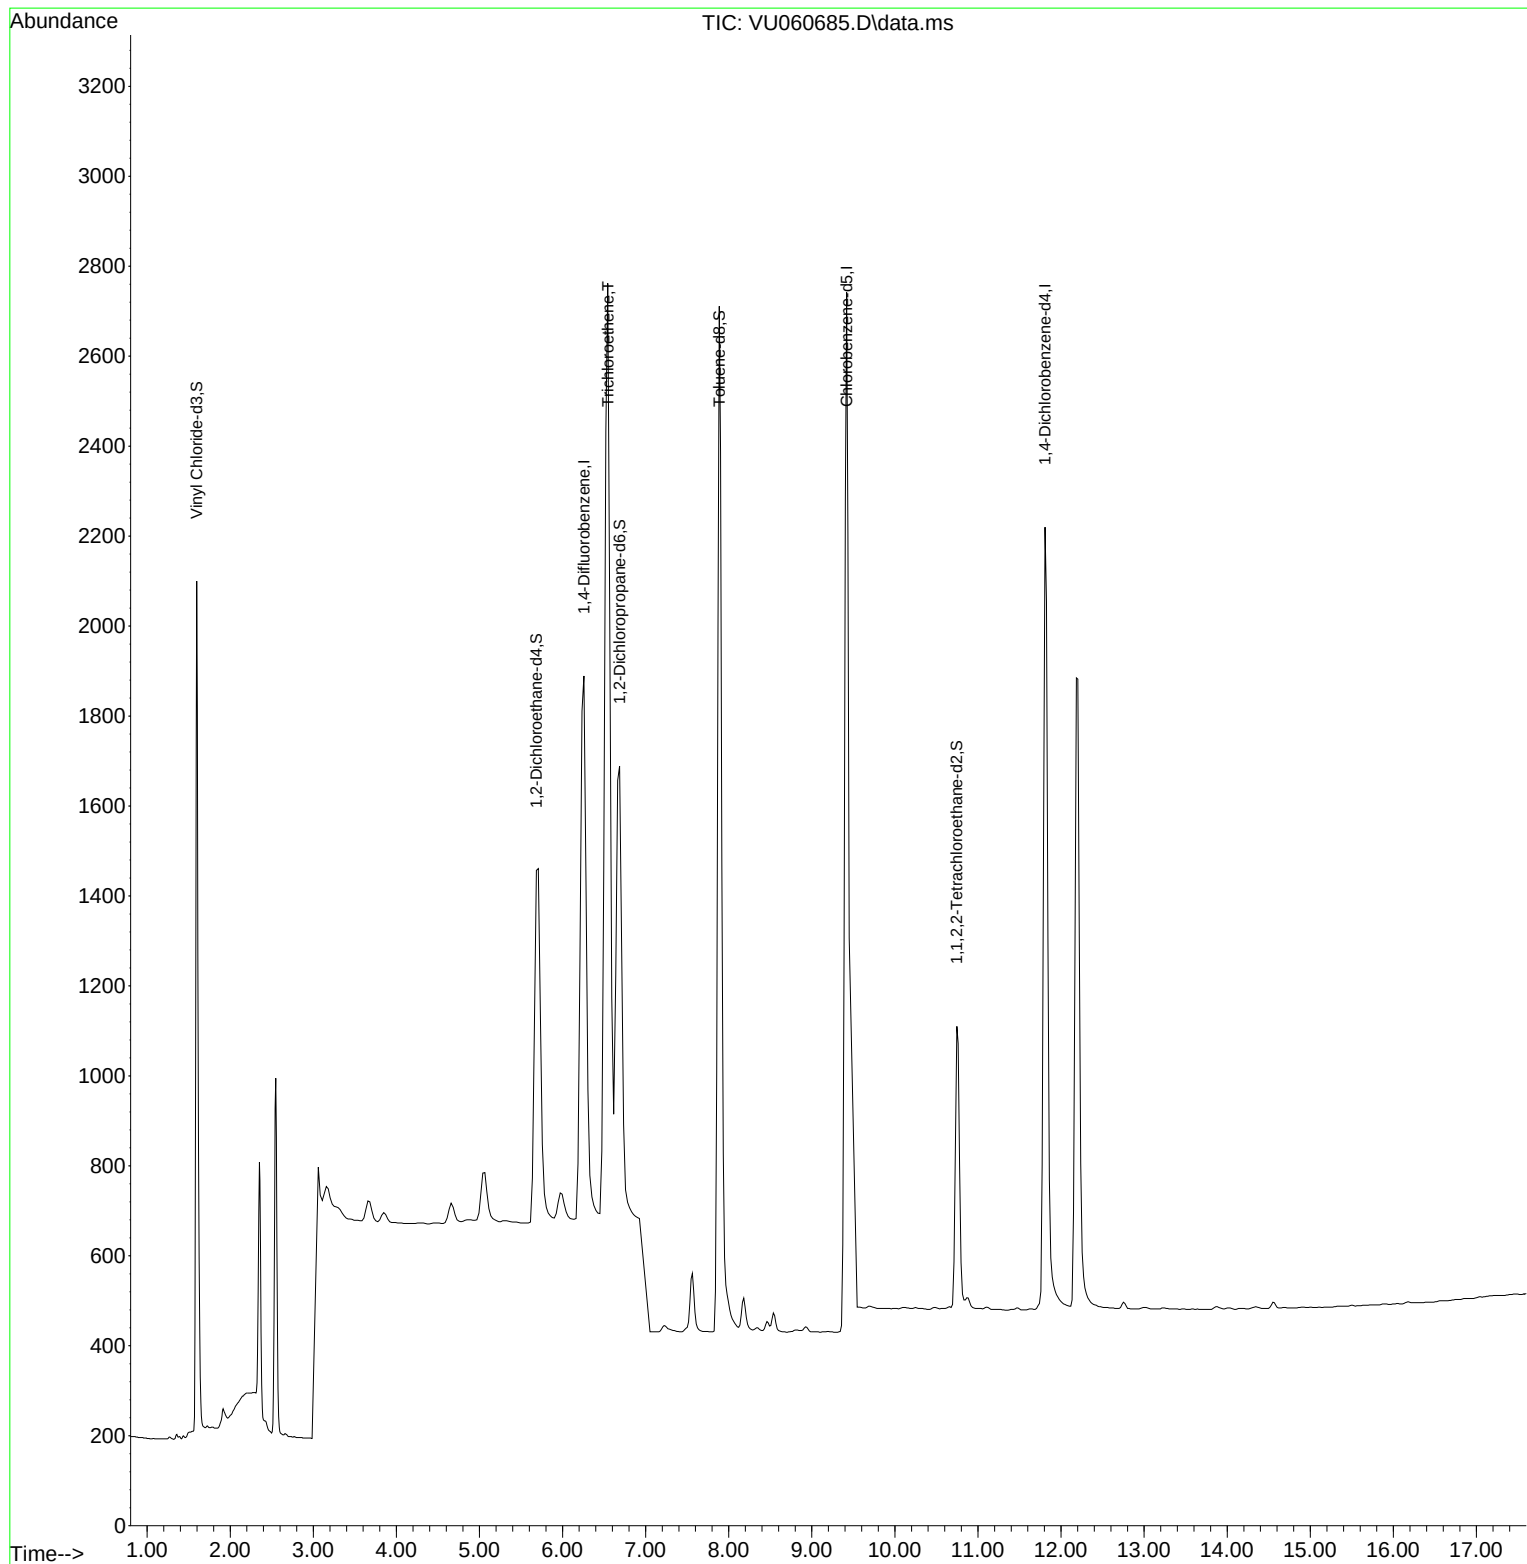

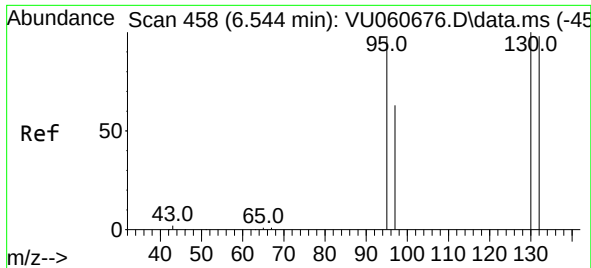

#6  
 Trichloroethene  
 Concen: 0.635 ug/L  
 RT: 6.544 min Scan# 458  
 Delta R.T. -0.000 min  
 Lab File: VU060685.D  
 Acq: 11 Sep 2024 15:41

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 C0AN7DL

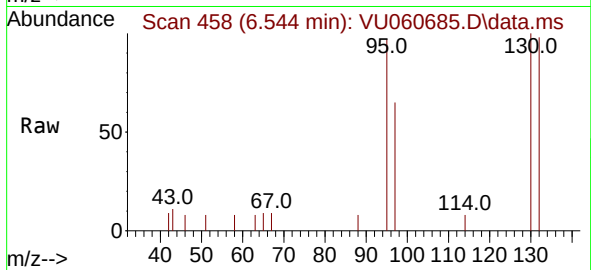

|             |             |
|-------------|-------------|
| Tgt Ion: 95 | Resp: 2651  |
| Ion Ratio   | Lower Upper |
| 95 100      |             |
| 97 67.6     | 48.5 90.1   |
| 132 101.3   | 75.5 140.1  |
| 130 103.2   | 76.3 141.7  |

