

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091124\
 Data File : VU060688.D
 Acq On : 11 Sep 2024 16:55
 Operator : MD/SY
 Sample : P3918-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AN7

Quant Time: Sep 12 02:23:09 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	4789	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.419	117	7236	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	2052	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	2722	0.349	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	70.000%		
4) 1,2-Dichloroethane-d4	5.685	65	1853	0.449	ug/L	-0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	90.000%		
7) 1,2-Dichloropropane-d6	6.687	67	1750	0.389	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	78.000%		
8) Toluene-d8	7.887	98	4180	0.450	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	90.000%		
10) 1,1,2,2-Tetrachloroeth...	10.745	84	1424	0.361	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	72.000%		
Target Compounds						
6) Trichloroethene	6.520	95	10869	2.378	ug/L	Qvalue 81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091124\
Data File : VU060688.D
Acq On : 11 Sep 2024 16:55
Operator : MD/SY
Sample : P3918-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AN7


Quant Time: Sep 12 02:23:09 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration

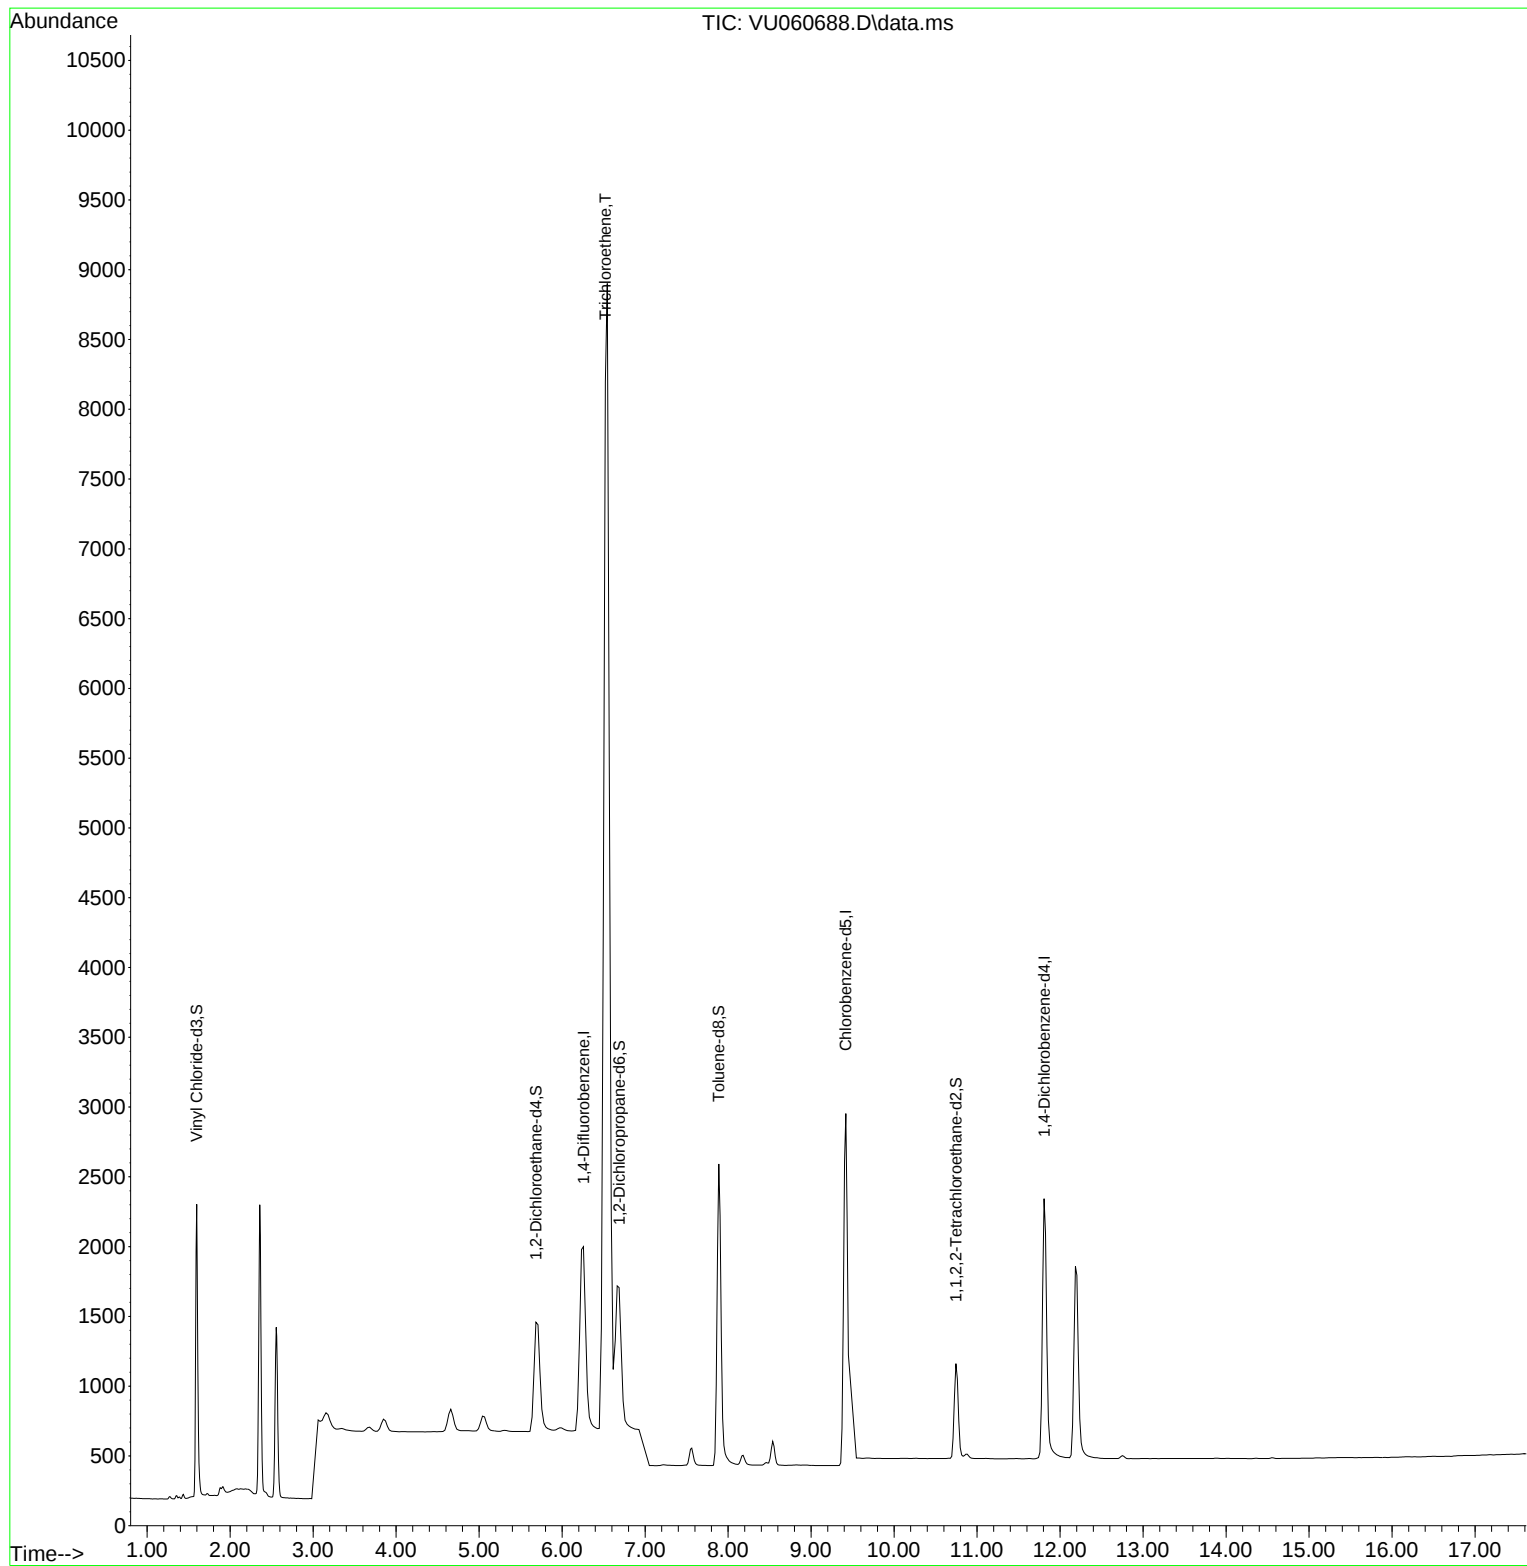

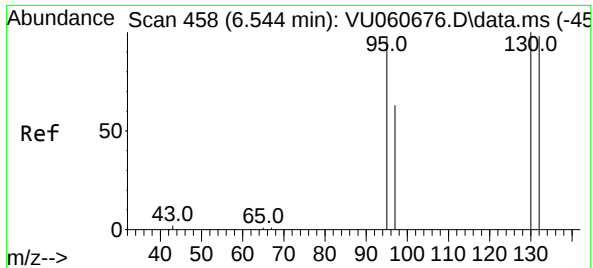

#6
Trichloroethene
Concen: 2.378 ug/L
RT: 6.520 min Scan# 457
Delta R.T. -0.024 min
Lab File: VU060688.D
Acq: 11 Sep 2024 16:55

Instrument :
MSVOA_U
ClientSampleId :
COAN7

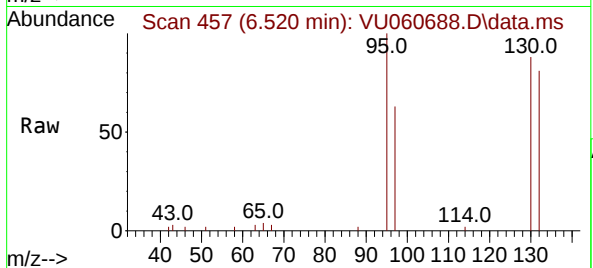

Tgt Ion:	95	Resp:	10869
Ion	Ratio	Lower	Upper
95	100		
97	62.5	48.5	90.1
132	81.5	75.5	140.1
130	88.0	76.3	141.7

