

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091124\
 Data File : VU060702.D
 Acq On : 11 Sep 2024 22:59
 Operator : MD/SY
 Sample : P3918-19
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AQ7

Quant Time: Sep 12 02:52:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	3507	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.419	117	5431	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	1601	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	2461	0.431	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	86.000%		
4) 1,2-Dichloroethane-d4	5.685	65	1722	0.570	ug/L	-0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	114.000%		
7) 1,2-Dichloropropane-d6	6.687	67	1581	0.468	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	94.000%		
8) Toluene-d8	7.887	98	3795	0.544	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	108.000%		
10) 1,1,2,2-Tetrachloroeth...	10.745	84	1269	0.429	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	86.000%		
Target Compounds						
6) Trichloroethene	6.544	95	64	0.019	ug/L	Qvalue # 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091124\
Data File : VU060702.D
Acq On : 11 Sep 2024 22:59
Operator : MD/SY
Sample : P3918-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AQ7


Quant Time: Sep 12 02:52:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration

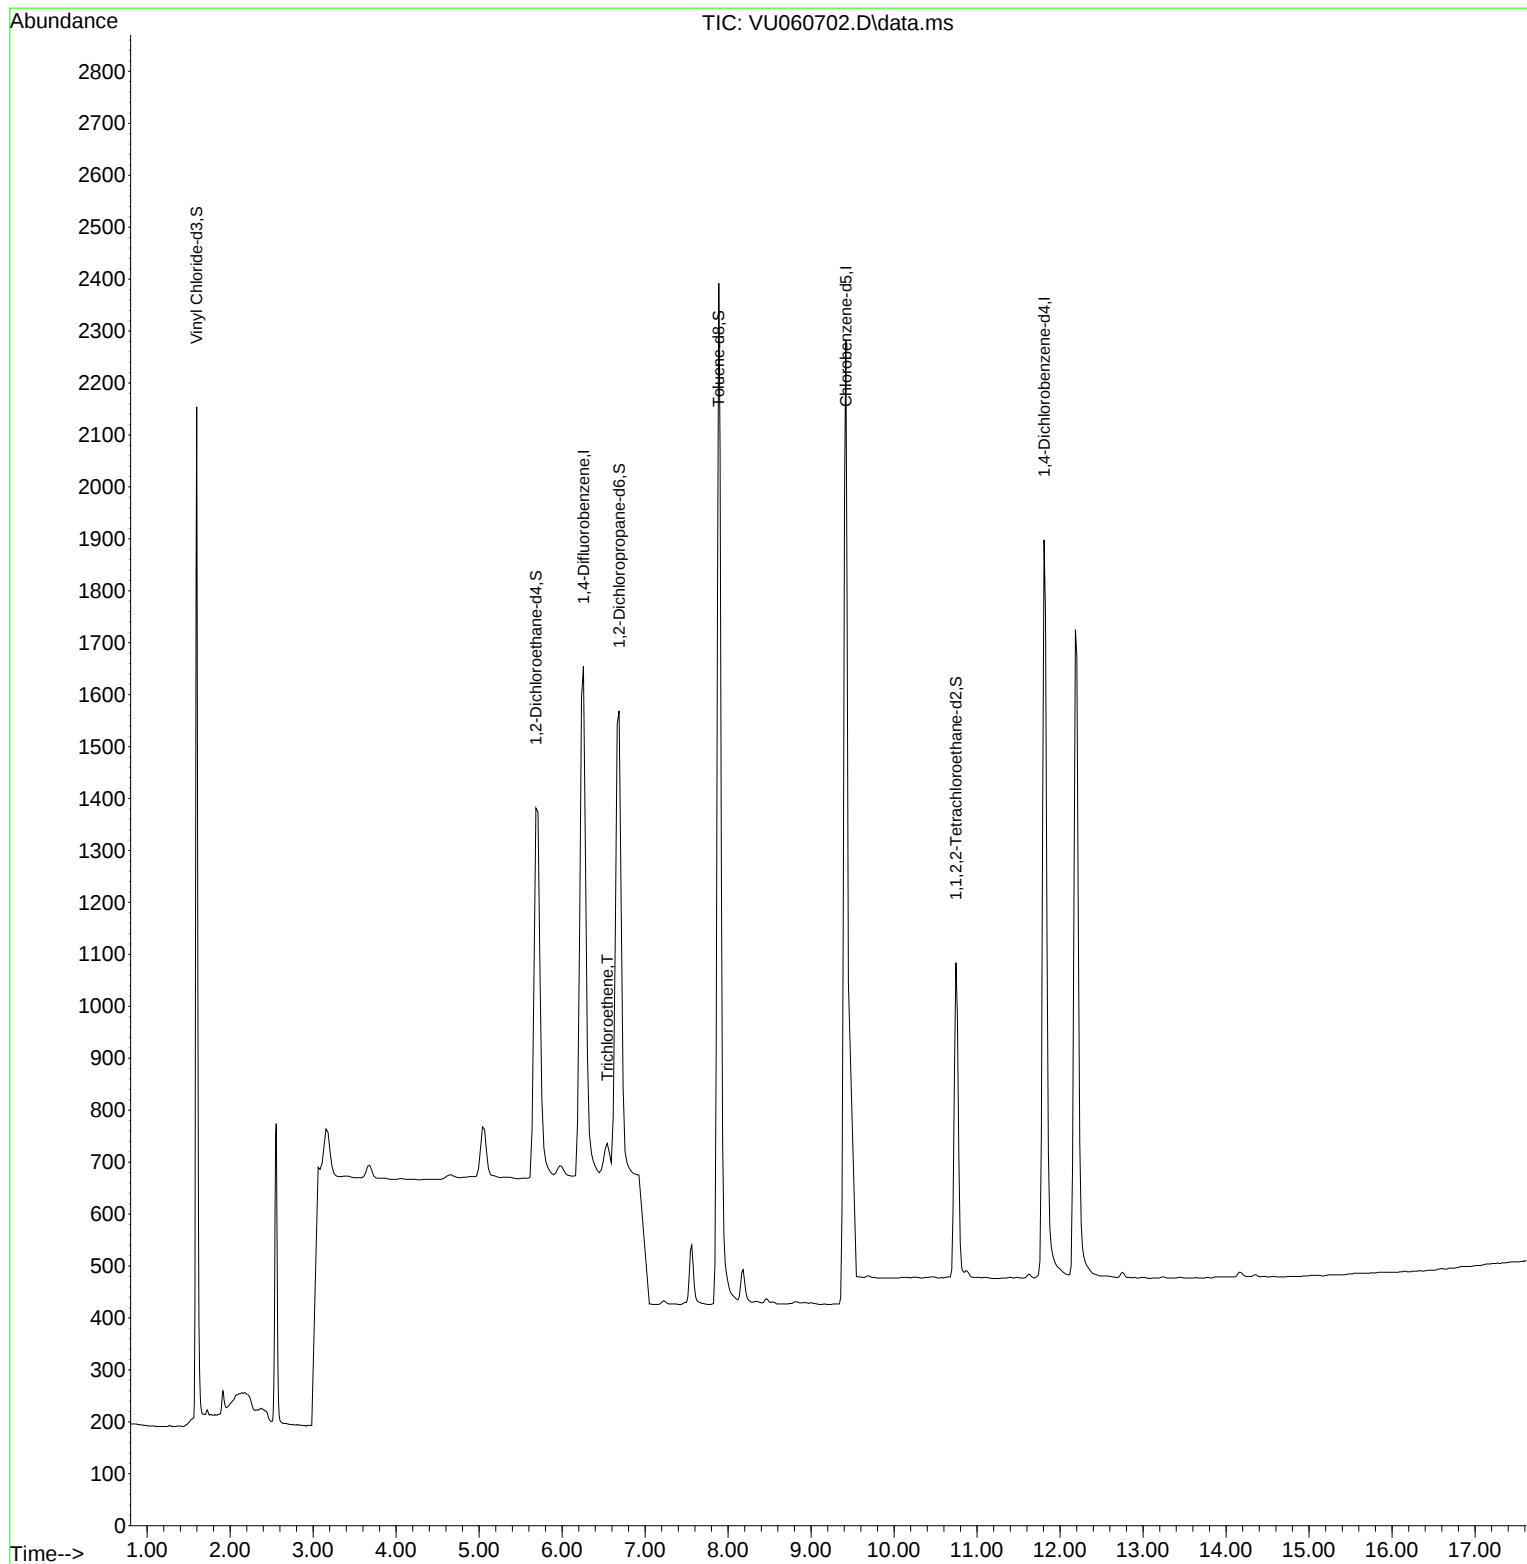

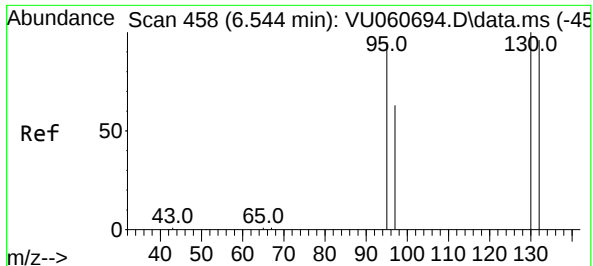

#6
 Trichloroethene
 Concen: 0.019 ug/L
 RT: 6.544 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: VU060702.D
 Acq: 11 Sep 2024 22:59

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AQ7

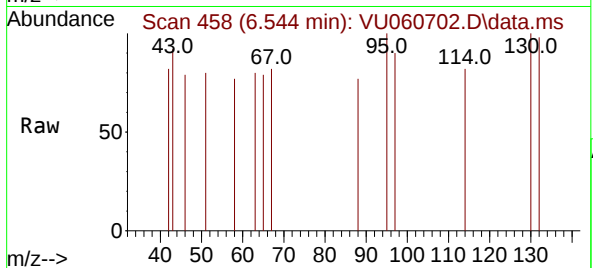

Tgt Ion: 95	Resp: 64
Ion Ratio	Lower Upper
95 100	
97 90.2	48.5 90.1#
132 98.4	75.5 140.1
130 100.0	76.3 141.7

