

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091124\
 Data File : VU060710.D
 Acq On : 12 Sep 2024 10:32
 Operator : MD/SY
 Sample : P3918-20DL 5X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AR2DL

Quant Time: Sep 13 05:22:18 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	4295	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.419	117	6450	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	1790	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	2856	0.409	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	82.000%
4) 1,2-Dichloroethane-d4	5.685	65	1744	0.471	ug/L	-0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	94.000%
7) 1,2-Dichloropropane-d6	6.687	67	1827	0.456	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	92.000%
8) Toluene-d8	7.887	98	4171	0.503	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	100.000%
10) 1,1,2,2-Tetrachloroeth...	10.745	84	1483	0.422	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	84.000%
Target Compounds						
6) Trichloroethene	6.544	95	3951	0.970	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091124\
Data File : VU060710.D
Acq On : 12 Sep 2024 10:32
Operator : MD/SY
Sample : P3918-20DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AR2DL


Quant Time: Sep 13 05:22:18 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration

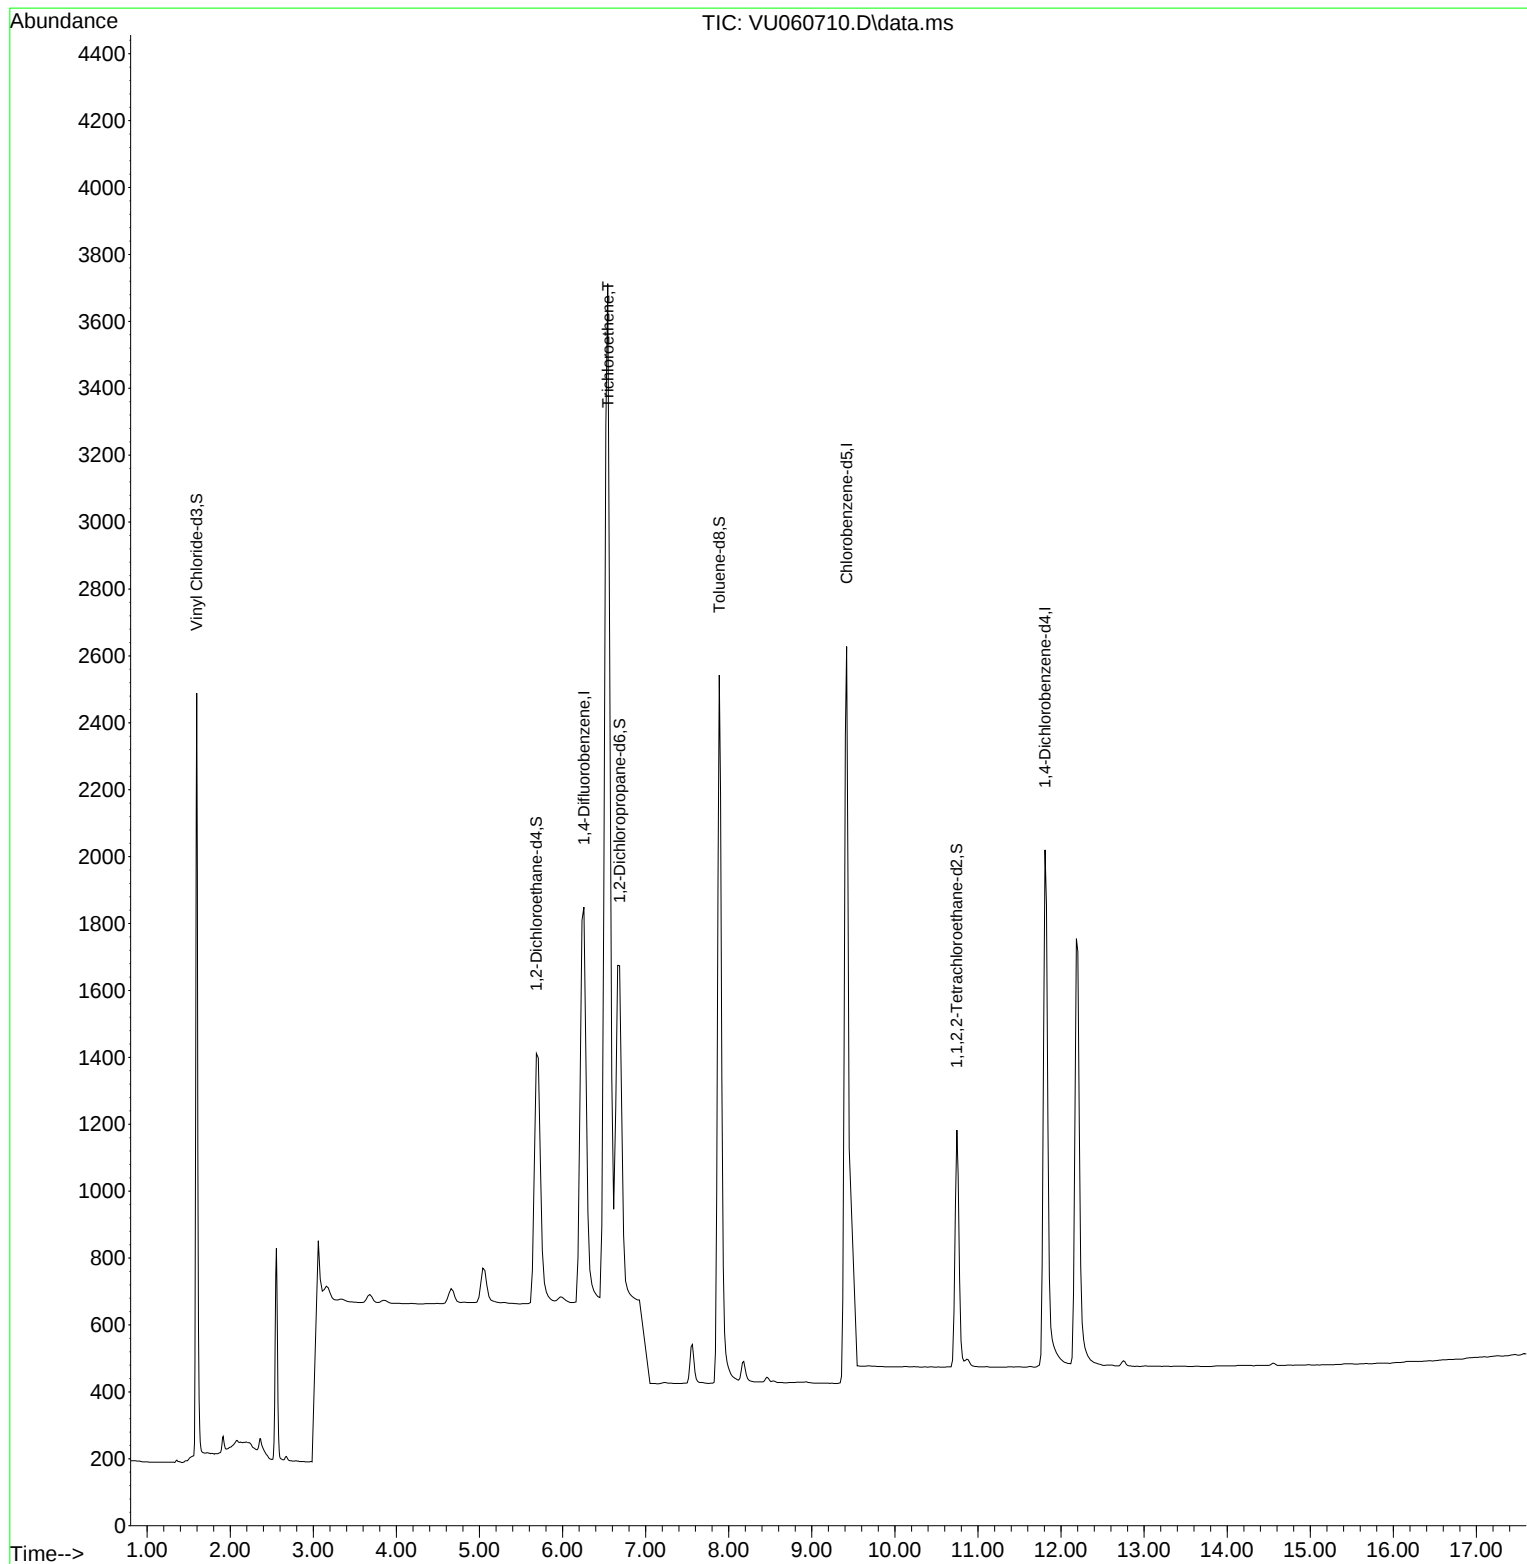

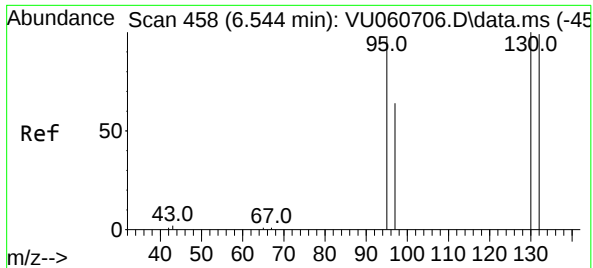

#6
 Trichloroethene
 Concen: 0.970 ug/L
 RT: 6.544 min Scan# 458
 Delta R.T. 0.000 min
 Lab File: VU060710.D
 Acq: 12 Sep 2024 10:32

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AR2DL

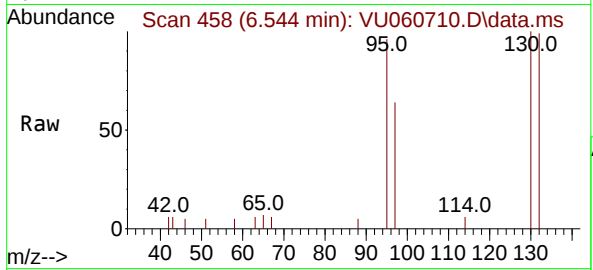

Tgt Ion: 95	Resp: 3951
Ion Ratio	Lower Upper
95 100	
97 67.1	48.5 90.1
132 103.2	75.5 140.1
130 104.4	76.3 141.7

