


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091124\
Data File : VU060675.D
Acq On : 11 Sep 2024 09:01
Operator : MD/SY
Sample : BFB015
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB015

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Title : TRACE VOA SOM01.0
Last Update : Sat Aug 17 05:03:57 2024

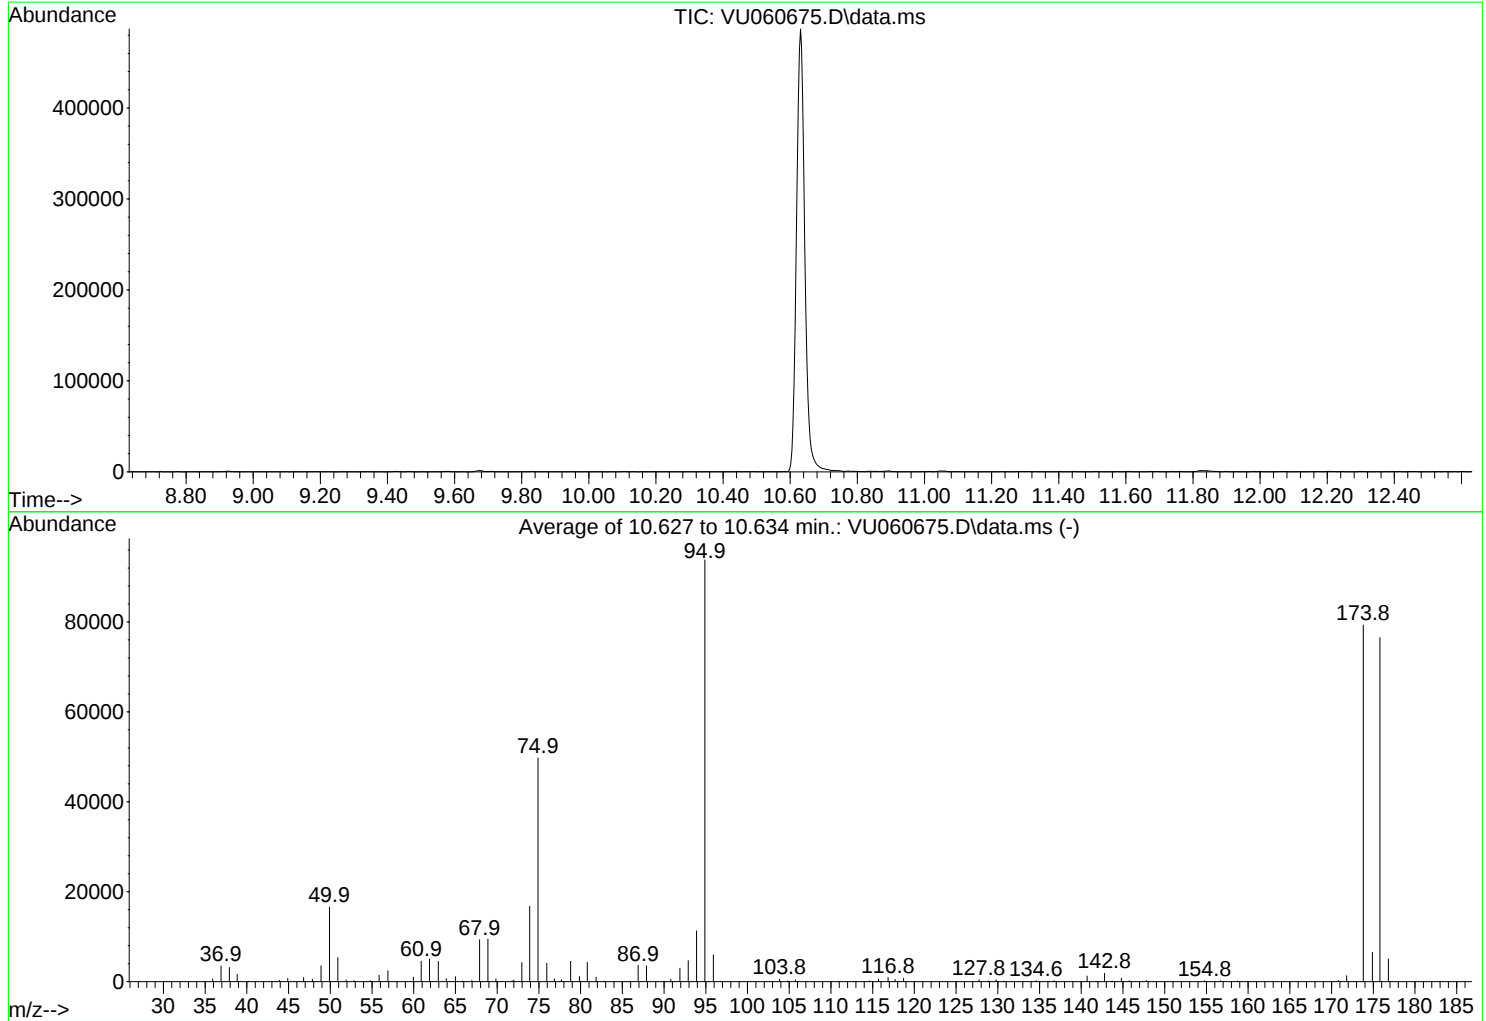

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.6	16539	PASS
75	95	30	80	53.0	49739	PASS
95	95	100	100	100.0	93811	PASS
96	95	5	9	6.3	5928	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.5	79307	PASS
175	174	5	9	8.2	6525	PASS
176	174	95	101	96.5	76523	PASS
177	176	5	9	6.6	5062	PASS

m/z	Abundance
43.90	238.0

Instrument :
MSVOA_U
ClientSampleId :
BFB015

m/z	Abundance
35.90	625.0
36.90	3489.0
37.90	2958.0
38.90	1737.0
43.90	543.0
44.90	723.0
46.80	861.0
47.80	515.0
48.90	3572.0
49.90	16373.0
50.90	5380.0
51.90	313.0
52.80	225.0
54.80	312.0
55.80	1384.0
56.90	2303.0
59.90	970.0
60.90	4557.0
61.90	5006.0
63.00	4378.0
63.90	744.0
65.00	1063.0
65.80	185.0
67.00	264.0
67.90	9326.0
68.90	9206.0
69.80	589.0
71.80	553.0
73.00	4219.0
73.90	16293.0
74.90	48400.0
76.00	4152.0
76.90	621.0
77.70	480.0
78.80	4592.0
79.80	1121.0
80.80	4154.0
81.80	1045.0
82.80	104.0
85.90	182.0
86.90	3541.0
87.90	3542.0
90.80	514.0
91.90	3111.0
92.90	4685.0
93.90	11220.0
94.90	91816.0
95.90	5793.0
96.80	177.0
103.80	521.0
104.90	149.0
105.80	415.0
114.60	120.0
115.70	610.0
116.80	907.0
117.70	502.0
118.70	715.0
127.70	430.0
128.90	170.0
129.80	388.0
134.60	167.0
136.60	172.0
136.80	175.0
140.70	1103.0
142.80	1865.0
143.70	158.0
144.80	903.0
145.70	162.0
147.80	227.0
149.80	118.0
154.80	235.0
156.70	159.0
158.80	174.0
170.80	294.0
171.80	1202.0
173.80	77576.0
174.90	6500.0
175.80	74536.0
176.80	5146.0

Instrument :
MSVOA_U
ClientSampleId :
BFB015

m/z	Abundance
35.90	639.0
36.90	3587.0
37.90	3214.0
38.80	1720.0
40.20	111.0
43.90	548.0
44.90	732.0
46.80	965.0
47.90	541.0
48.90	3646.0
49.90	17072.0
50.90	5529.0
51.90	406.0
52.80	239.0
54.80	281.0
55.90	1476.0
56.90	2528.0
60.00	1016.0
60.90	4722.0
61.90	5165.0
63.00	4704.0
63.90	707.0
65.00	1107.0
65.80	169.0
67.00	278.0
67.90	9534.0
68.90	9667.0
69.80	662.0
72.00	533.0
72.90	4408.0
73.90	17288.0
74.90	51176.0
75.90	4206.0
76.80	631.0
77.70	494.0
78.80	4618.0
79.90	1171.0
80.80	4485.0
81.90	1013.0
82.70	133.0
85.90	150.0
86.90	3760.0
87.90	3654.0
90.80	566.0
91.90	3061.0
92.90	4782.0
93.90	11519.0
94.90	96720.0
95.90	6098.0
97.00	117.0
103.80	537.0
104.80	182.0
105.70	392.0
107.90	120.0
112.70	133.0
114.60	149.0
115.70	587.0
116.80	918.0
117.70	520.0
118.70	763.0
127.80	425.0
128.80	206.0
129.80	411.0
130.70	121.0
134.60	233.0
136.70	197.0
140.70	1313.0
141.90	102.0
142.80	1903.0
143.70	166.0
144.80	791.0
145.80	230.0
147.80	276.0
154.80	220.0
156.70	222.0
158.70	156.0
160.70	106.0
170.80	295.0
171.80	1368.0
173.80	81504.0
174.90	6790.0
175.80	78752.0
176.80	5121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB015

m/z	Abundance
35.90	603.0
36.90	3370.0
37.90	3325.0
38.80	1491.0
40.20	102.0
43.90	460.0
44.90	685.0
46.80	901.0
47.90	523.0
48.90	3355.0
49.90	16172.0
50.90	5067.0
51.90	419.0
52.90	260.0
54.80	203.0
55.90	1403.0
56.90	2438.0
60.00	985.0
60.90	4409.0
61.90	4942.0
62.90	4343.0
63.90	583.0
65.00	1093.0
65.90	125.0
66.90	238.0
67.90	9134.0
68.90	9534.0
69.90	704.0
72.00	506.0
72.90	4131.0
73.90	16712.0
74.90	49640.0
75.90	3945.0
76.80	583.0
77.70	339.0
78.80	4407.0
79.90	1165.0
80.80	4305.0
81.90	933.0
82.70	131.0
86.90	3556.0
87.90	3269.0
90.80	512.0
91.90	2813.0
92.90	4566.0
93.90	11103.0
94.90	92896.0
95.90	5892.0
103.90	515.0
104.80	191.0
105.70	425.0
107.80	133.0
110.90	122.0
112.70	121.0
114.60	133.0
115.70	468.0
116.90	932.0
117.70	484.0
118.70	805.0
127.70	392.0
128.80	213.0
129.80	379.0
130.70	171.0
134.60	237.0
136.80	179.0
140.70	1379.0
141.90	119.0
142.80	1802.0
143.70	165.0
144.80	662.0
145.80	244.0
147.80	332.0
154.80	198.0
156.70	251.0
158.70	118.0
160.70	100.0
170.80	288.0
171.80	1336.0
173.80	78840.0
174.90	6284.0
175.80	76280.0
176.80	4918.0

Instrument :
MSVOA_U
ClientSampleId :
BFB015