



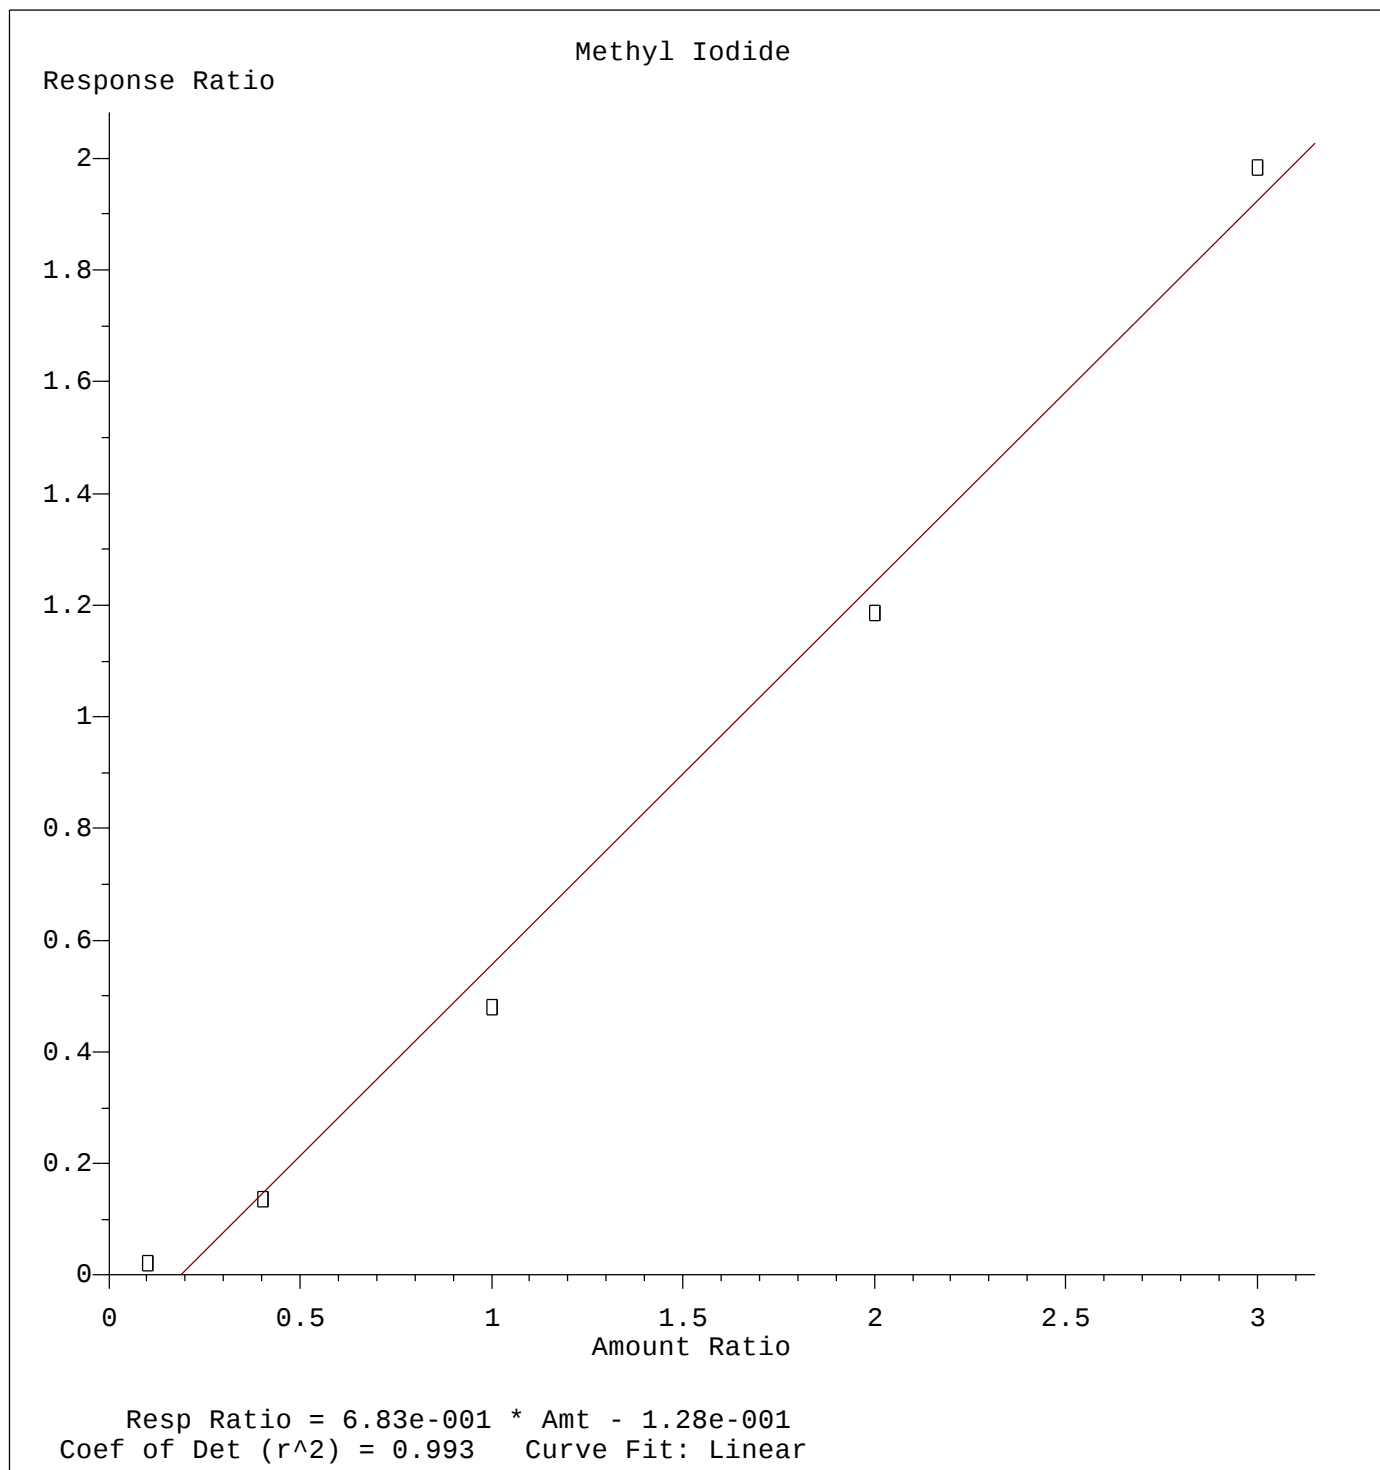

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U091218W.M
Calibration Table Last Updated: Thu Sep 13 17:11:41 2018


Naphthalene

Response Ratio

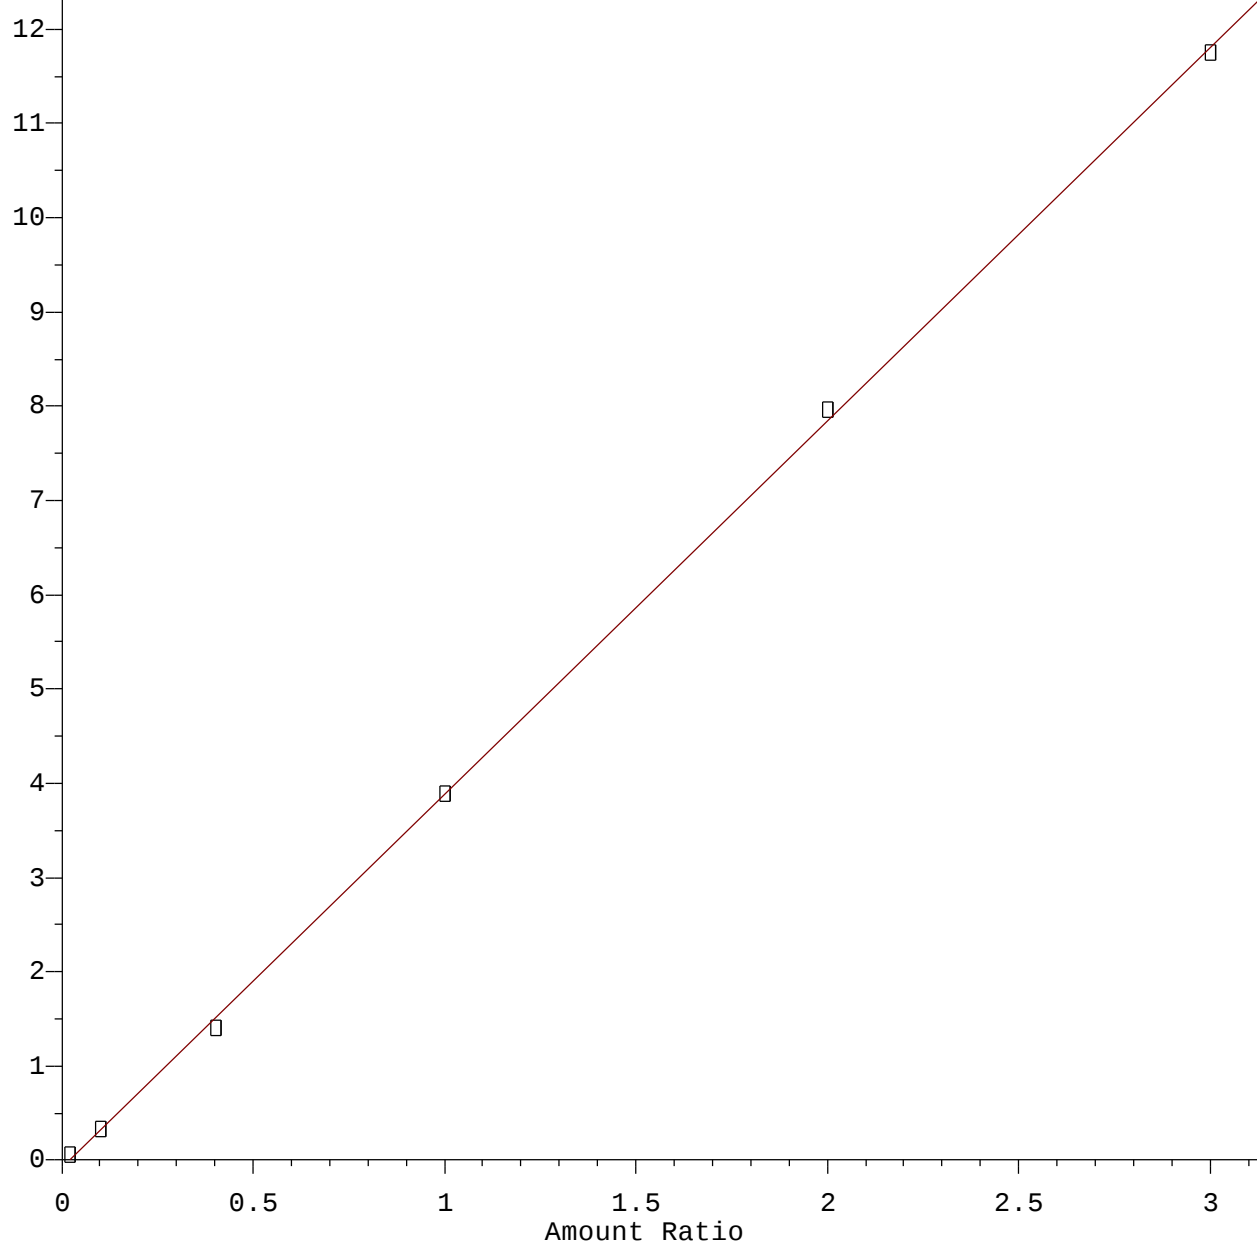

Resp Ratio = 3.96e+000 * Amt - 8.05e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U091218W.M
Calibration Table Last Updated: Thu Sep 13 17:11:41 2018

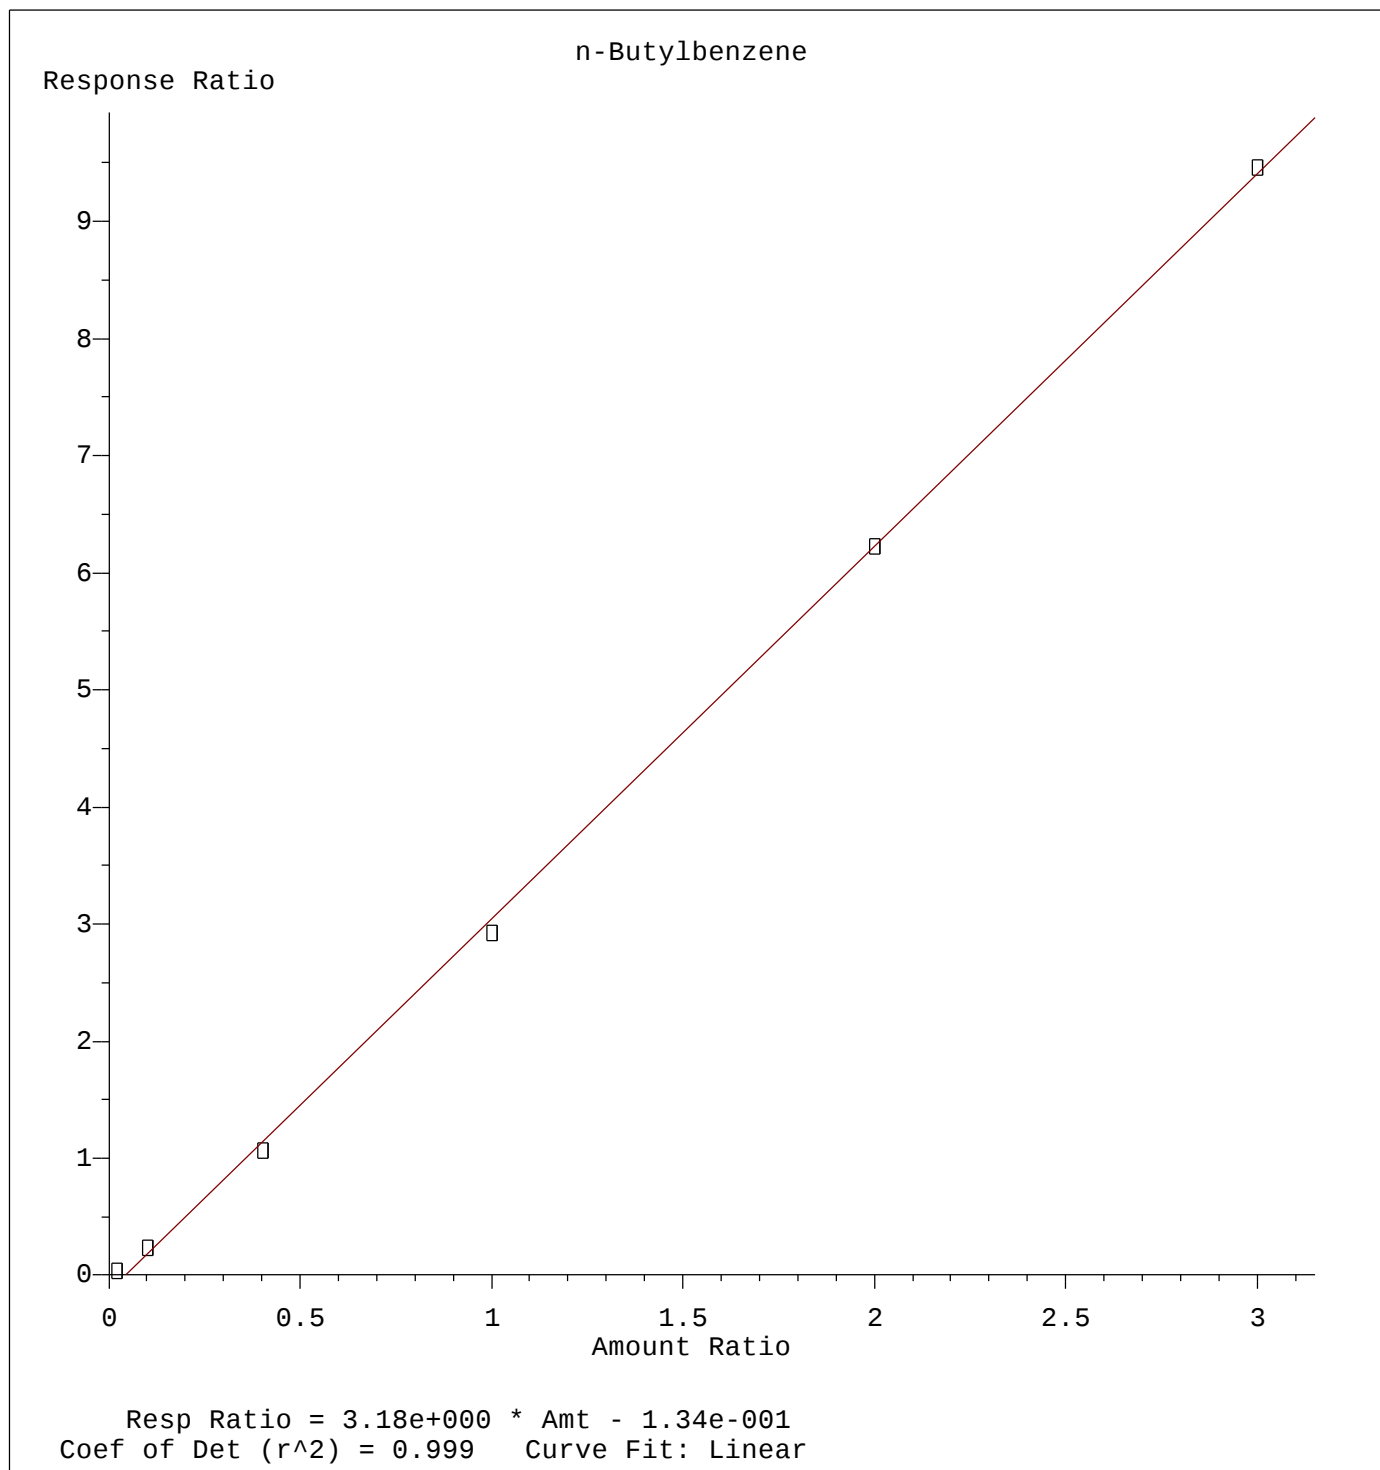

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U091218W.M
Calibration Table Last Updated: Thu Sep 13 17:11:41 2018


p-Isopropyltoluene

Response Ratio

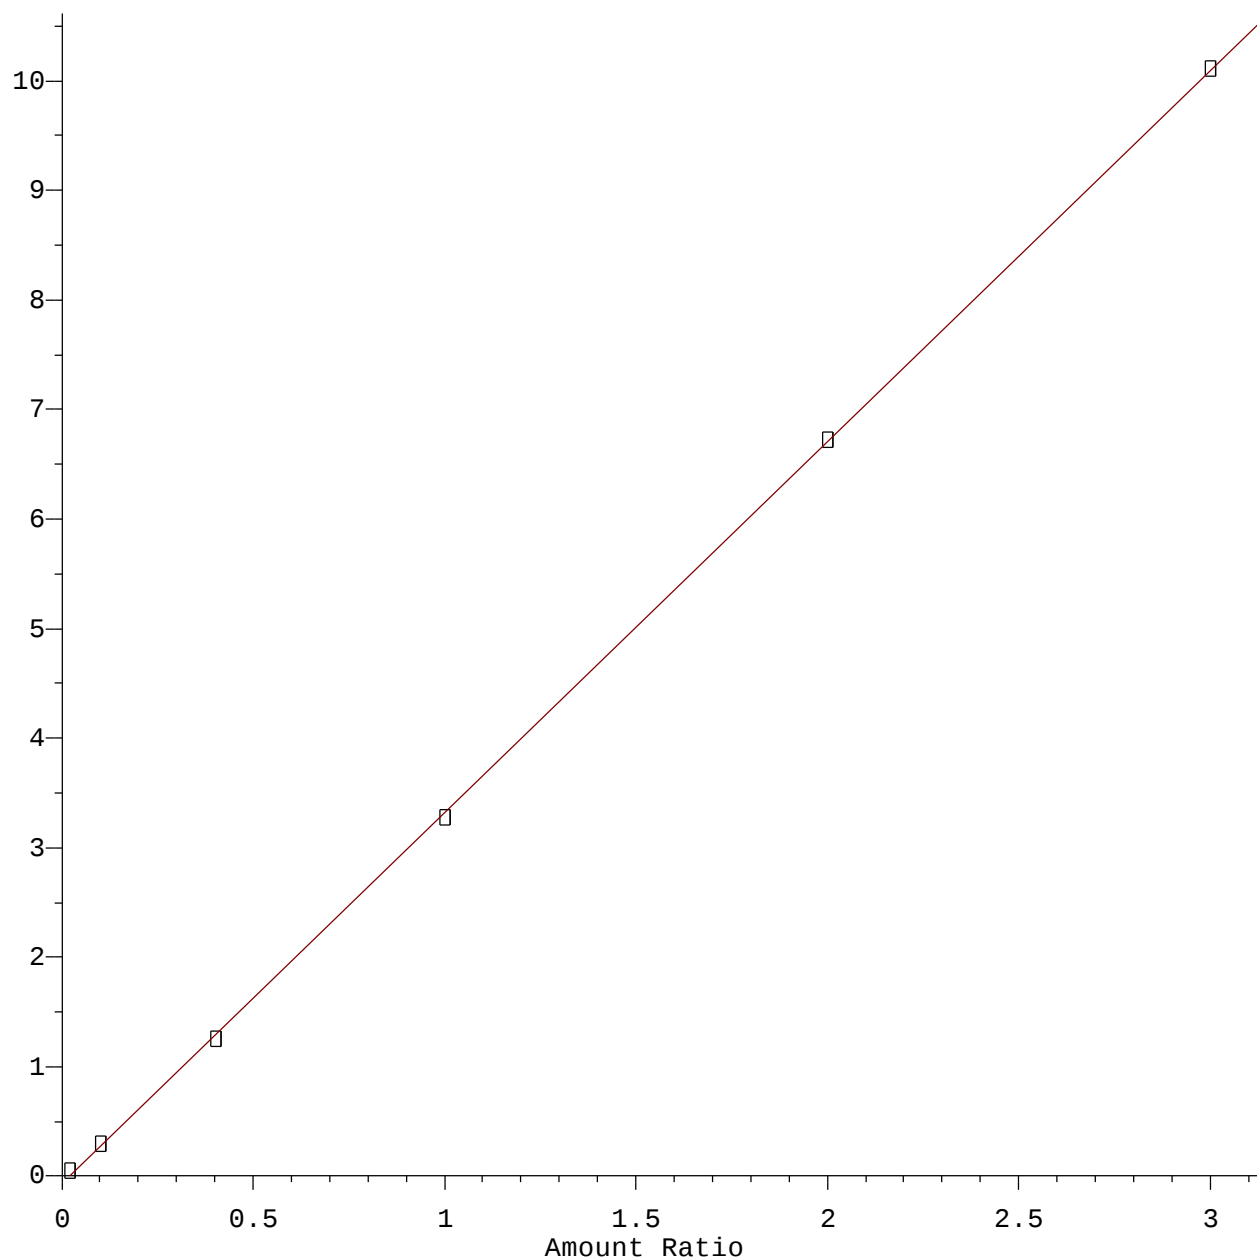


Resp Ratio = 3.39e+000 * Amt - 7.10e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U091218W.M
Calibration Table Last Updated: Thu Sep 13 17:11:41 2018

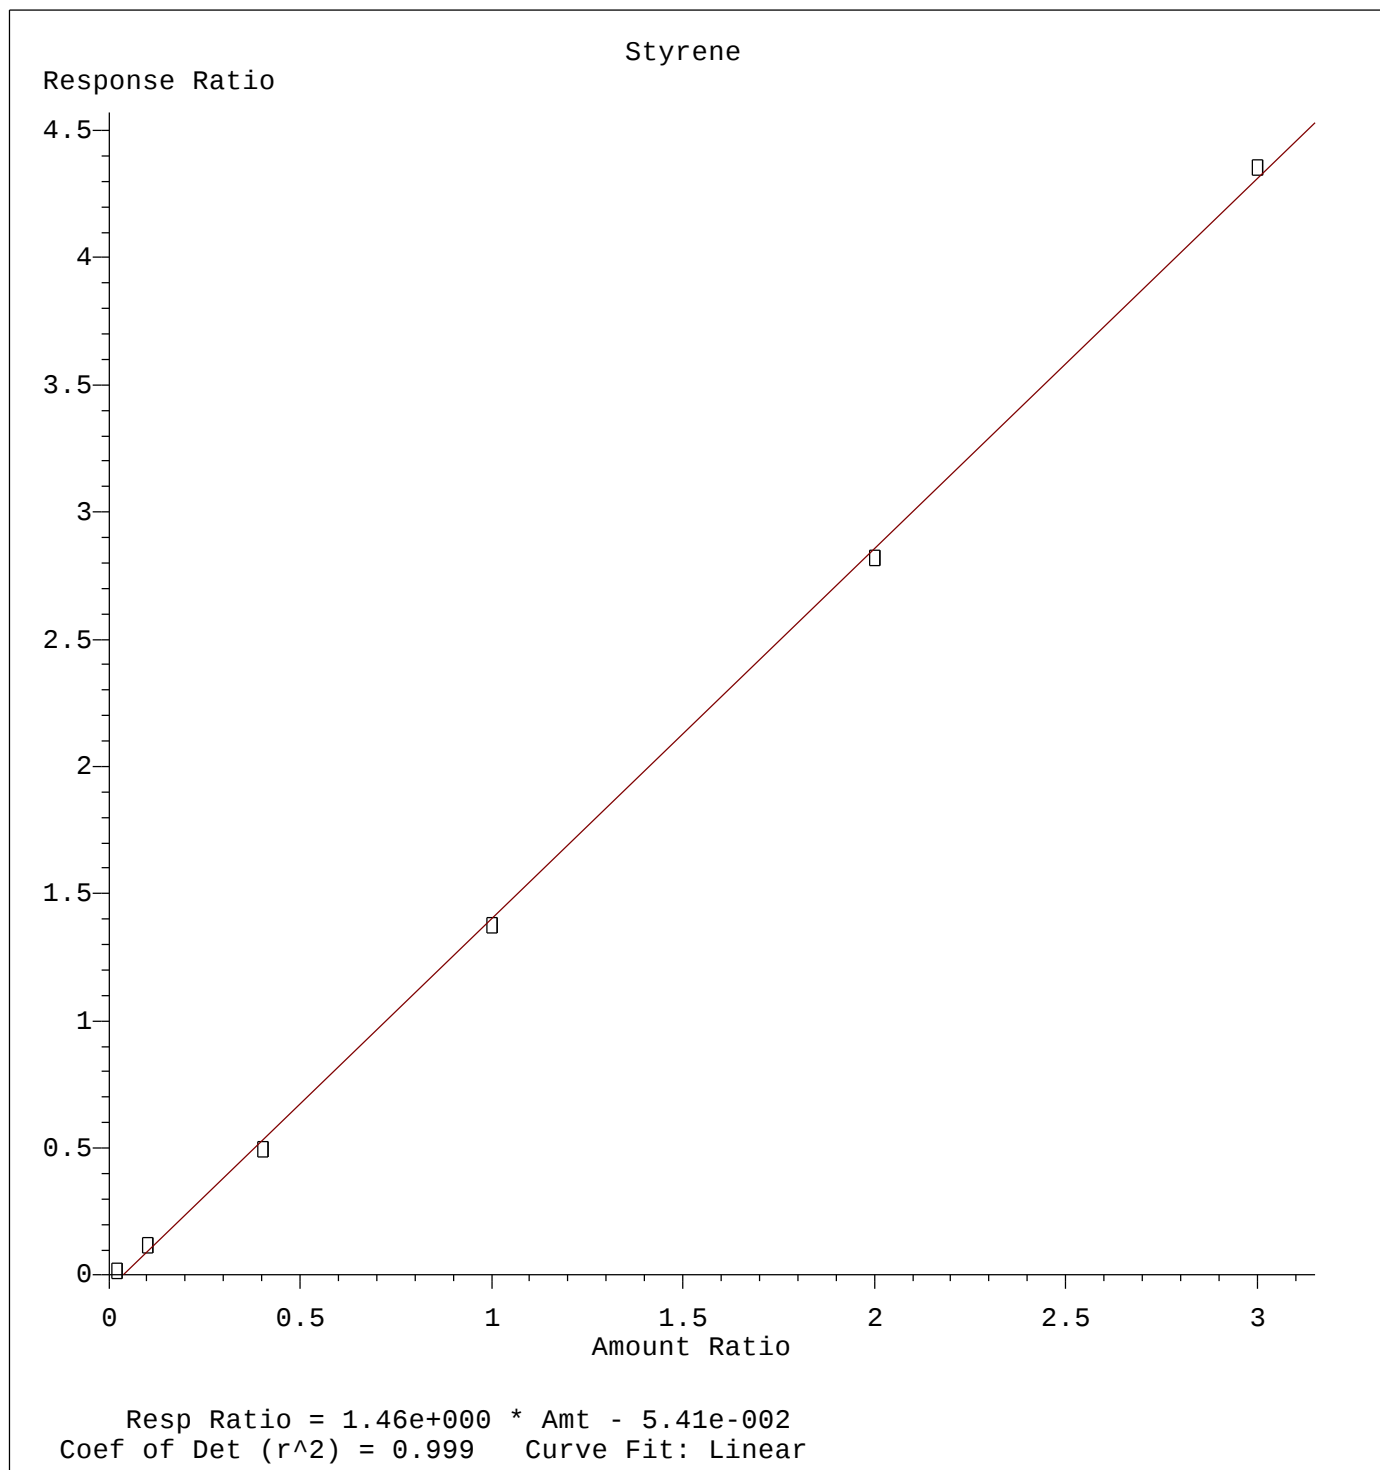


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U091218W.M
Calibration Table Last Updated: Thu Sep 13 17:11:41 2018

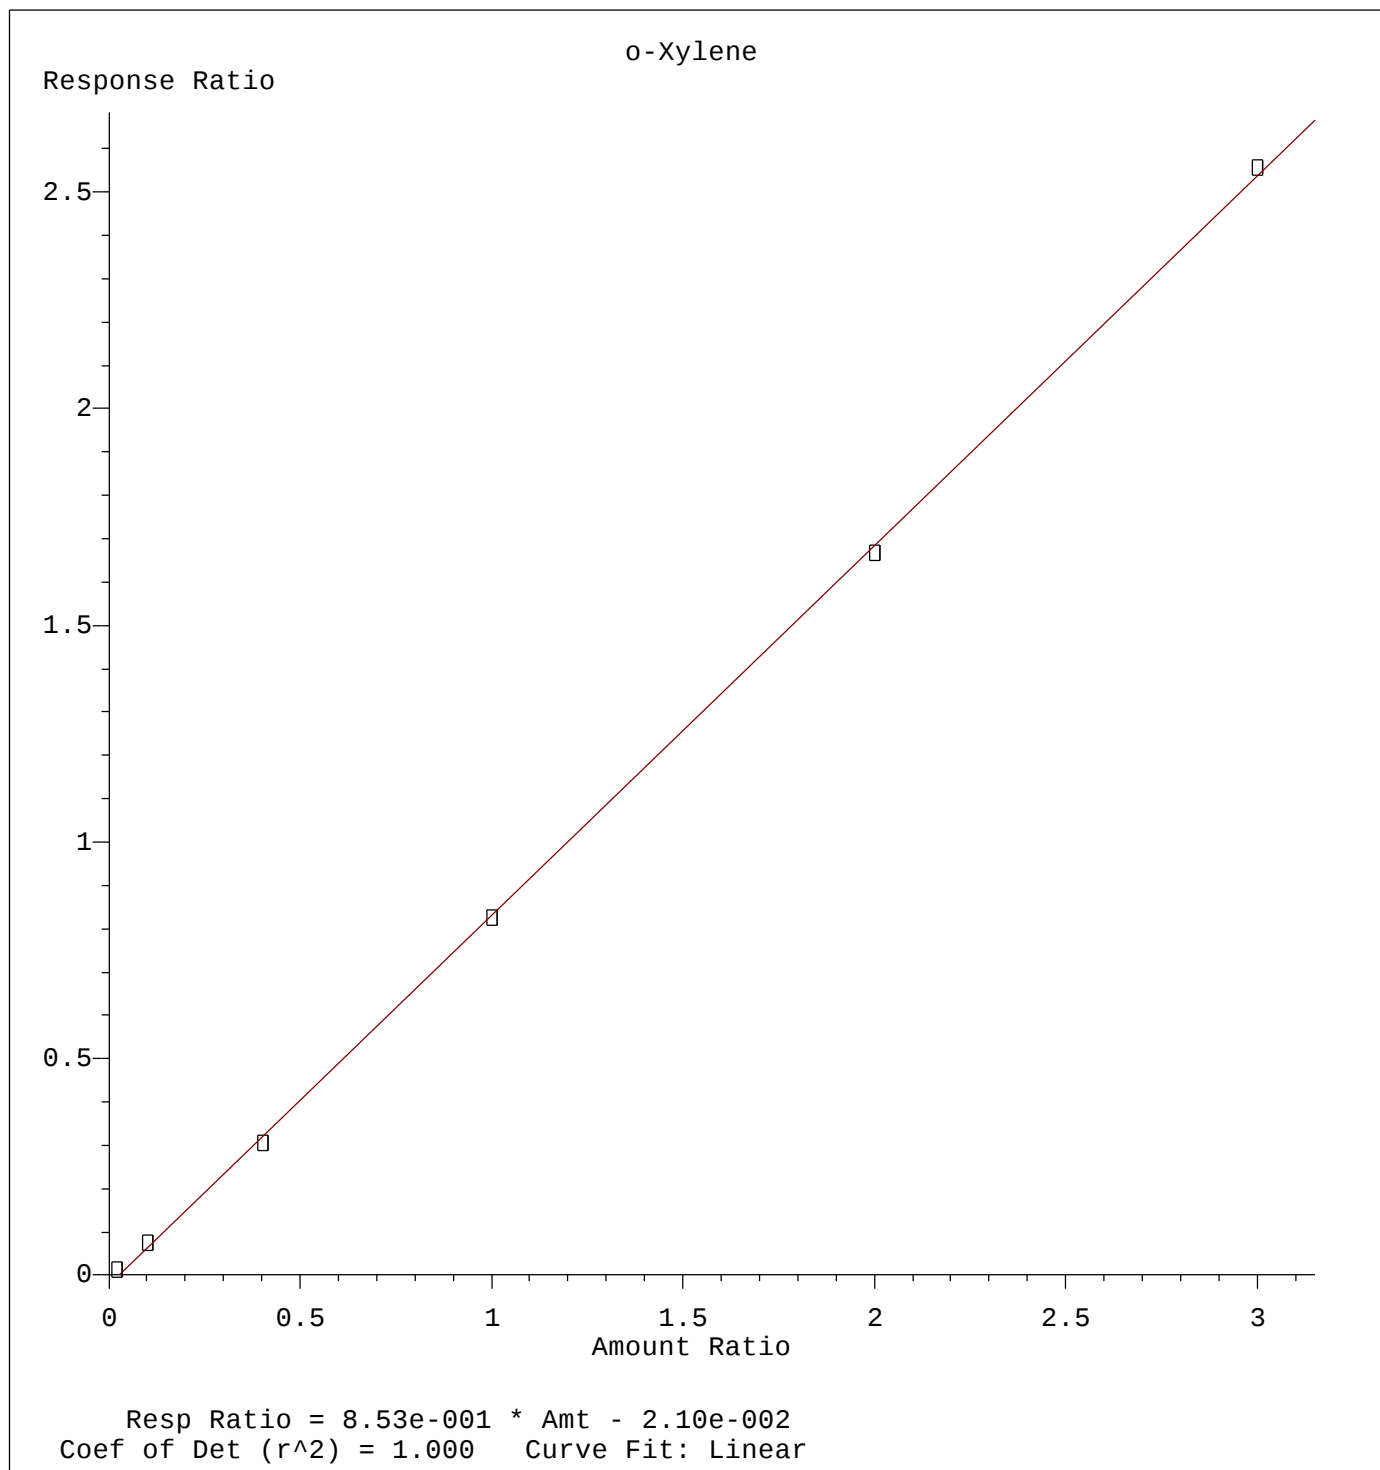

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U091218W.M
Calibration Table Last Updated: Thu Sep 13 17:11:41 2018

2-Chloroethyl Vinyl ether

Response Ratio

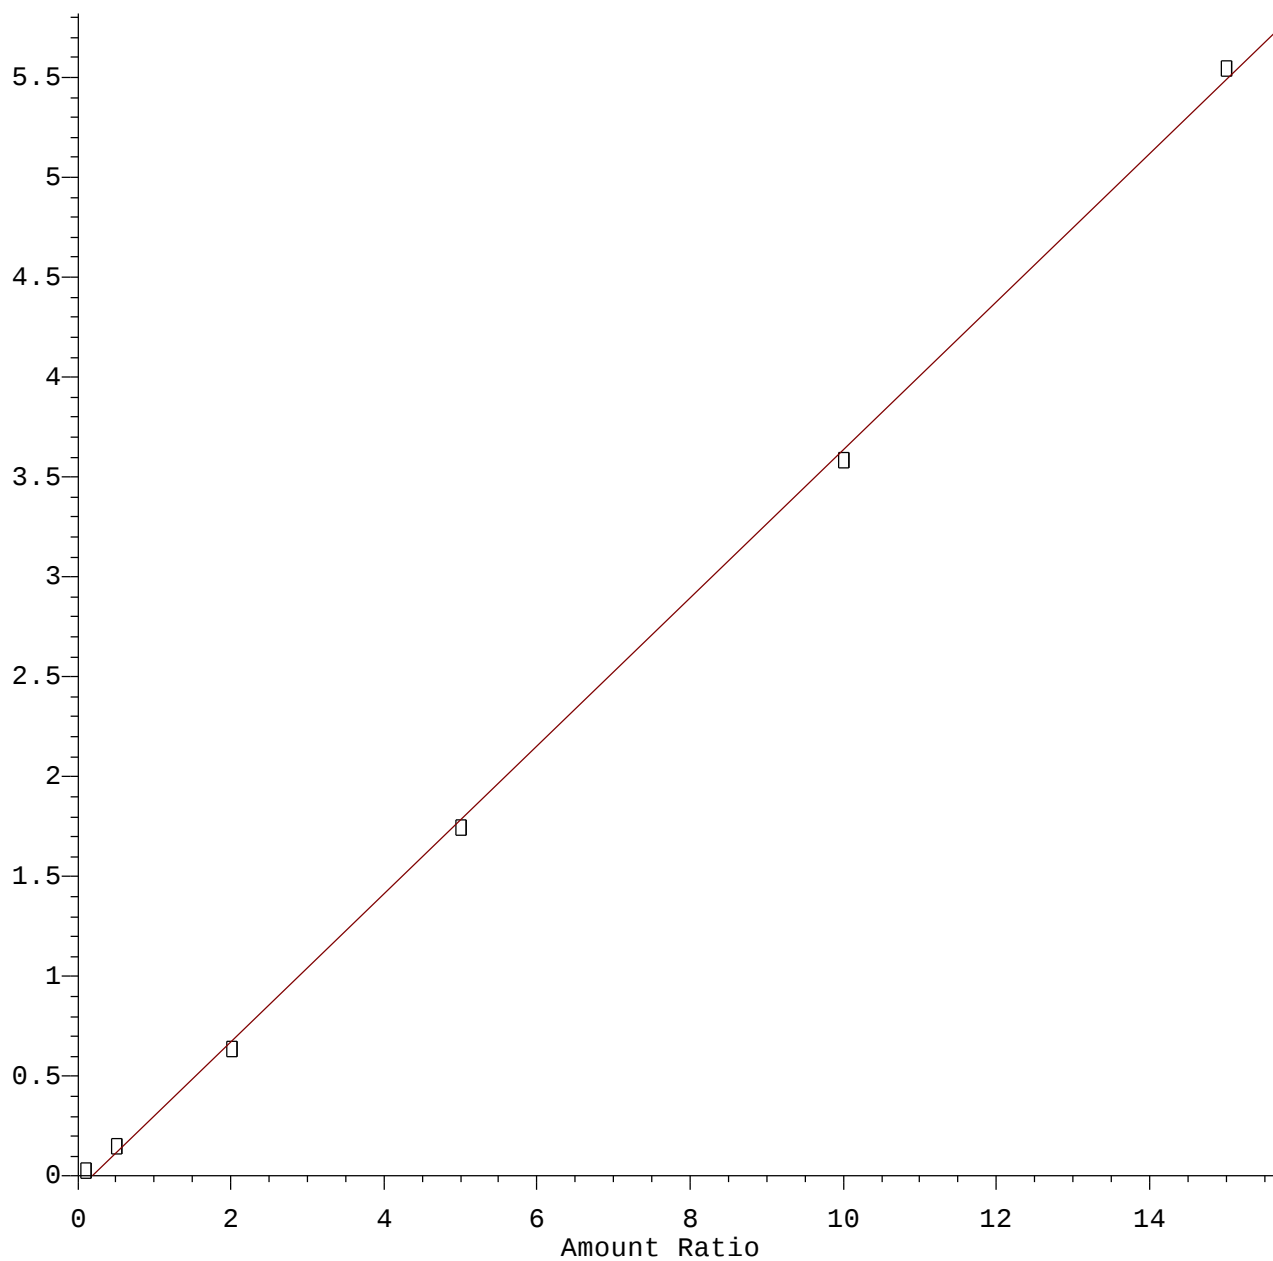


Resp Ratio = $3.70 \times 10^{-1} \times \text{Amt} - 6.60 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U091218W.M
Calibration Table Last Updated: Thu Sep 13 17:11:41 2018


Ethyl methacrylate

Response Ratio

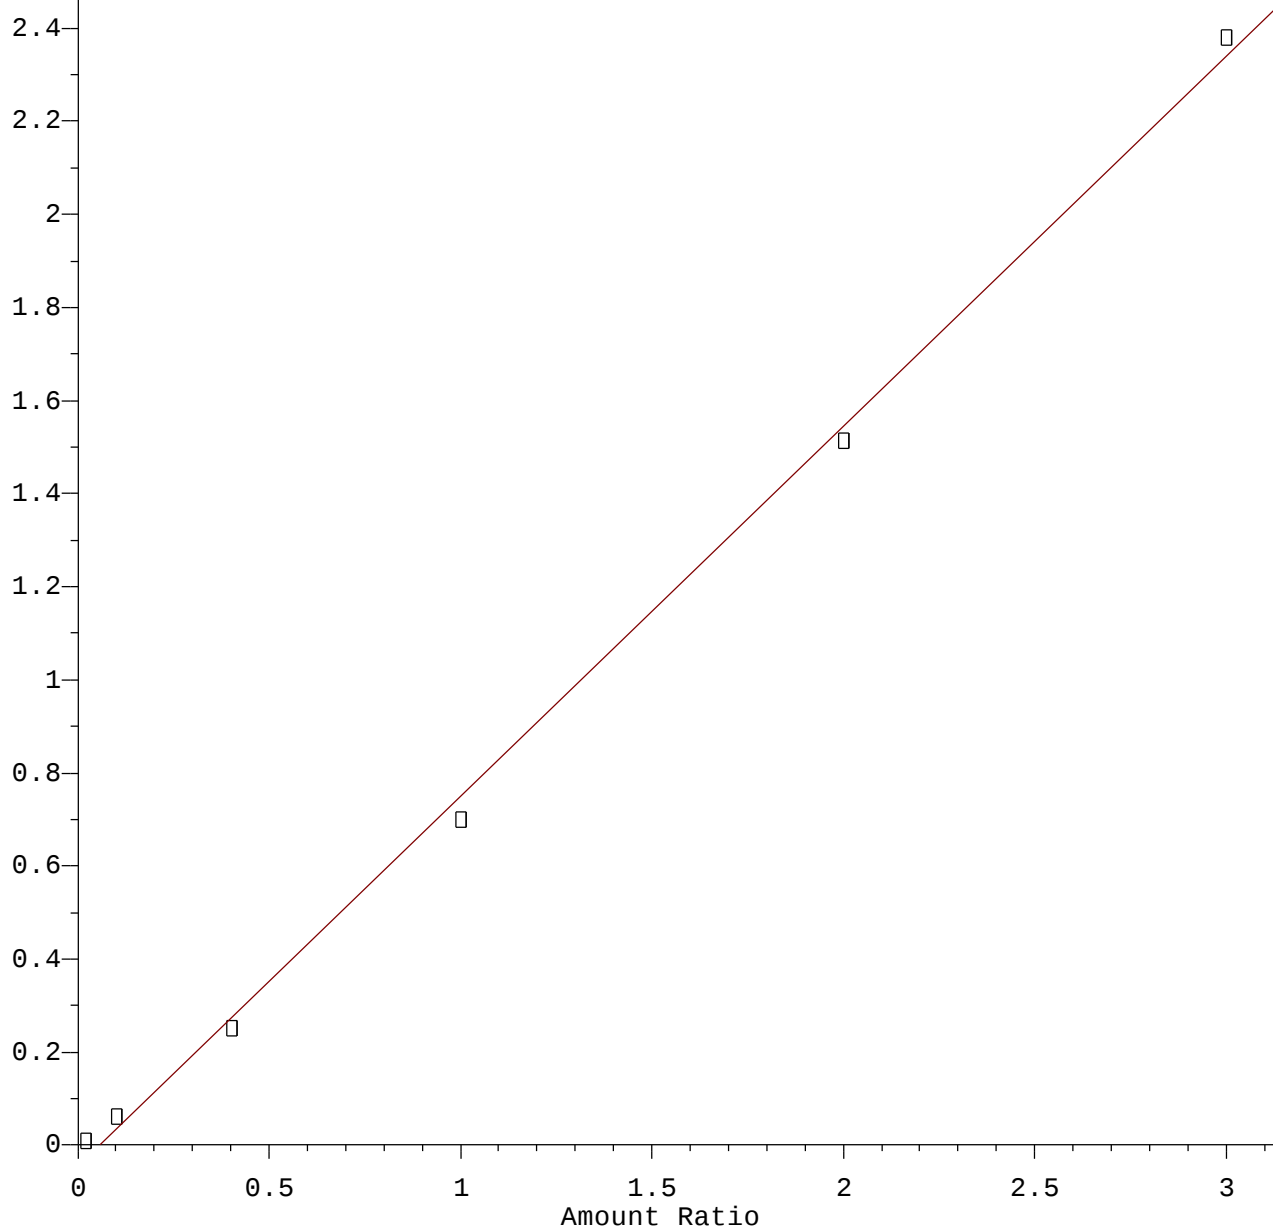


Resp Ratio = $7.95 \times 10^{-1} \times \text{Amt} - 4.53 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U091218W.M
Calibration Table Last Updated: Thu Sep 13 17:11:41 2018

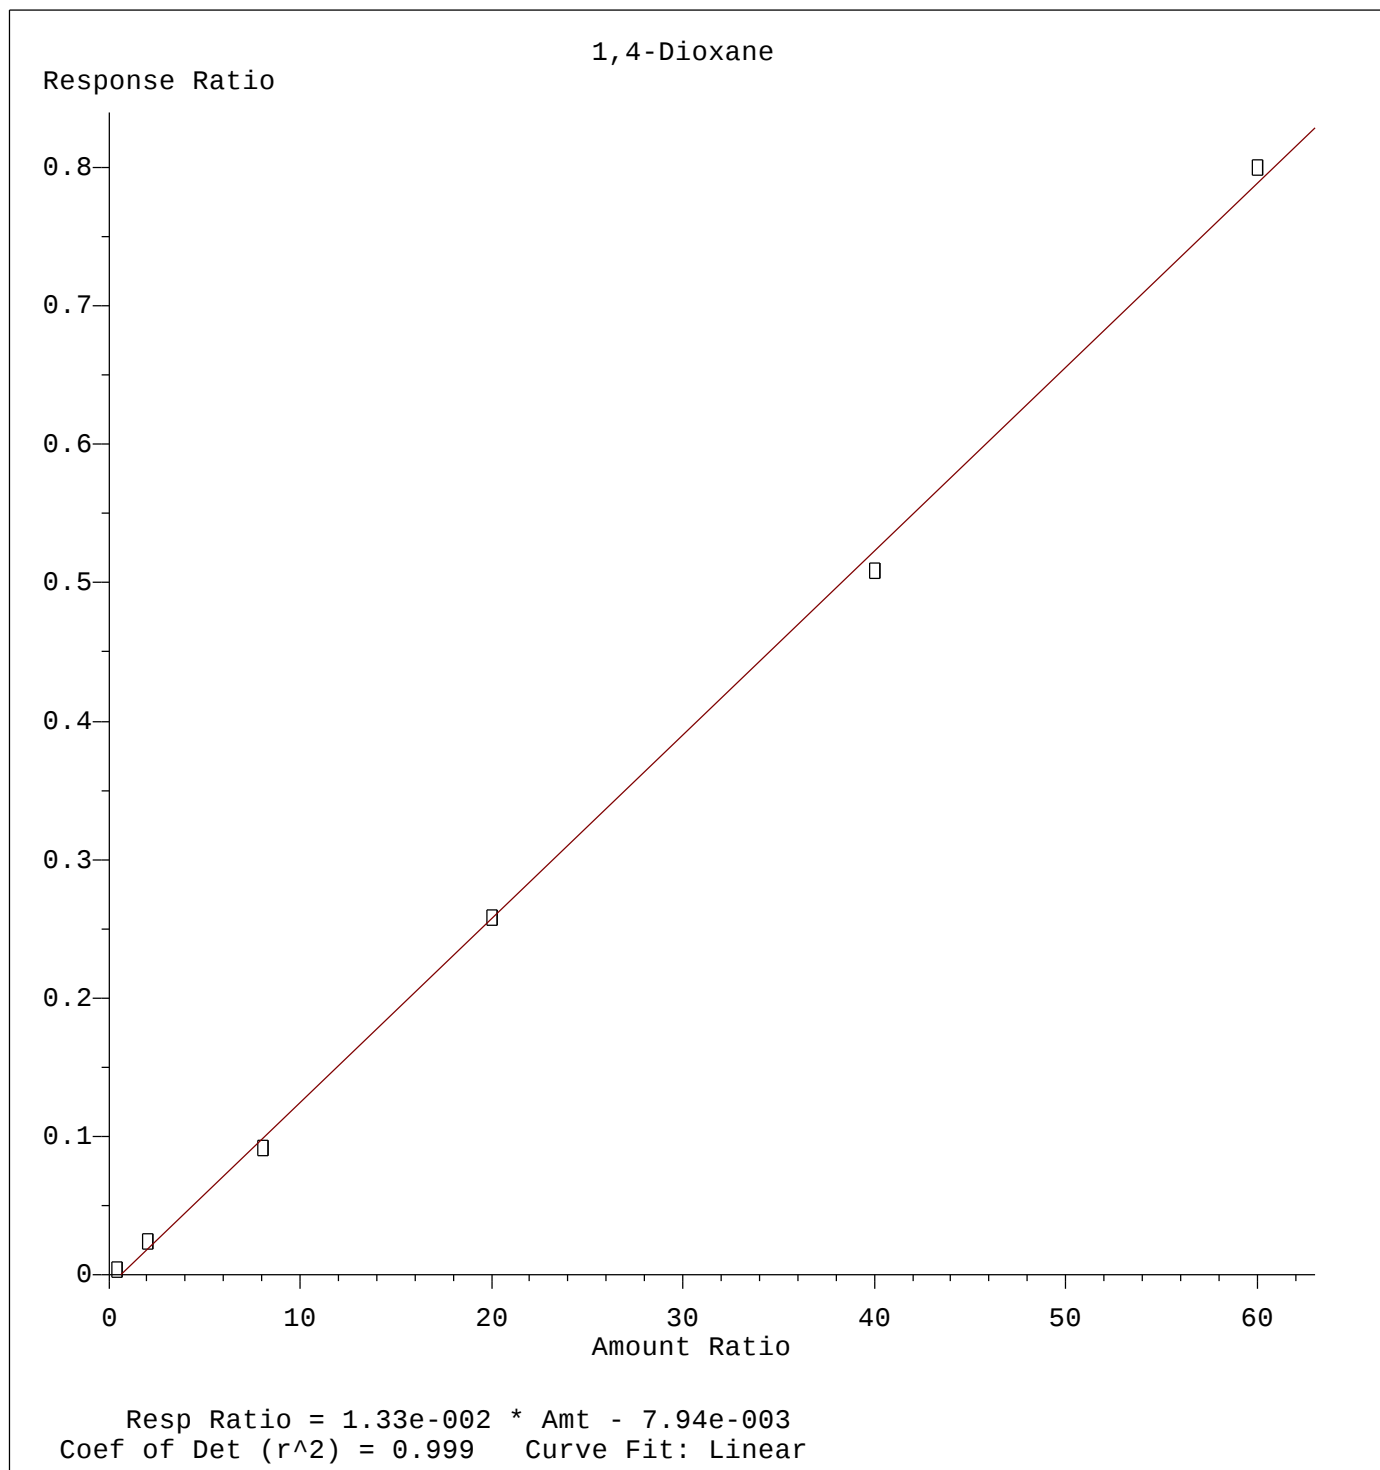


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U091218W.M
Calibration Table Last Updated: Thu Sep 13 17:11:41 2018

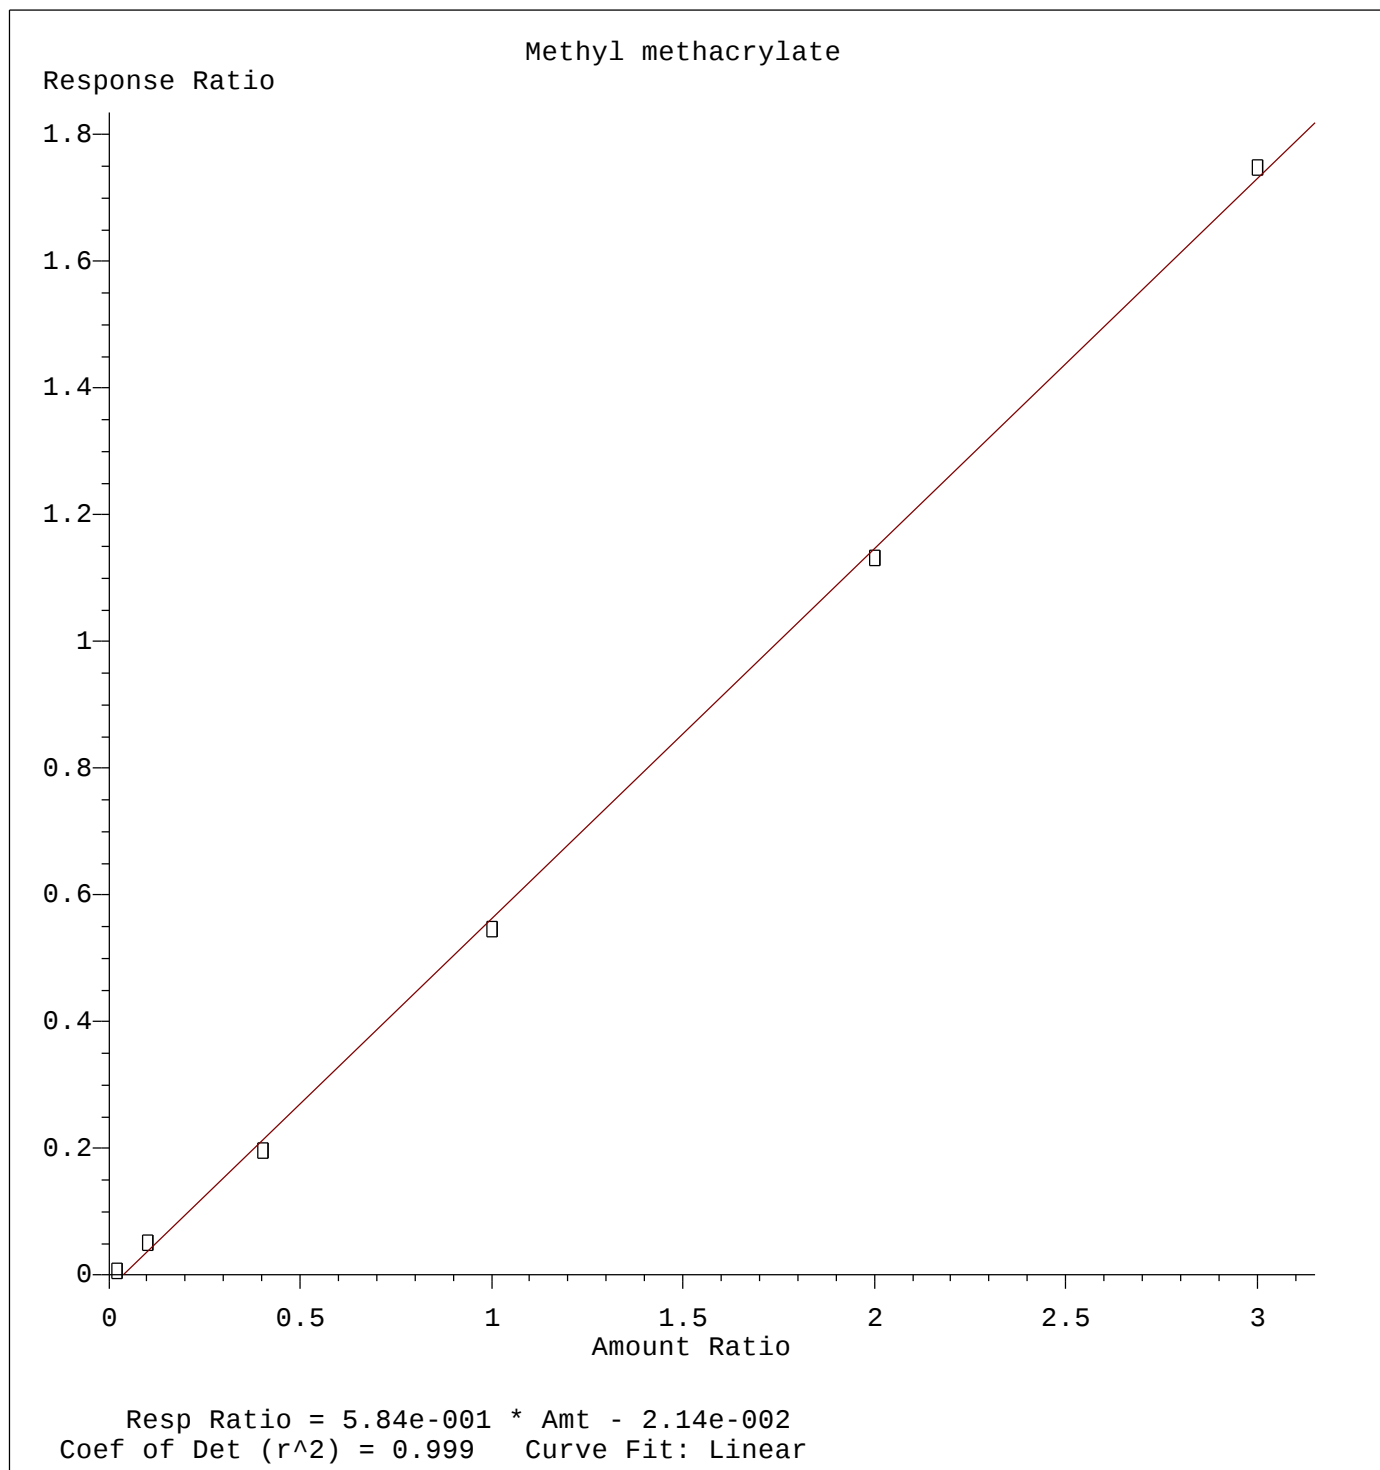

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U091218W.M
Calibration Table Last Updated: Thu Sep 13 17:11:41 2018


Methacrylonitrile

Response Ratio

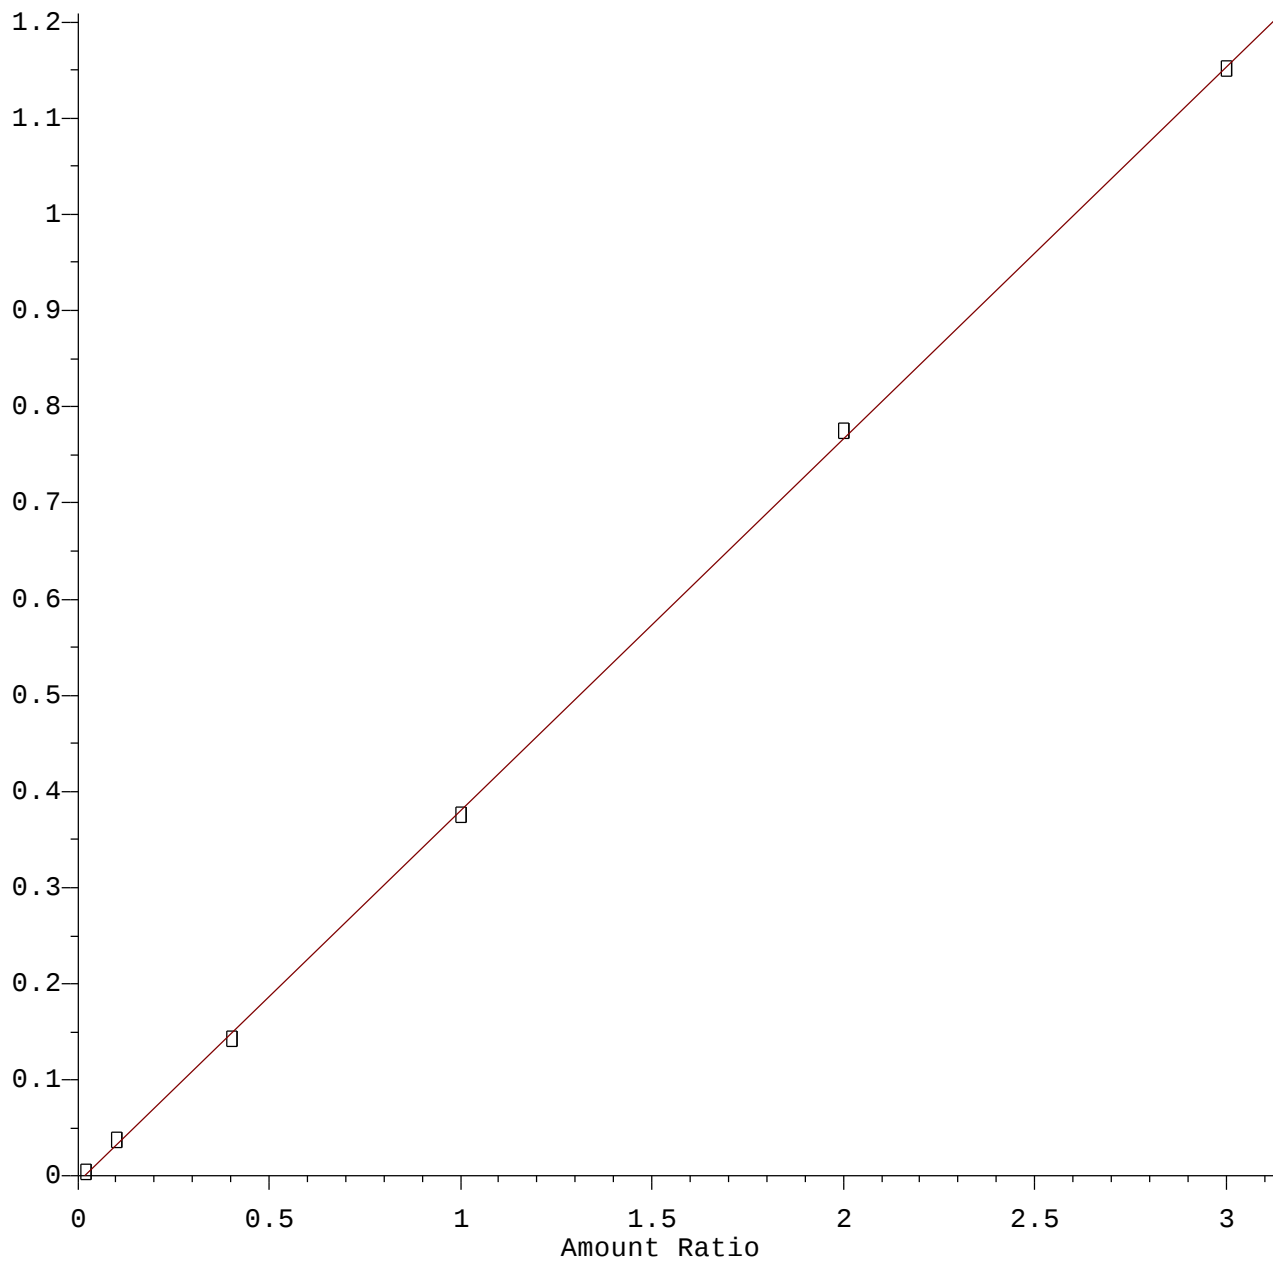

Resp Ratio = $3.86 \times 10^{-1} \times \text{Amt} - 5.76 \times 10^{-3}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U091218W.M
Calibration Table Last Updated: Thu Sep 13 17:11:41 2018

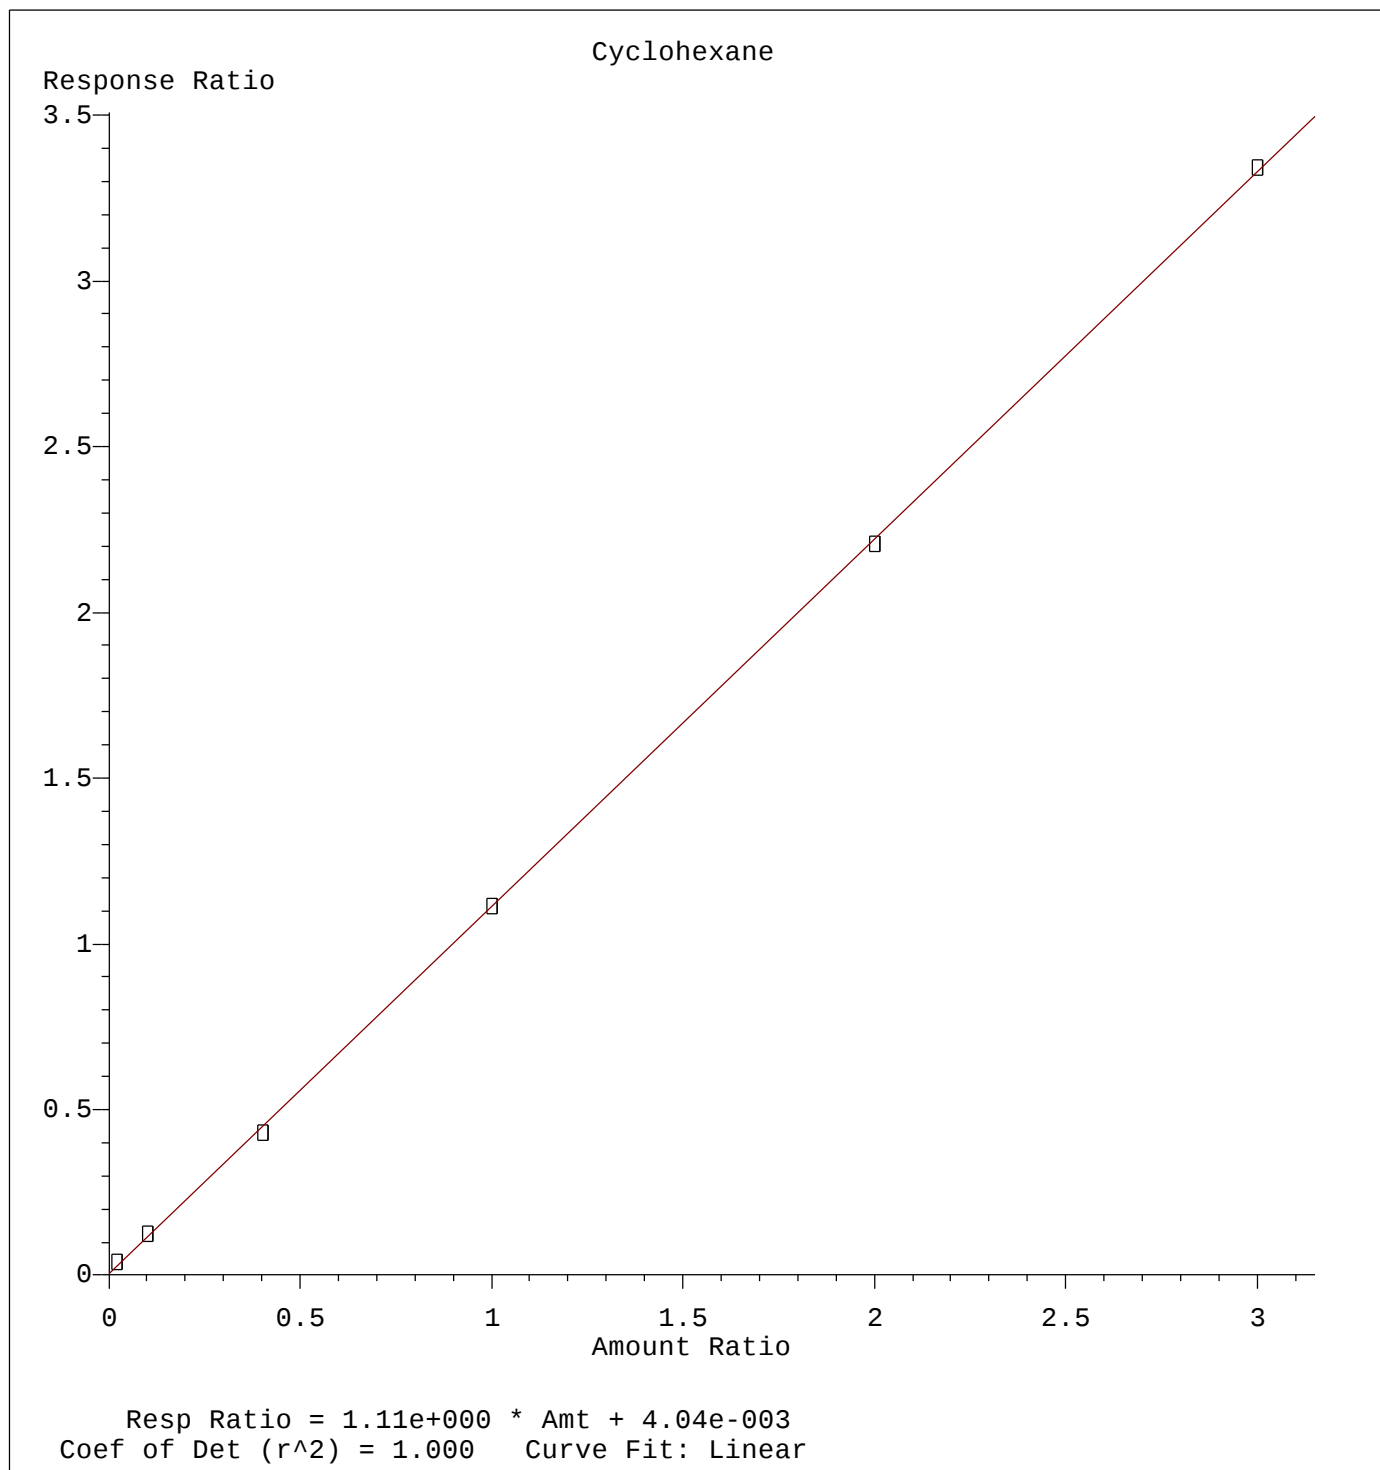

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U091218W.M
Calibration Table Last Updated: Thu Sep 13 17:11:41 2018